

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112619\
 Data File : FB023096.D
 Signal(s) : FID2B.CH
 Acq On : 26 Nov 2019 11:33
 Operator : DD/AJ
 Sample : VBF1126S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Nov 26 14:17:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.795	536768	21.852 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.700	2812	0.086 ng/ml
2) t	2,2,4-Trimethylpentane	7.400	4093	0.117 ng/ml
3) t	n-Heptane	7.760	1063	0.031 ng/ml
4) t	Benzene	7.906	3486	0.084 ng/ml
6) t	Toluene	10.627	10822	0.269 ng/ml
7) t	Ethylbenzene	13.076	5217	0.135 ng/ml
8) t	m-Xylene	13.201	7477	0.205 ng/ml
9) t	O-Xylene	13.925	9106	0.262 ng/ml
10) t	1,2,4-Trimethylbenzene	16.213	7030	0.251 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112619\
Data File : FB023096.D
Signal(s) : FID2B.CH
Acq On : 26 Nov 2019 11:33
Operator : DD/AJ
Sample : VBF1126S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Nov 26 14:17:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

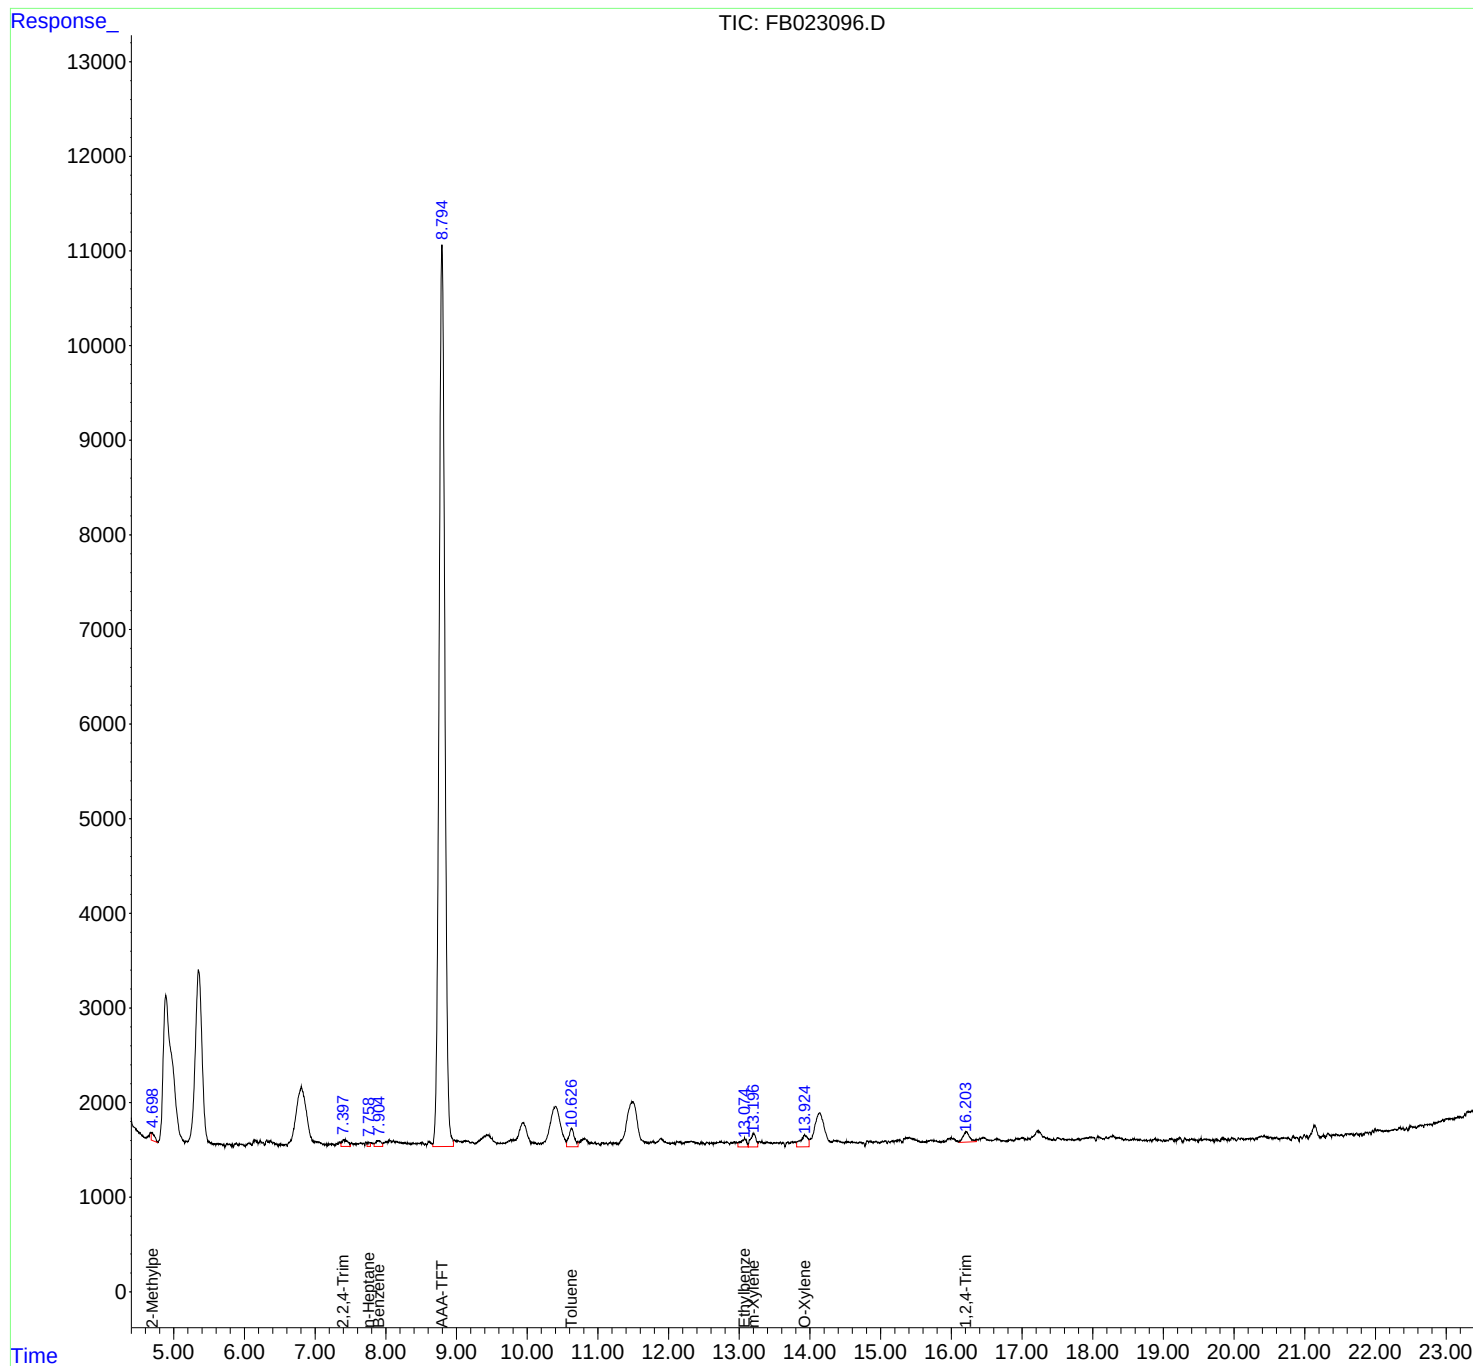

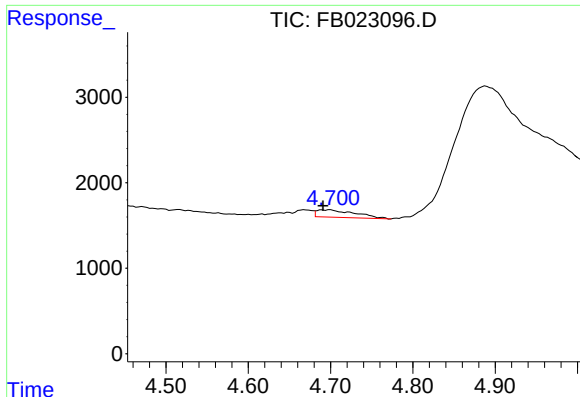


#1 2-Methylpentane

R.T.: 4.700 min
Delta R.T.: 0.009 min
Response: 2812
Conc: 0.09 ng/ml

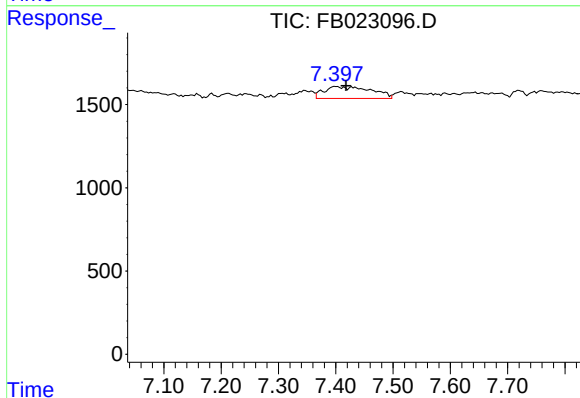


#2 2,2,4-Trimethylpentane

R.T.: 7.400 min
Delta R.T.: -0.018 min
Response: 4093
Conc: 0.12 ng/ml

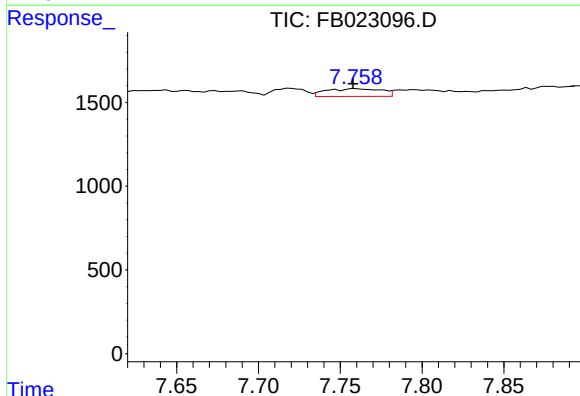


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.002 min
Response: 1063
Conc: 0.03 ng/ml

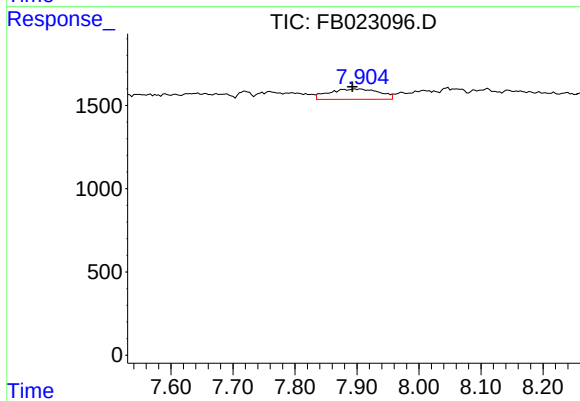


#4 Benzene

R.T.: 7.906 min
Delta R.T.: 0.014 min
Response: 3486
Conc: 0.08 ng/ml

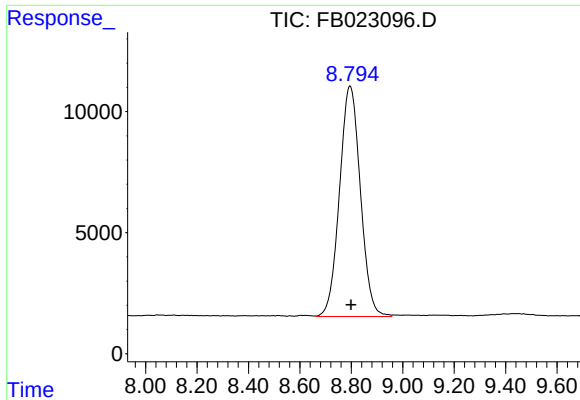


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 536768
Conc: 21.85 ng/ml

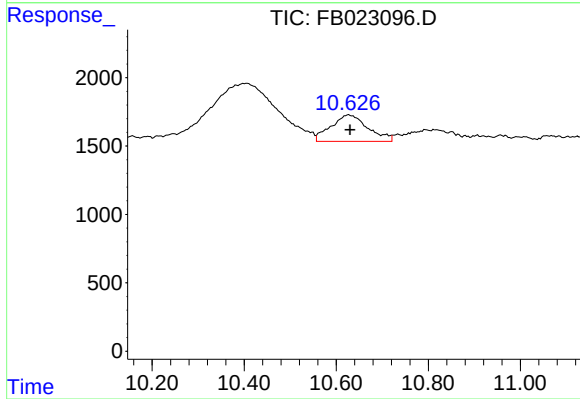


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.003 min
Response: 10822
Conc: 0.27 ng/ml

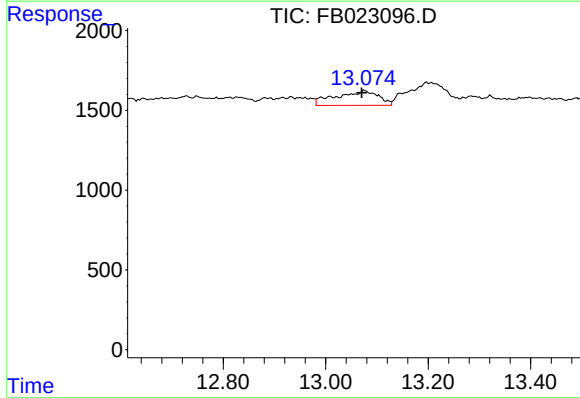


#7 Ethylbenzene

R.T.: 13.076 min
Delta R.T.: 0.006 min
Response: 5217
Conc: 0.14 ng/ml

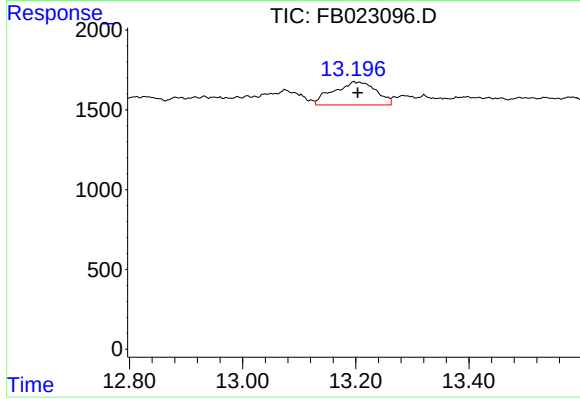


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 7477
Conc: 0.21 ng/ml

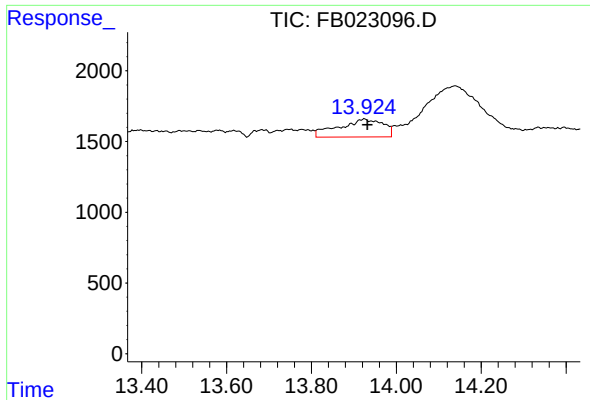

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.007 min
Response: 9106
Conc: 0.26 ng/ml

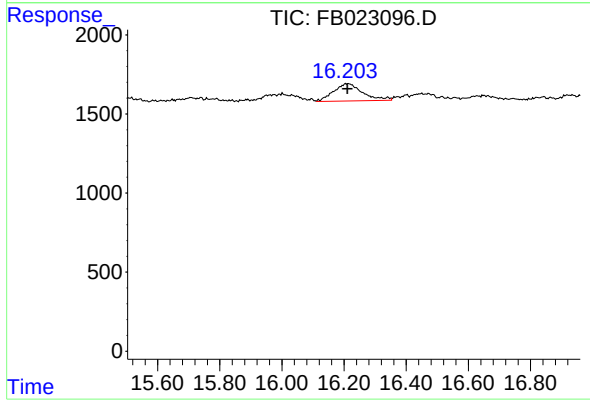

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.002 min
Response: 7030
Conc: 0.25 ng/ml