

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112619\
 Data File : FB023097.D
 Signal(s) : FID2B.CH
 Acq On : 26 Nov 2019 12:03
 Operator : DD/AJ
 Sample : BSF1126S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Nov 26 14:17:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	558248	22.726 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	968226	29.629 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1194970	34.269 ng/ml
3) t n-Heptane	7.755	394987	11.488 ng/ml
4) t Benzene	7.889	468723	11.250 ng/ml
6) t Toluene	10.628	1333199	33.095 ng/ml
7) t Ethylbenzene	13.068	422858	10.958 ng/ml
8) t m-Xylene	13.201	798718	21.949 ng/ml
9) t O-Xylene	13.929	758803	21.854 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	618892	22.069 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112619\
Data File : FB023097.D
Signal(s) : FID2B.CH
Acq On : 26 Nov 2019 12:03
Operator : DD/AJ
Sample : BSF1126S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Nov 26 14:17:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

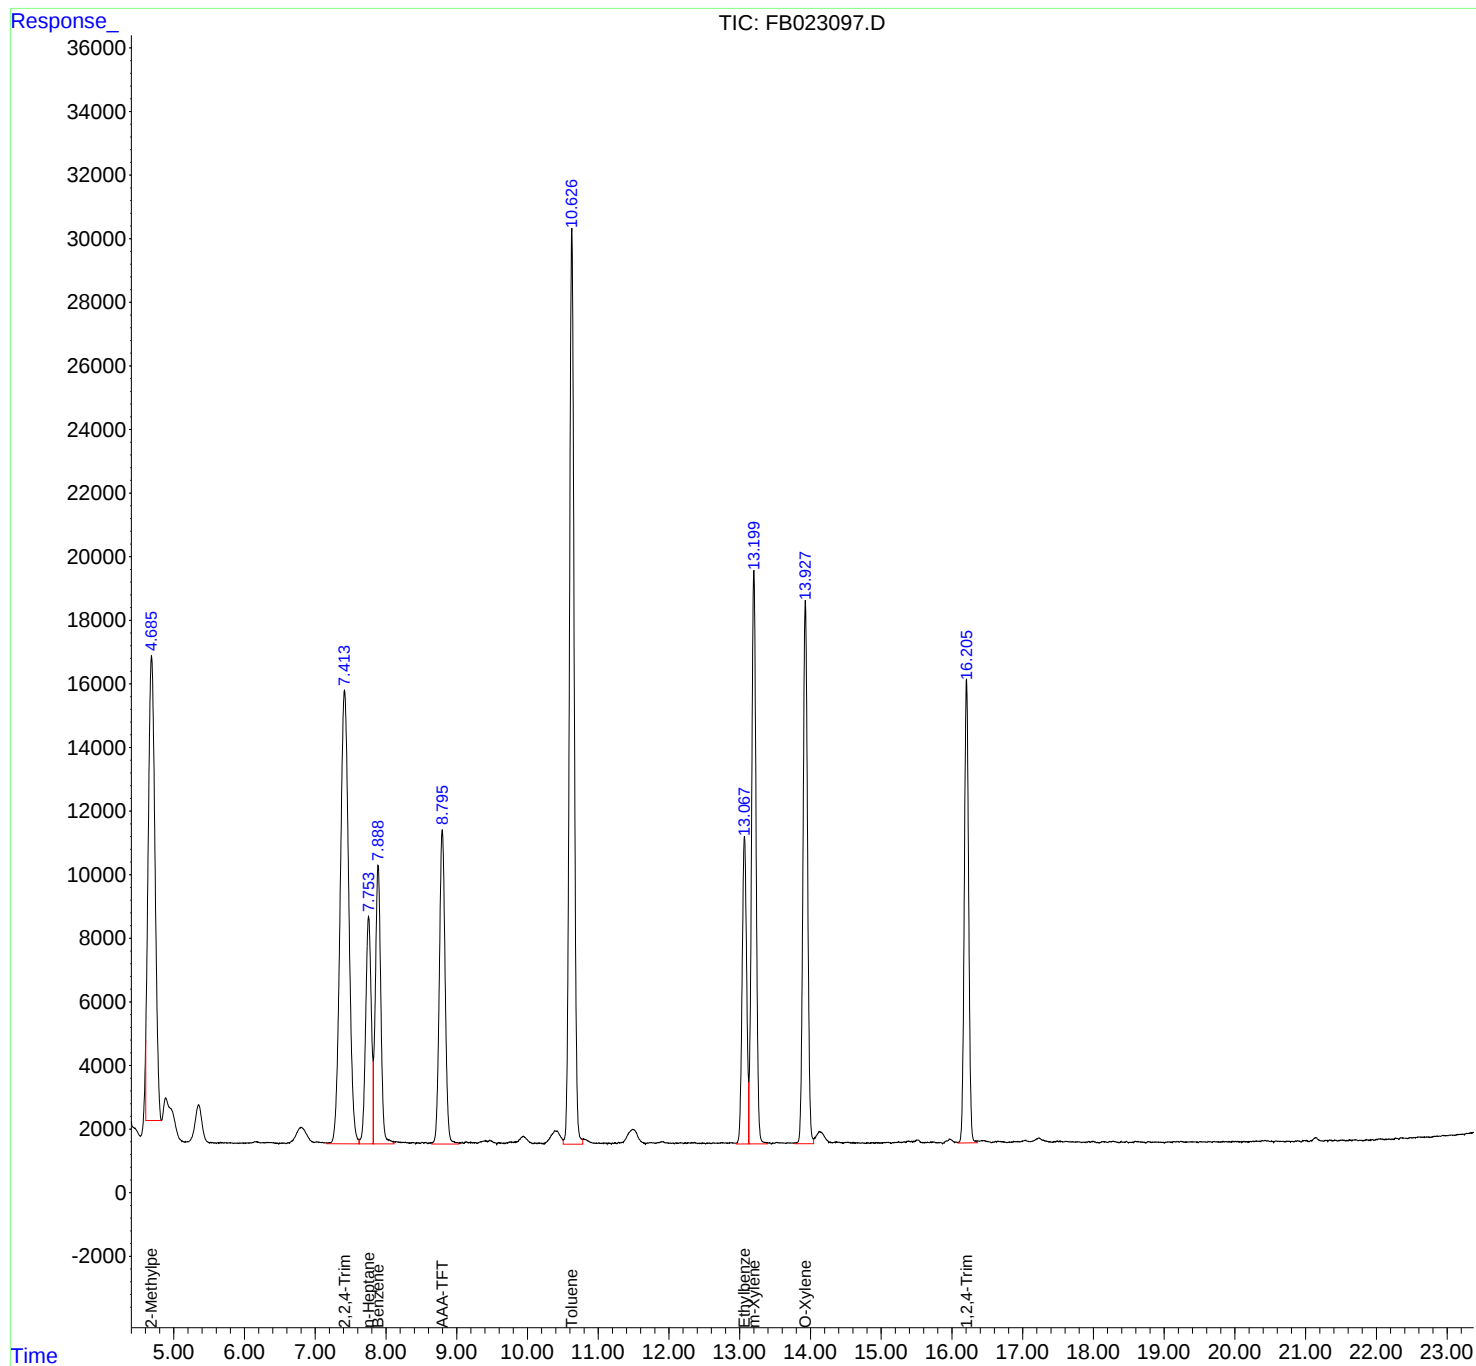

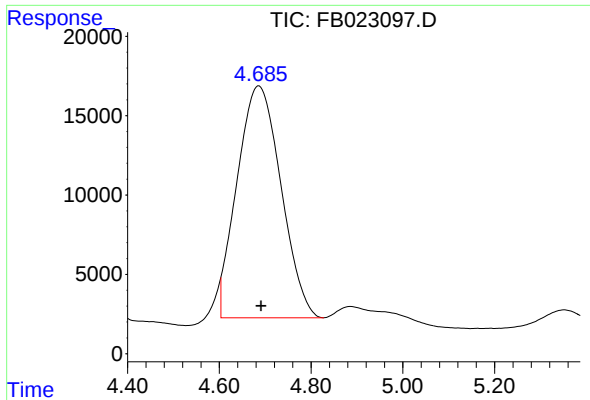


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.005 min
Response: 968226
Conc: 29.63 ng/ml

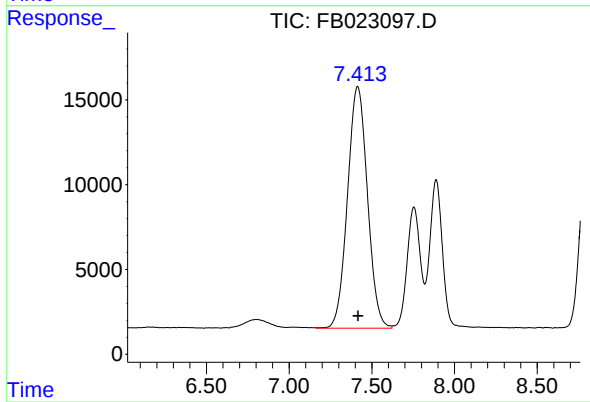


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 1194970
Conc: 34.27 ng/ml

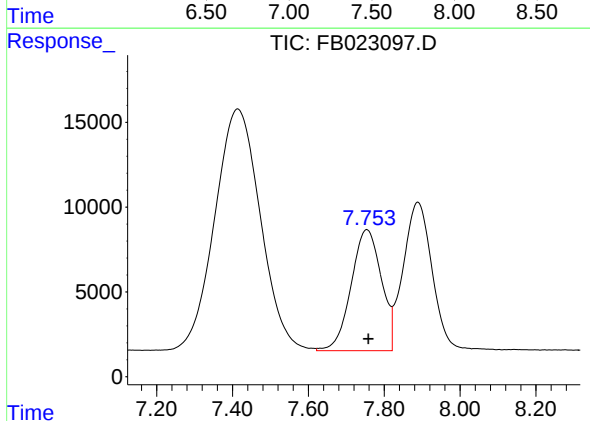


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 394987
Conc: 11.49 ng/ml

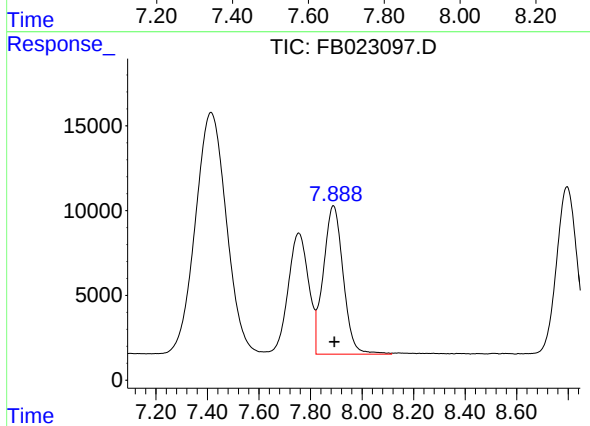


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.003 min
Response: 468723
Conc: 11.25 ng/ml

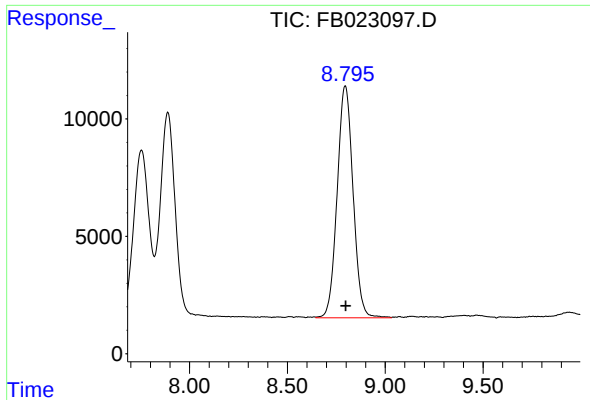


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 558248
Conc: 22.73 ng/ml

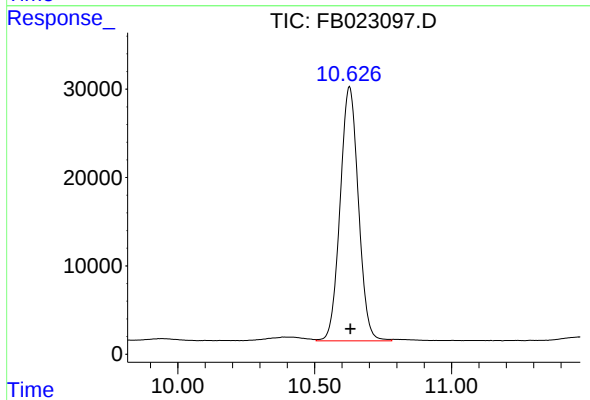


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 1333199
Conc: 33.10 ng/ml

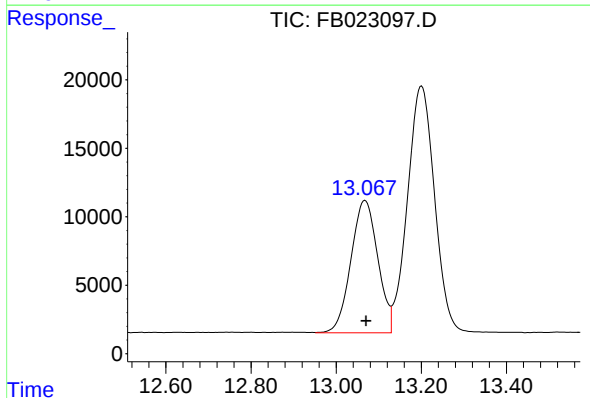


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 422858
Conc: 10.96 ng/ml

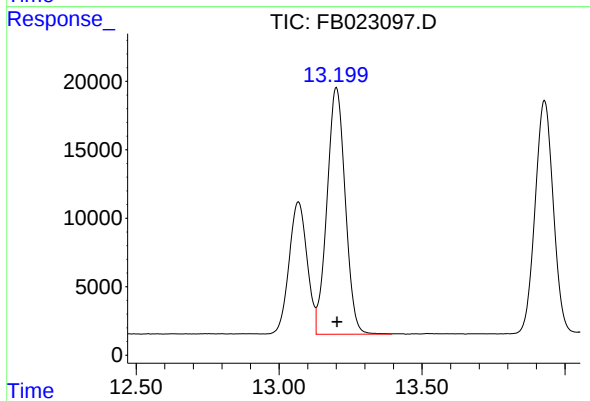

#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.003 min
Response: 798718
Conc: 21.95 ng/ml

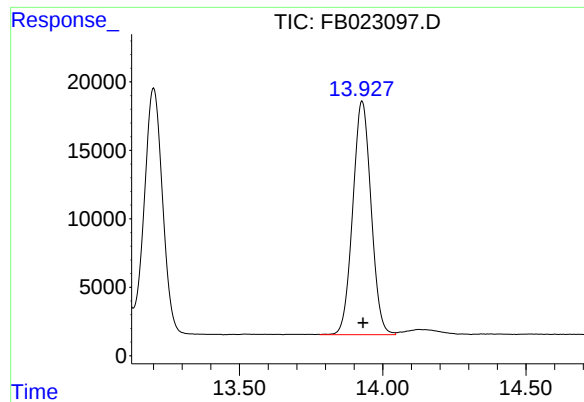


#9 O-Xylene

R.T.: 13.929 min

Delta R.T.: -0.003 min

Response: 758803

Conc: 21.85 ng/ml

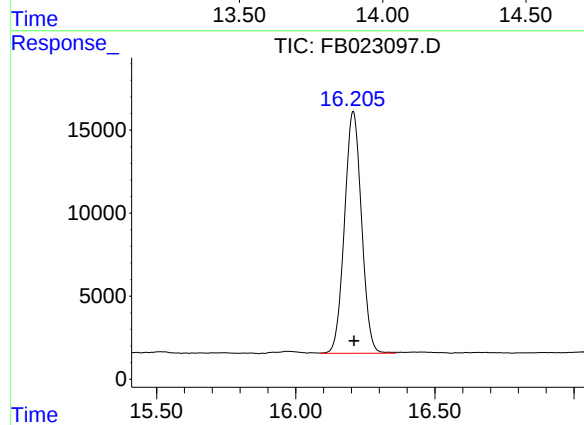

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min

Delta R.T.: -0.003 min

Response: 618892

Conc: 22.07 ng/ml