

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112619\
 Data File : FB023098.D
 Signal(s) : FID2B.CH
 Acq On : 26 Nov 2019 13:02
 Operator : DD/AJ
 Sample : K5948-01
 Misc : 7.99g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Nov 26 14:17:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	515872	21.001 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	1436	0.044 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	6179	0.177 ng/ml
3) t n-Heptane	7.744	356	0.010 ng/ml
4) t Benzene	7.887	3683	0.088 ng/ml
6) t Toluene	10.630	8963	0.222 ng/ml
8) t m-Xylene	13.203	5590	0.154 ng/ml
9) t O-Xylene	13.933	4678	0.135 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	13689	0.488 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112619\
Data File : FB023098.D
Signal(s) : FID2B.CH
Acq On : 26 Nov 2019 13:02
Operator : DD/AJ
Sample : K5948-01
Misc : 7.99g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Nov 26 14:17:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

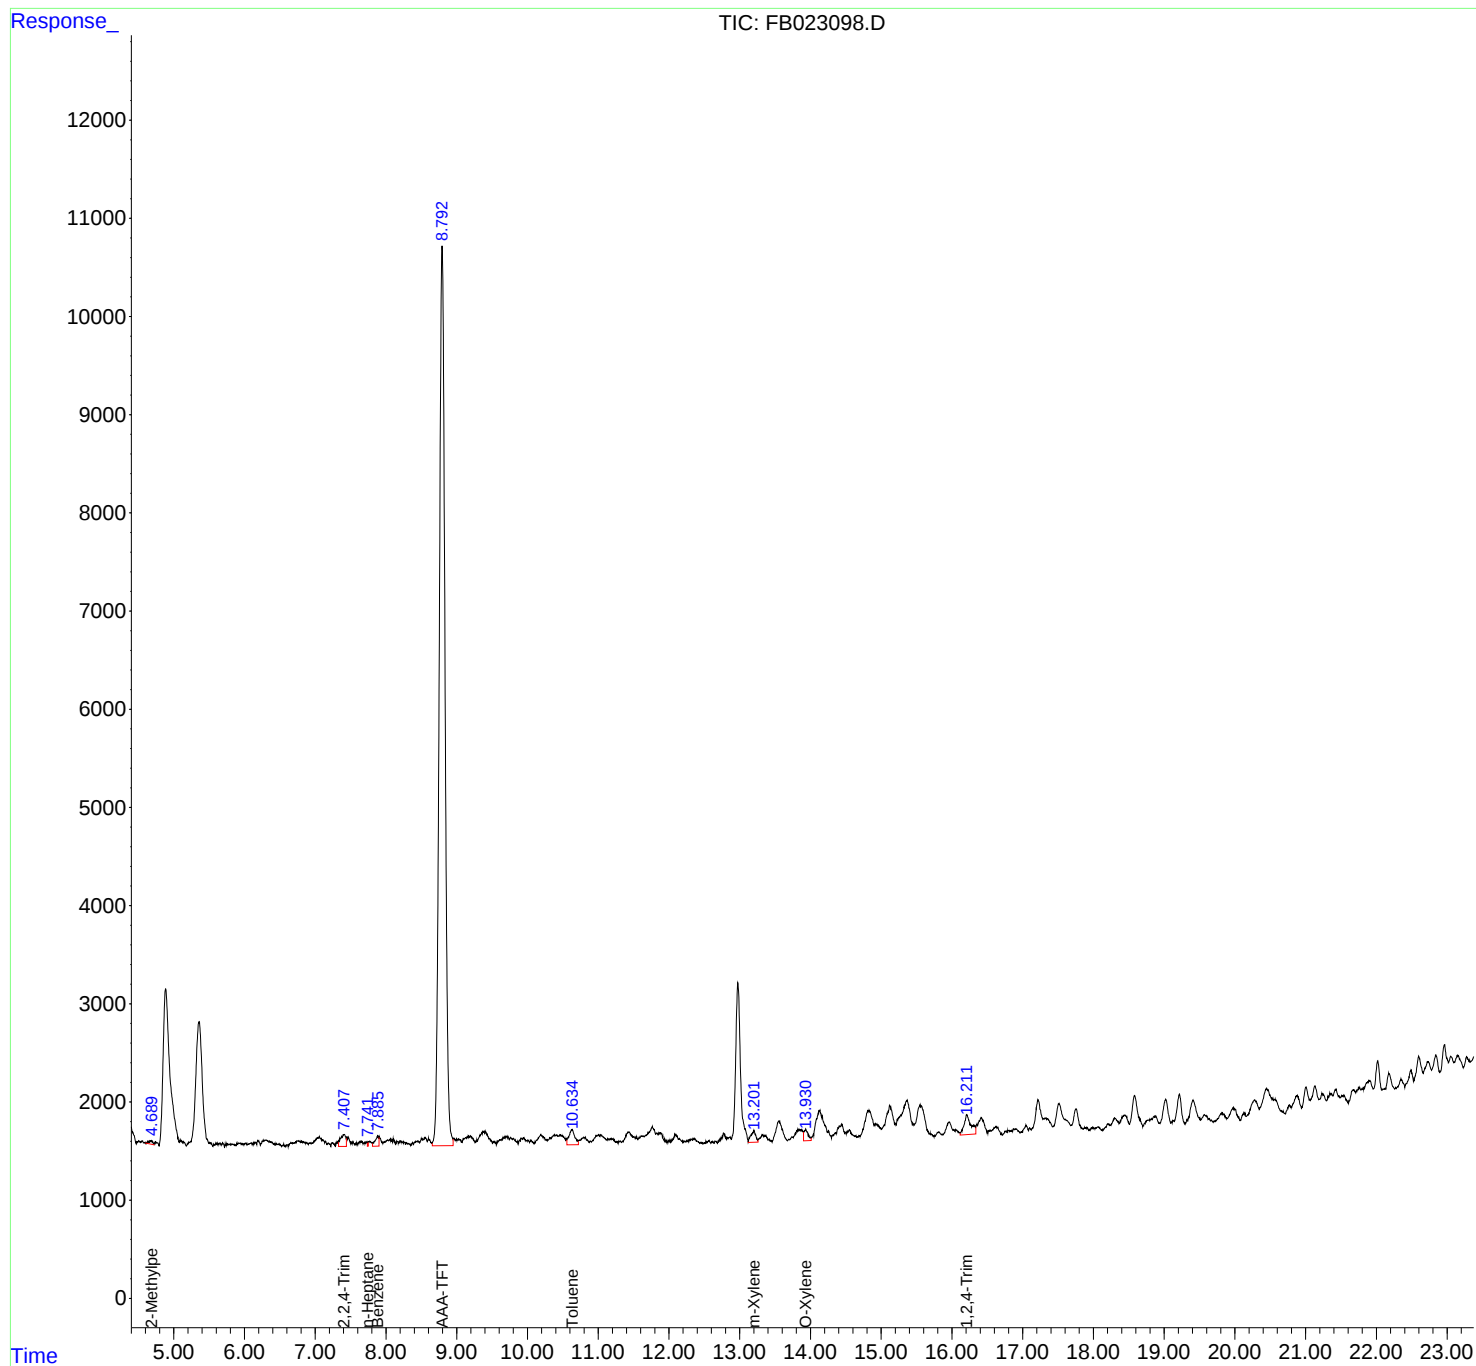

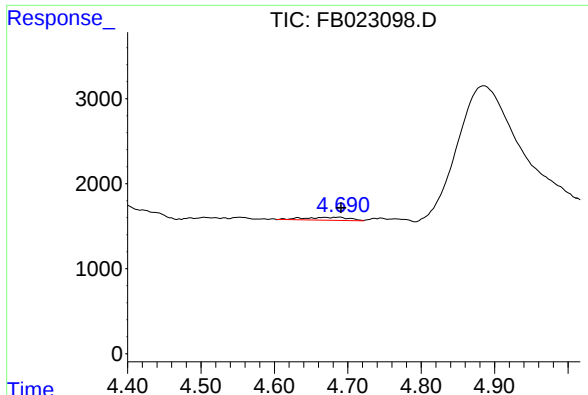


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 1436
Conc: 0.04 ng/ml

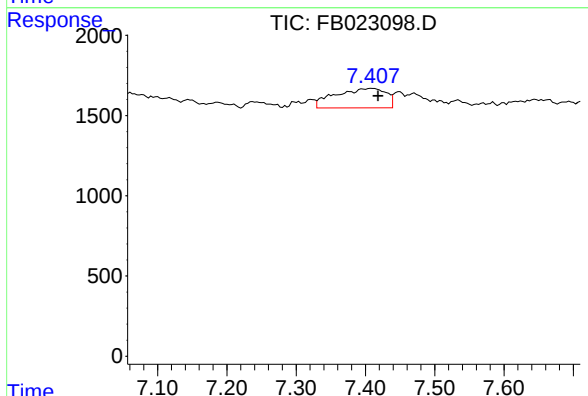


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.008 min
Response: 6179
Conc: 0.18 ng/ml

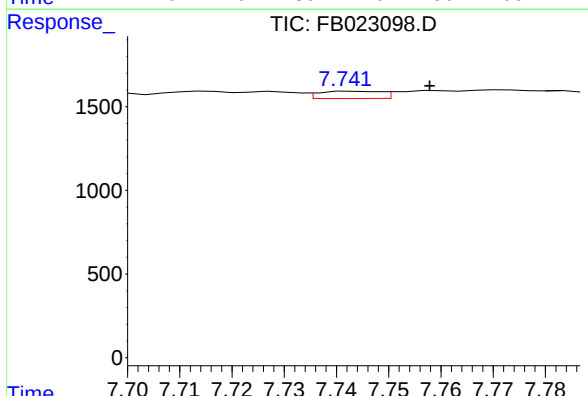


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.014 min
Response: 356
Conc: 0.01 ng/ml

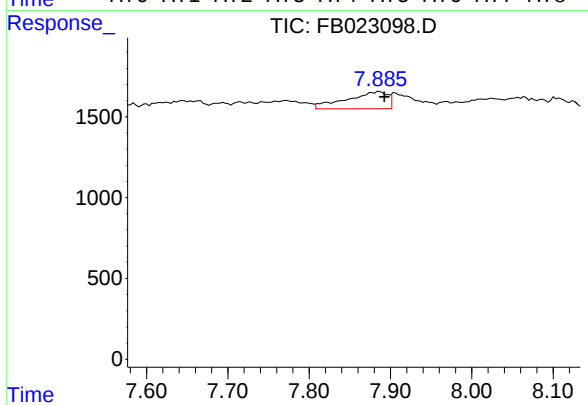


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.006 min
Response: 3683
Conc: 0.09 ng/ml

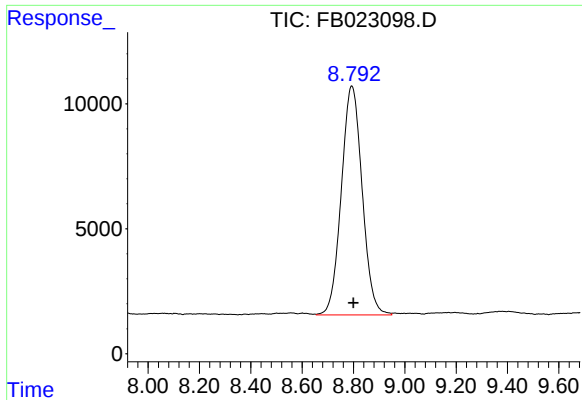


#5 AAA-TFT

R.T.: 8.794 min
 Delta R.T.: -0.005 min
 Response: 515872
 Conc: 21.00 ng/ml

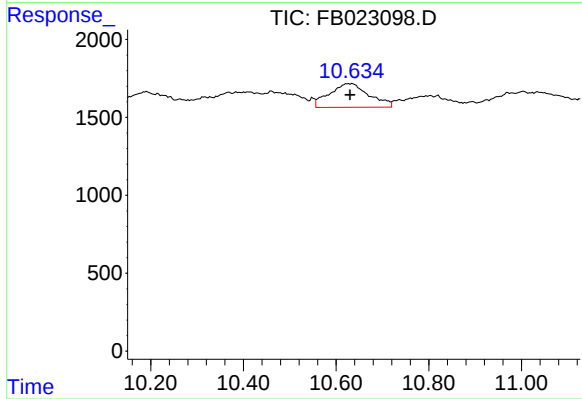


#6 Toluene

R.T.: 10.630 min
 Delta R.T.: 0.000 min
 Response: 8963
 Conc: 0.22 ng/ml

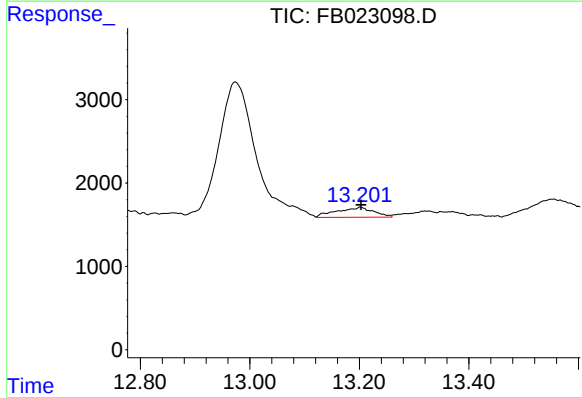


#8 m-Xylene

R.T.: 13.203 min
 Delta R.T.: 0.000 min
 Response: 5590
 Conc: 0.15 ng/ml

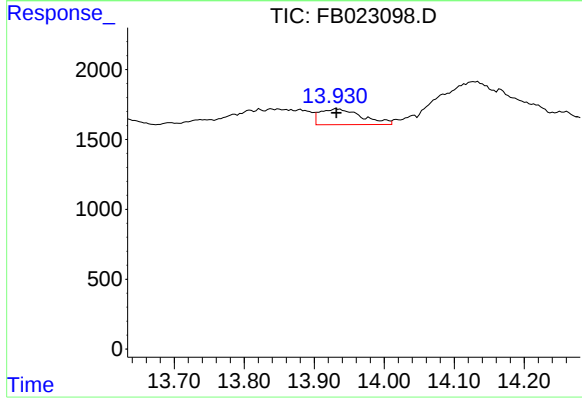

#9 O-Xylene

R.T.: 13.933 min
 Delta R.T.: 0.002 min
 Response: 4678
 Conc: 0.13 ng/ml

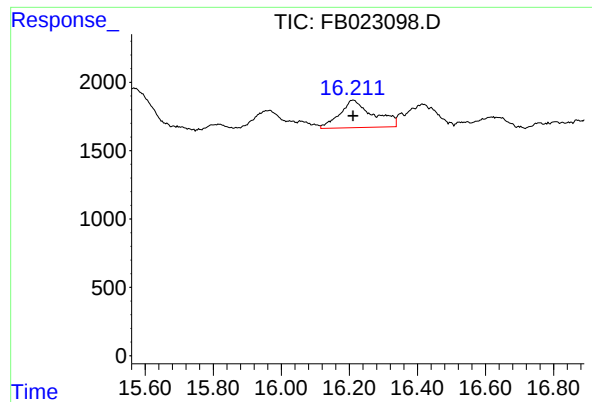

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 13689
Conc: 0.49 ng/ml