

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112519\
 Data File : FB023084.D
 Signal(s) : FID2B.CH
 Acq On : 25 Nov 2019 11:36
 Operator : DD/AJ
 Sample : BSF112551
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Nov 25 12:00:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	540123	21.988 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	1043567	31.935 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	1143567	32.795 ng/ml
3) t n-Heptane	7.755	376754	10.958 ng/ml
4) t Benzene	7.889	441625	10.600 ng/ml
6) t Toluene	10.627	1272856	31.597 ng/ml
7) t Ethylbenzene	13.068	402053	10.419 ng/ml
8) t m-Xylene	13.201	757175	20.807 ng/ml
9) t O-Xylene	13.929	720905	20.763 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	577777	20.603 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112519\
Data File : FB023084.D
Signal(s) : FID2B.CH
Acq On : 25 Nov 2019 11:36
Operator : DD/AJ
Sample : BSF1125S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Nov 25 12:00:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

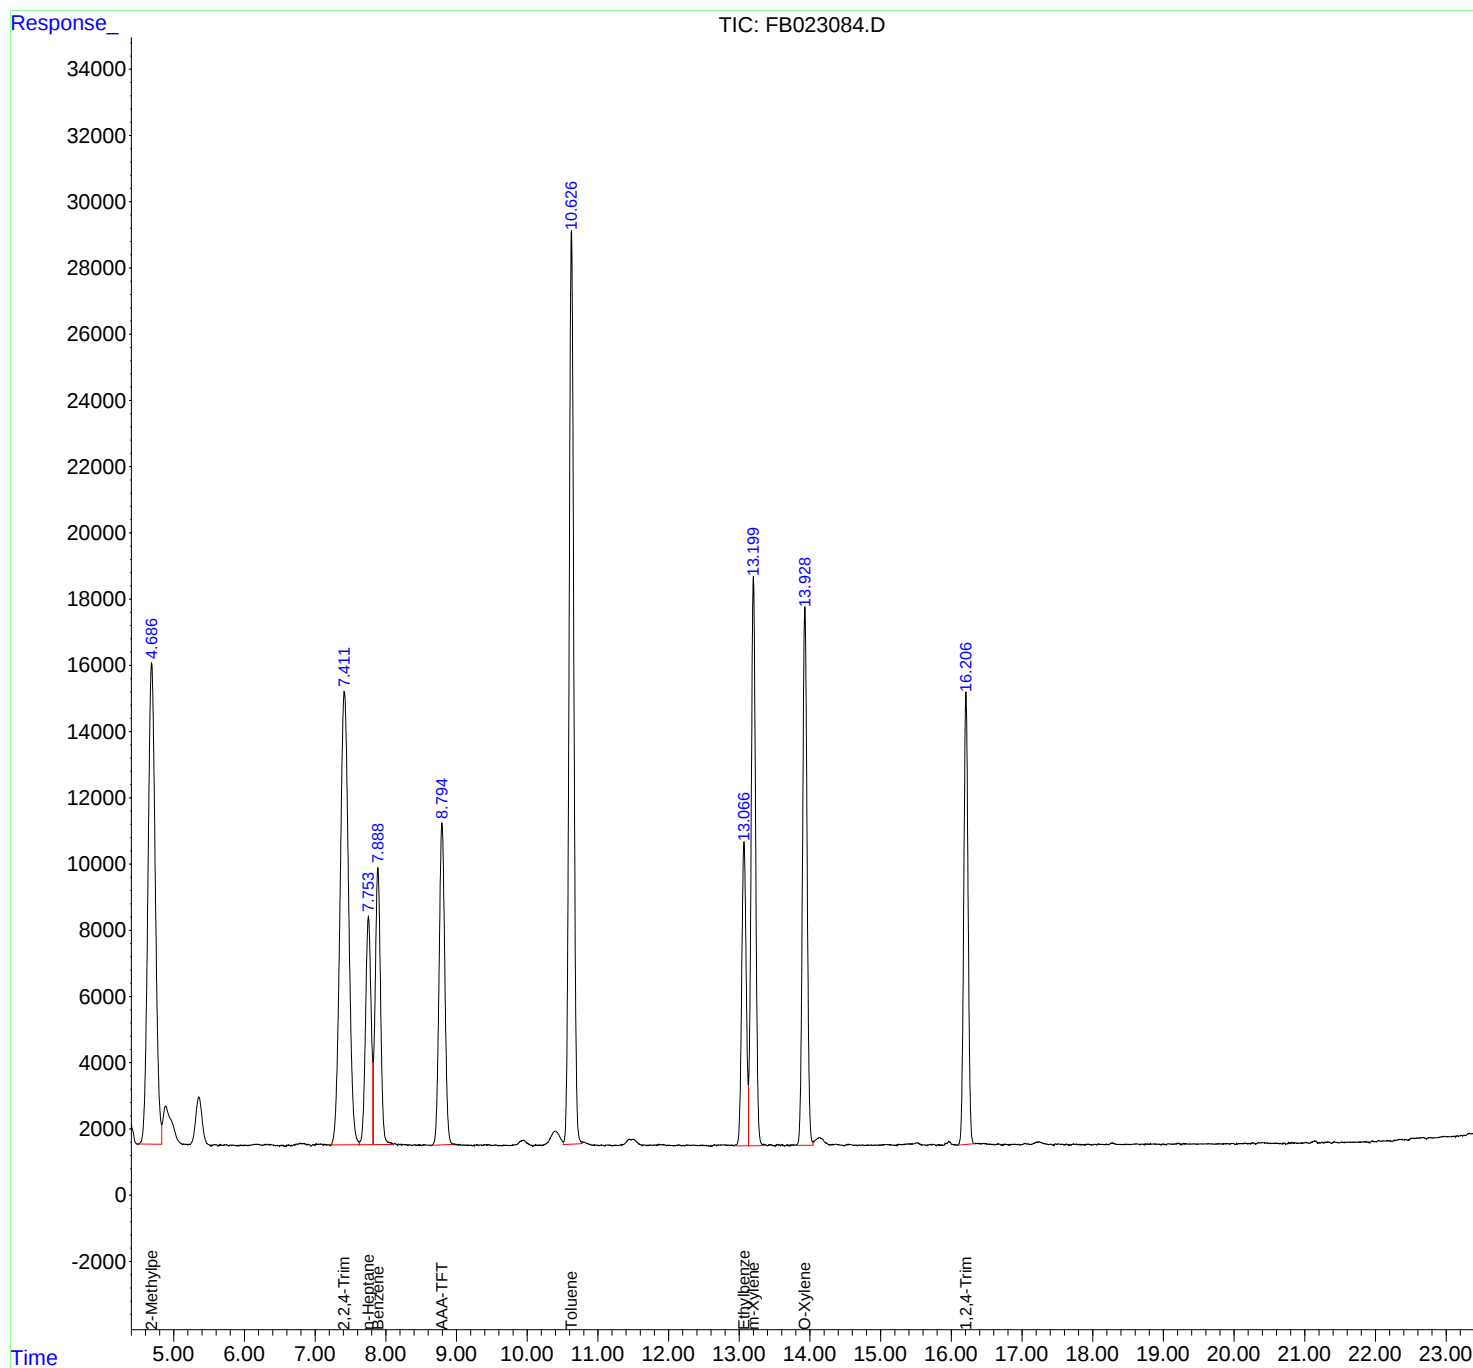

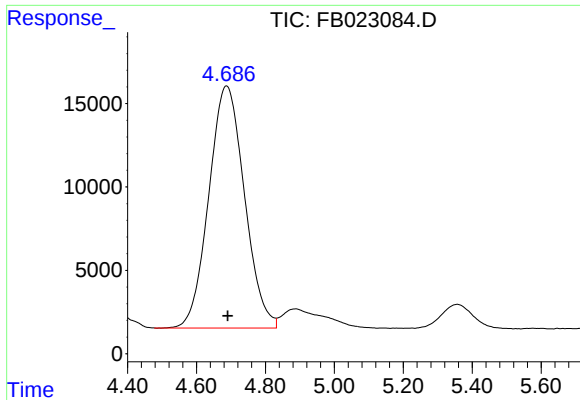


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 1043567
Conc: 31.93 ng/ml

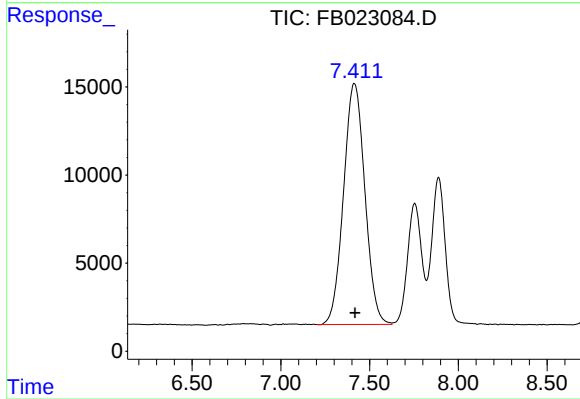


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.005 min
Response: 1143567
Conc: 32.79 ng/ml

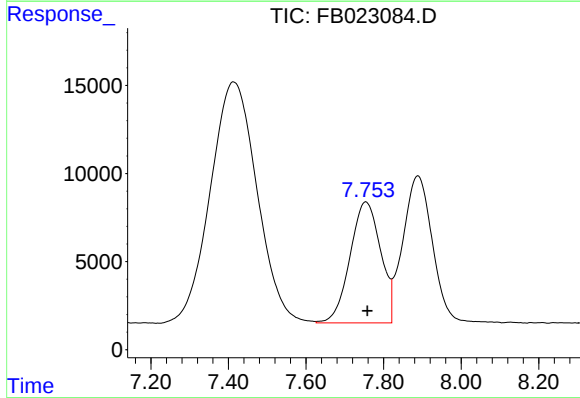


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 376754
Conc: 10.96 ng/ml

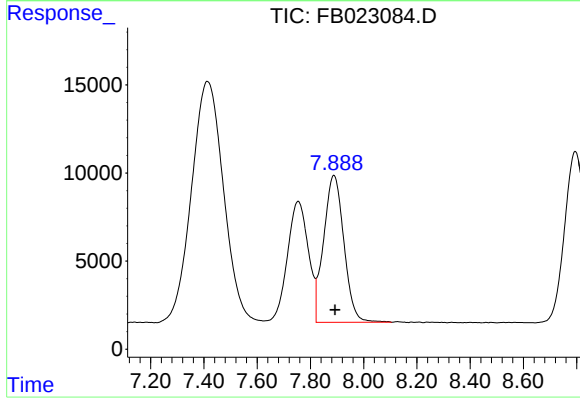


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 441625
Conc: 10.60 ng/ml

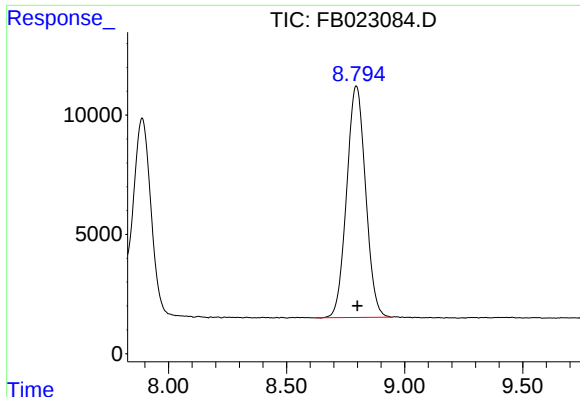


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 540123
Conc: 21.99 ng/ml

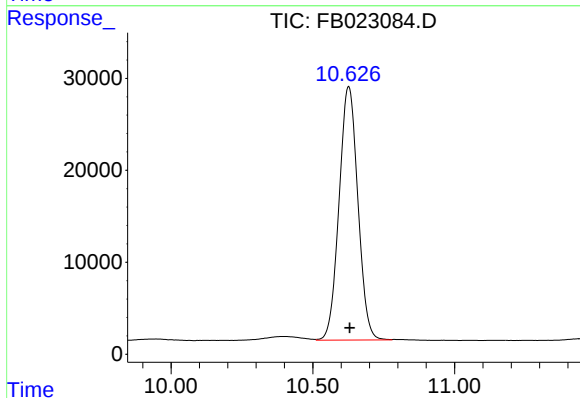


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.003 min
Response: 1272856
Conc: 31.60 ng/ml

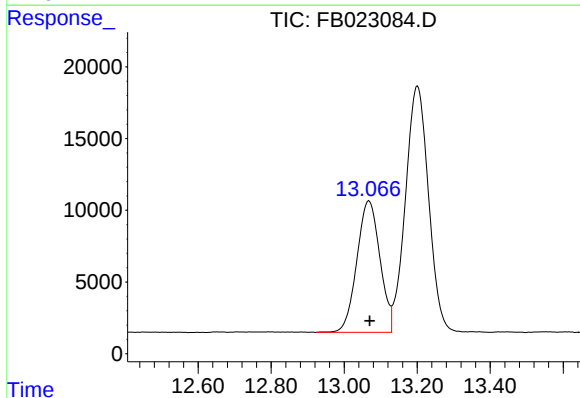


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 402053
Conc: 10.42 ng/ml

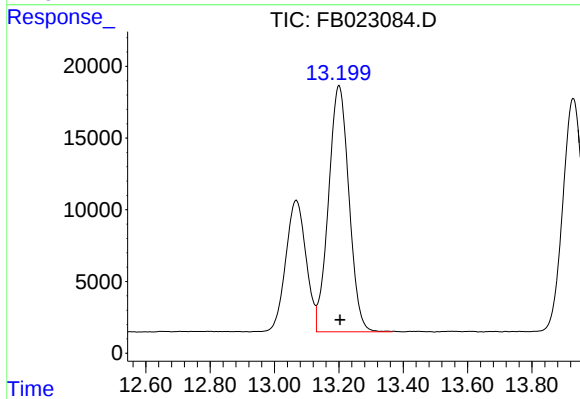


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.003 min
Response: 757175
Conc: 20.81 ng/ml

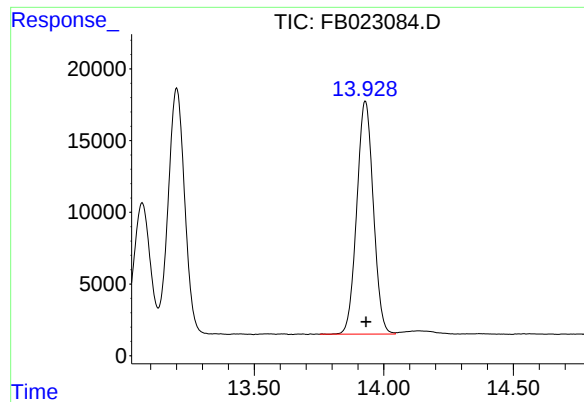

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.003 min
Response: 720905
Conc: 20.76 ng/ml

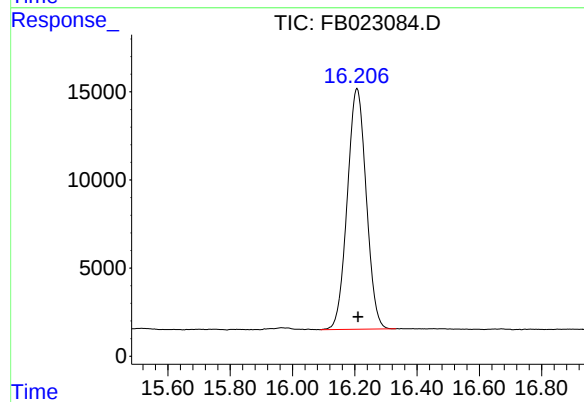

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 577777
Conc: 20.60 ng/ml