

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112520\
 Data File : FB025277.D
 Signal(s) : FID2B.CH
 Acq On : 25 Nov 2020 10:43
 Operator : DD/AJ
 Sample : BSF1125S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1125S1

Integration File: Calibration.e
 Quant Time: Nov 26 00:16:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	453828	20.099 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	987928	30.607 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1075972	32.430 ng/ml
3) t n-Heptane	7.755	350193	10.662 ng/ml
4) t Benzene	7.889	424426	10.675 ng/ml
6) t Toluene	10.627	1203386	32.184 ng/ml
7) t Ethylbenzene	13.068	369089	10.748 ng/ml
8) t m-Xylene	13.200	738682	21.877 ng/ml
9) t O-Xylene	13.928	712797	21.800 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	625244	22.724 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112520\
Data File : FB025277.D
Signal(s) : FID2B.CH
Acq On : 25 Nov 2020 10:43
Operator : DD/AJ
Sample : BSF1125S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1125S1

Integration File: Calibration.e
Quant Time: Nov 26 00:16:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

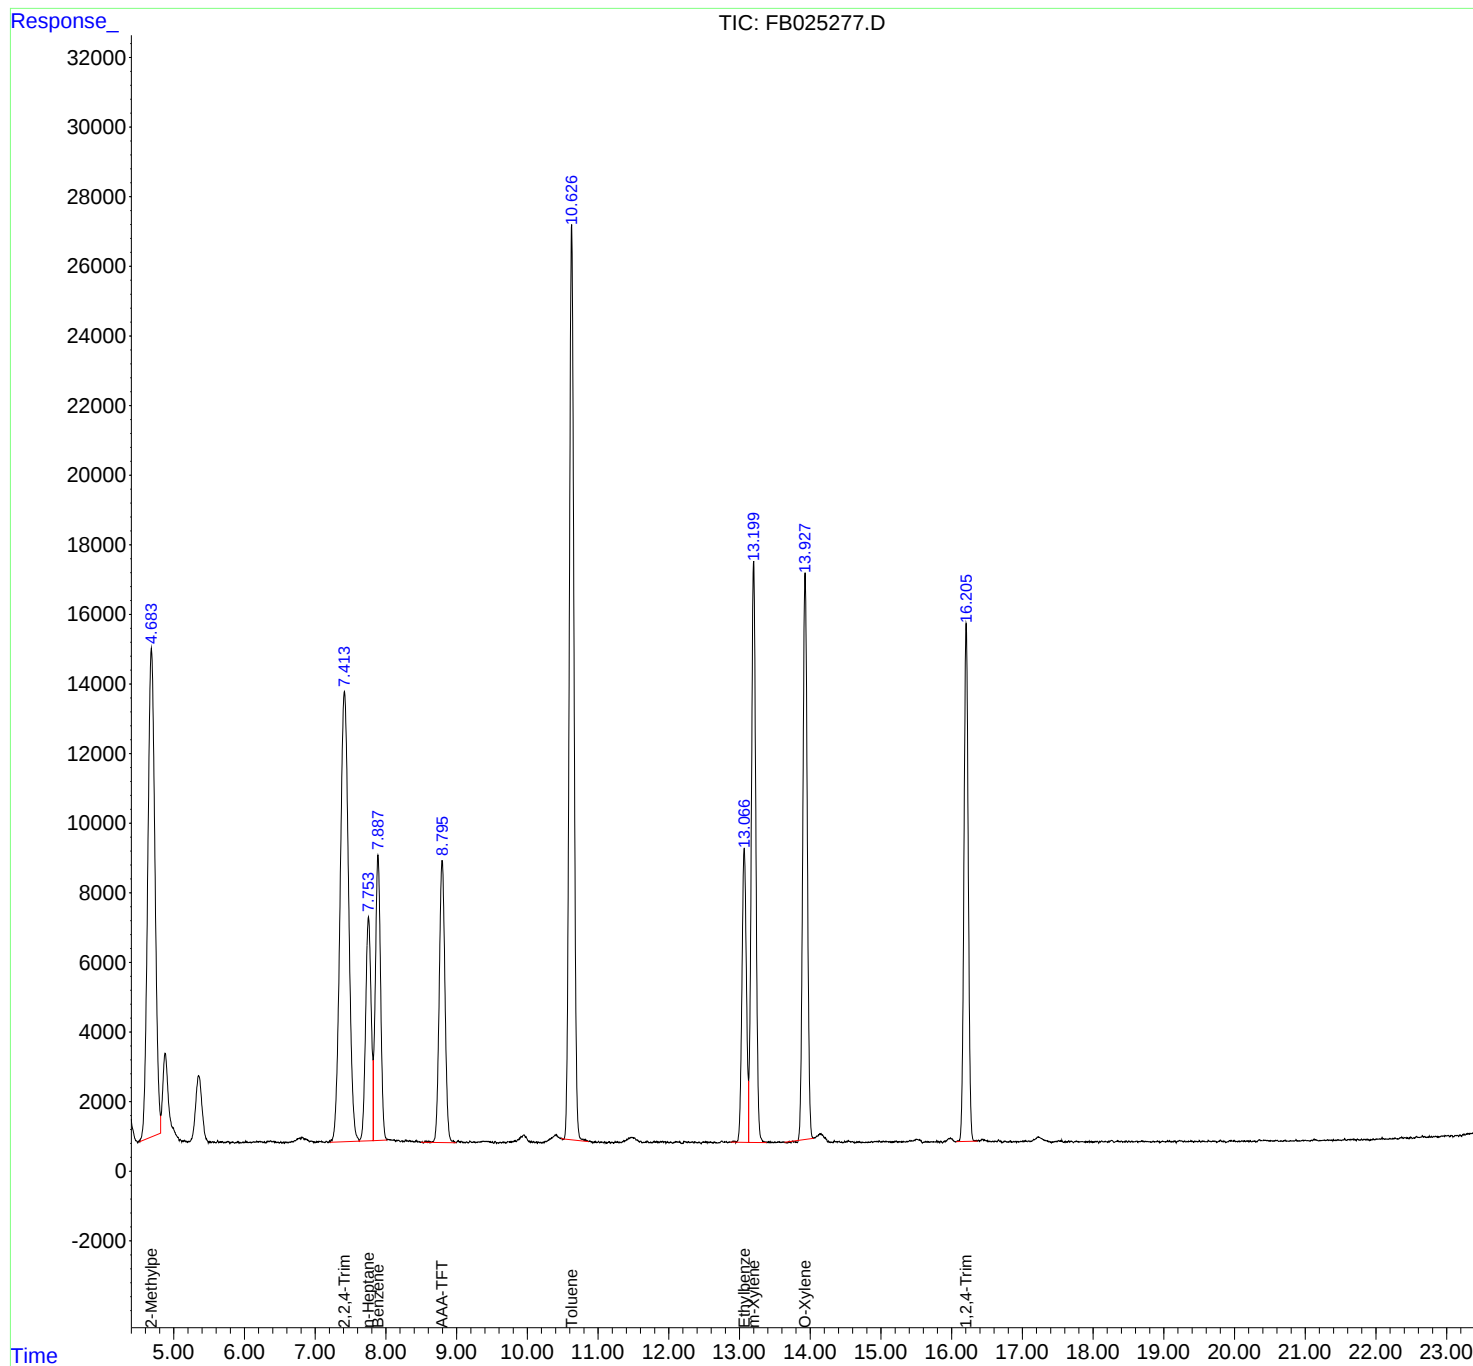


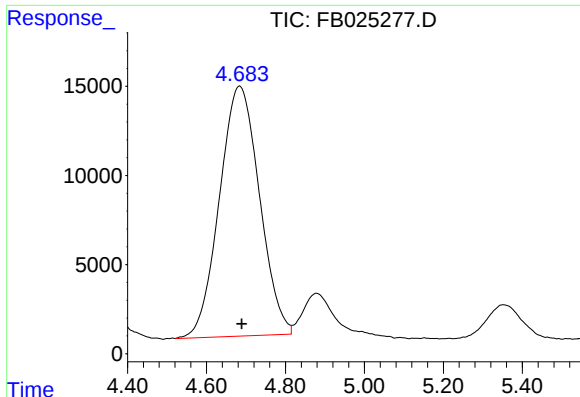

#1 2-Methylpentane


R.T.: 4.684 min
Delta R.T.: -0.005 min
Response: 987928
Conc: 30.61 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1125S1

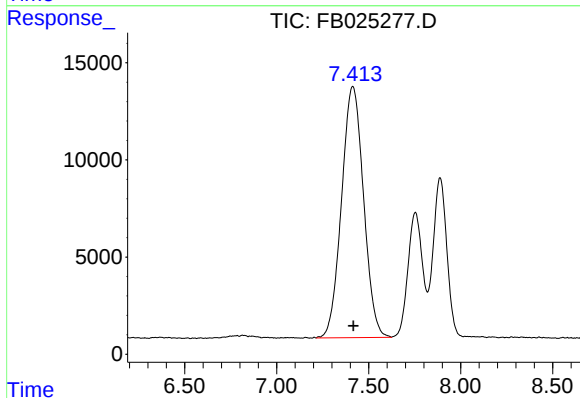


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 1075972
Conc: 32.43 ng/ml

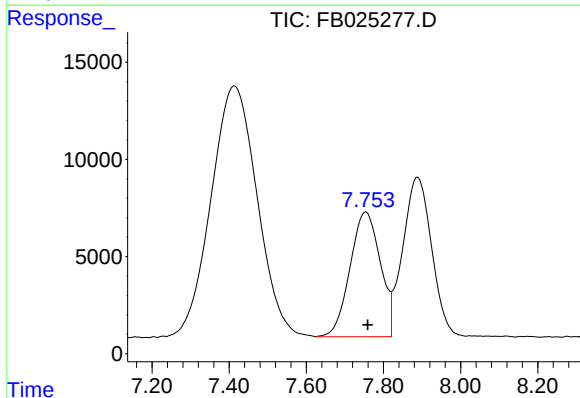


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.004 min
Response: 350193
Conc: 10.66 ng/ml

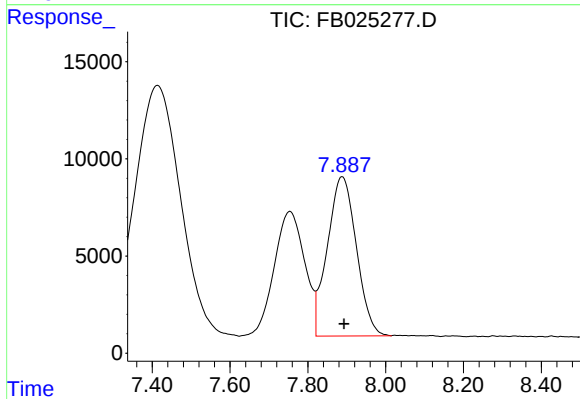

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.005 min
Response: 424426
Conc: 10.67 ng/ml

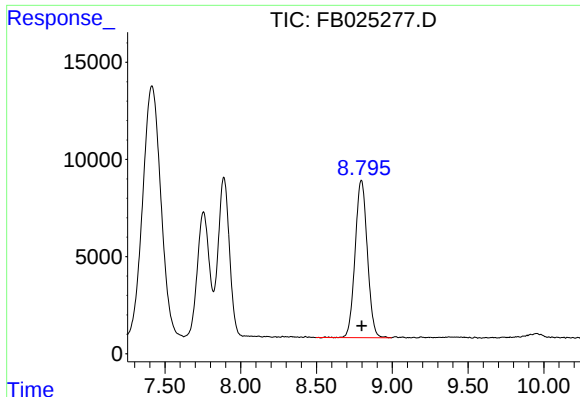

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 453828
Conc: 20.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1125S1

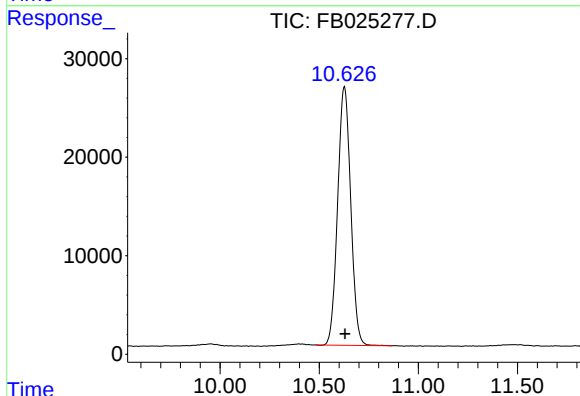


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.003 min
Response: 1203386
Conc: 32.18 ng/ml

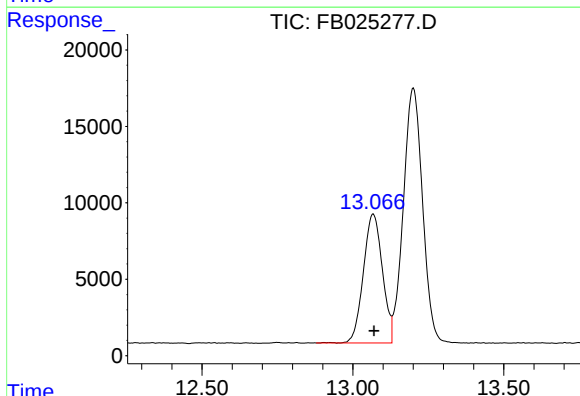


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 369089
Conc: 10.75 ng/ml

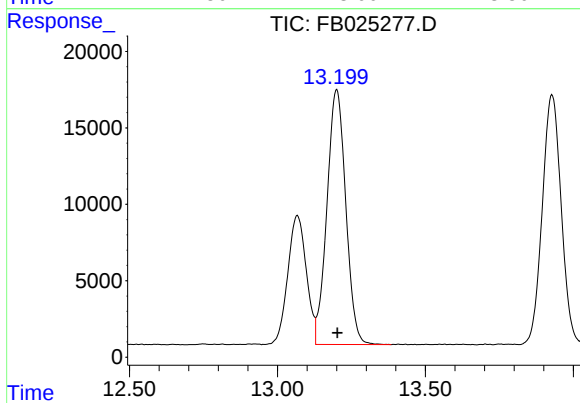

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 738682
Conc: 21.88 ng/ml

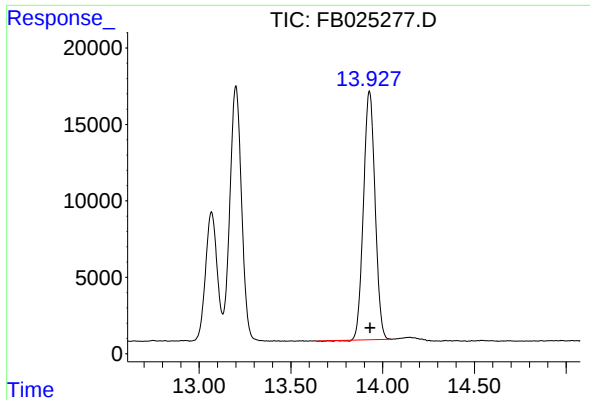

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.003 min
Response: 712797
Conc: 21.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1125S1

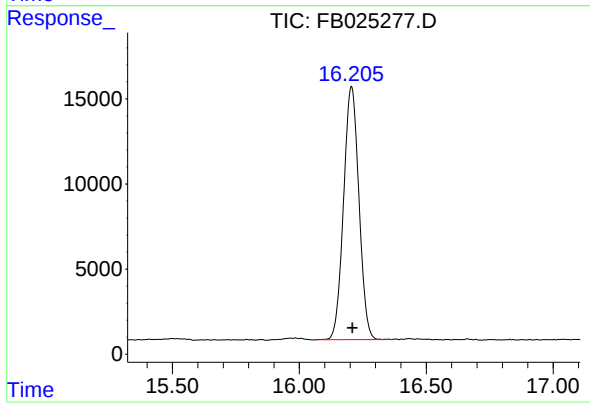

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.003 min
Response: 625244
Conc: 22.72 ng/ml