

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112520\
 Data File : FB025280.D
 Signal(s) : FID2B.CH
 Acq On : 25 Nov 2020 12:29
 Operator : DD/AJ
 Sample : L4868-04MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 KENS-B3-112020-8-10MSD

Integration File: Calibration.e
 Quant Time: Nov 26 00:17:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	489668	21.686 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	874910	27.106 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	771604	23.256 ng/ml
3) t n-Heptane	7.756	254592	7.751 ng/ml
4) t Benzene	7.890	409711	10.305 ng/ml
6) t Toluene	10.628	1126374	30.124 ng/ml
7) t Ethylbenzene	13.068	329167	9.585 ng/ml
8) t m-Xylene	13.201	661398	19.589 ng/ml
9) t O-Xylene	13.929	637280	19.491 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	536830	19.510 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112520\
Data File : FB025280.D
Signal(s) : FID2B.CH
Acq On : 25 Nov 2020 12:29
Operator : DD/AJ
Sample : L4868-04MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-B3-112020-8-10MSD

Integration File: Calibration.e
Quant Time: Nov 26 00:17:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

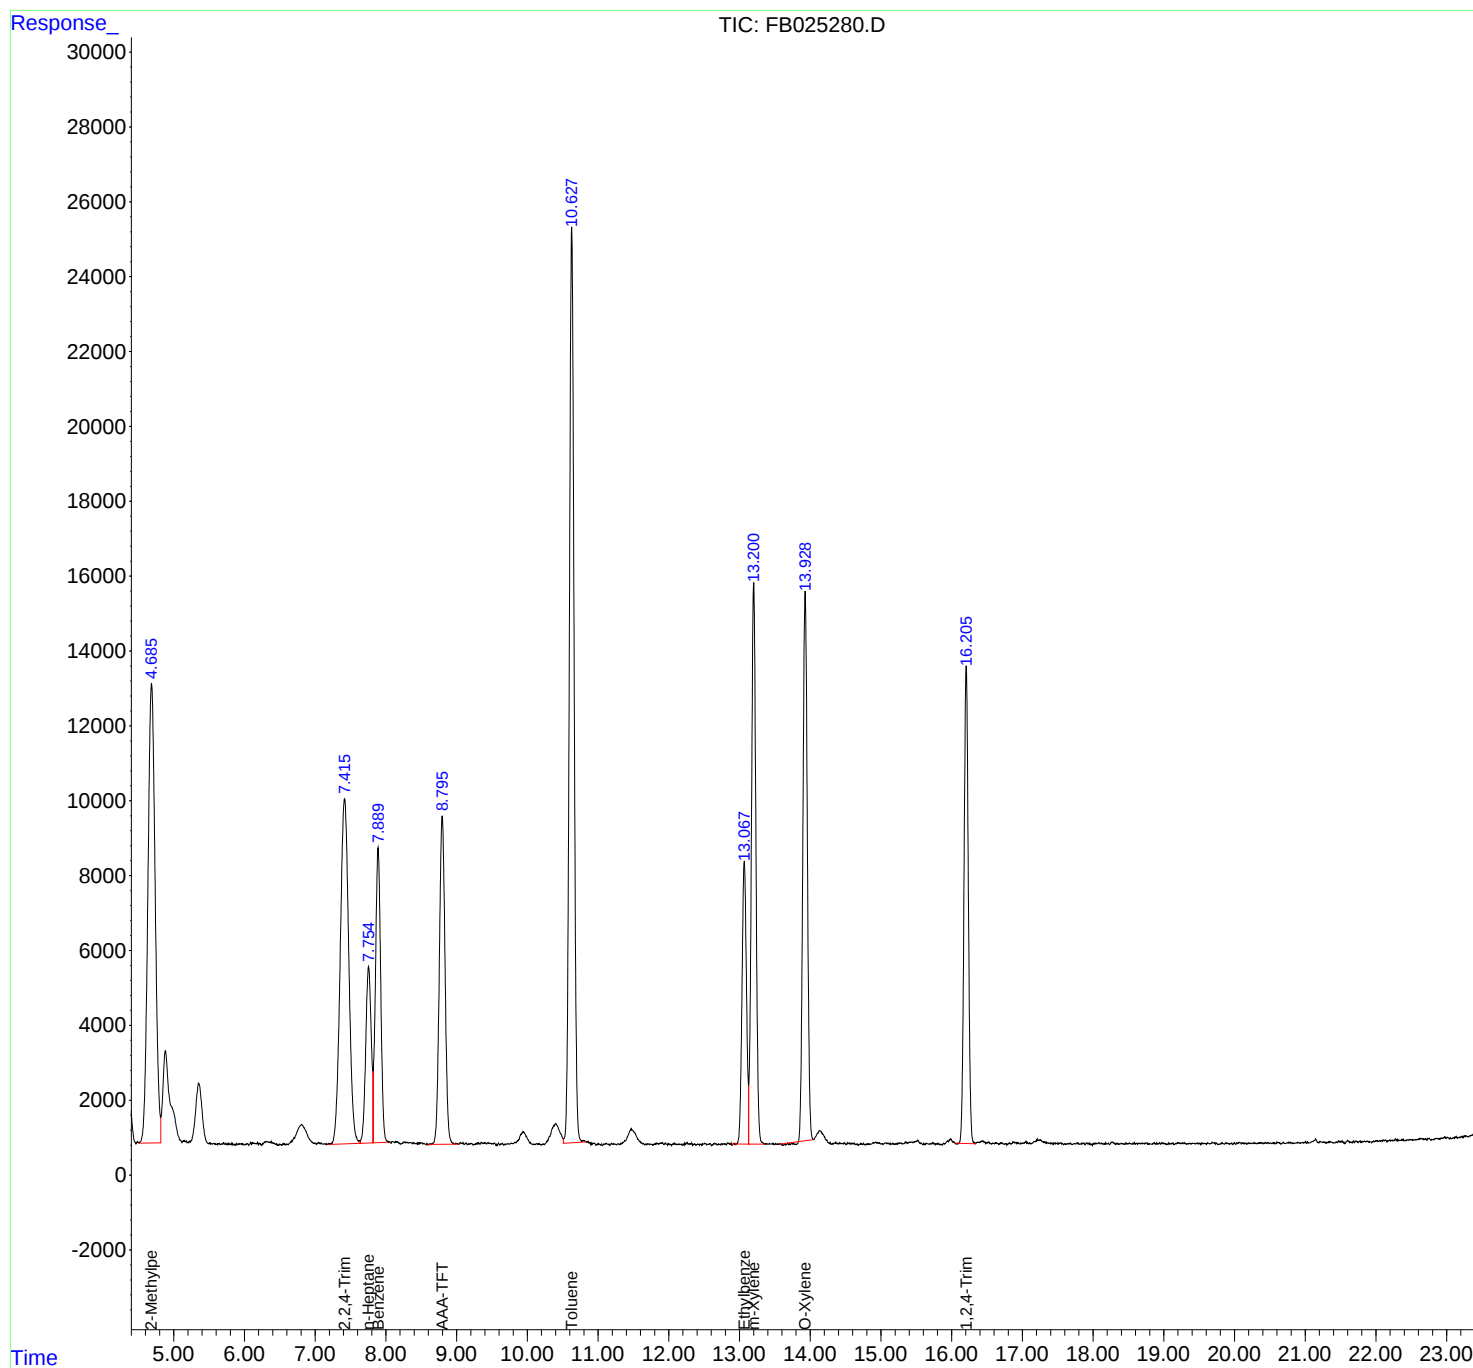


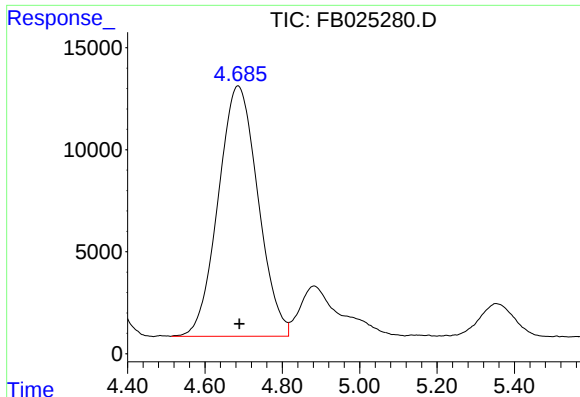

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 874910
Conc: 27.11 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B3-112020-8-10MSD

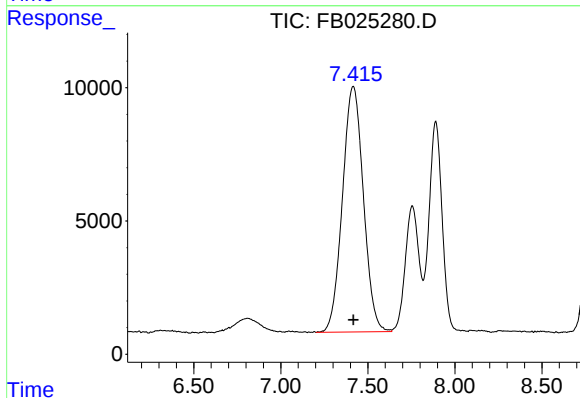


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 771604
Conc: 23.26 ng/ml

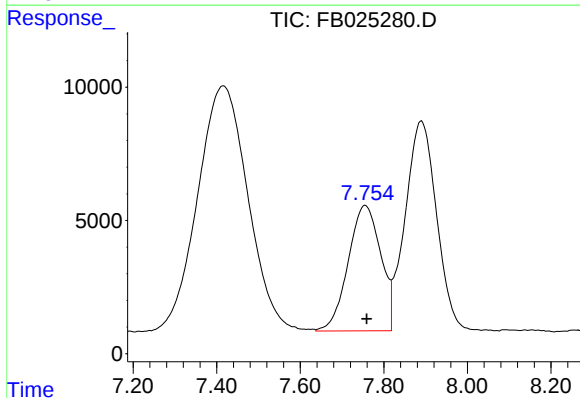


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 254592
Conc: 7.75 ng/ml

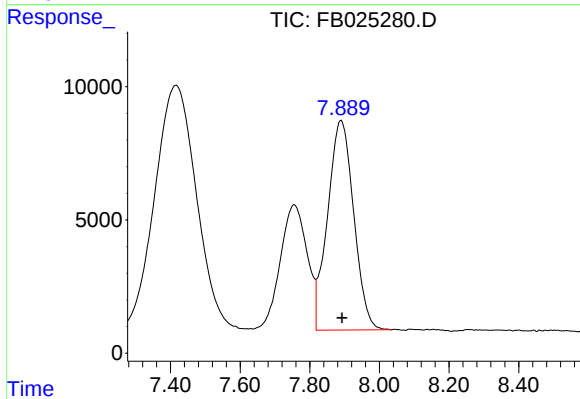

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 409711
Conc: 10.30 ng/ml

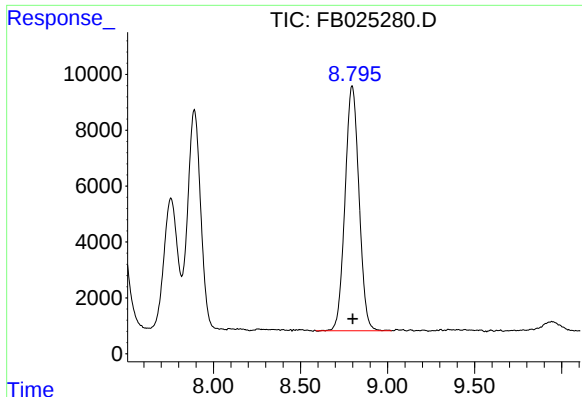

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.003 min
Response: 489668
Conc: 21.69 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B3-112020-8-10MSD

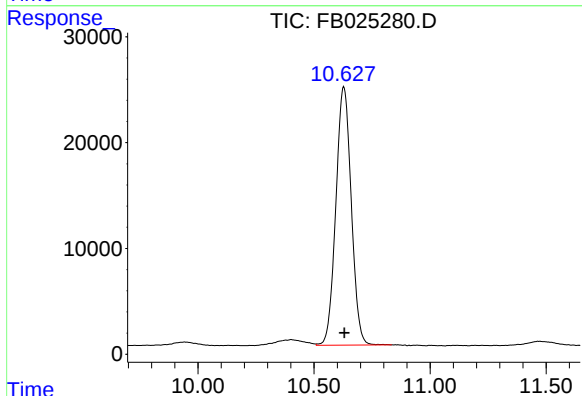


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 1126374
Conc: 30.12 ng/ml

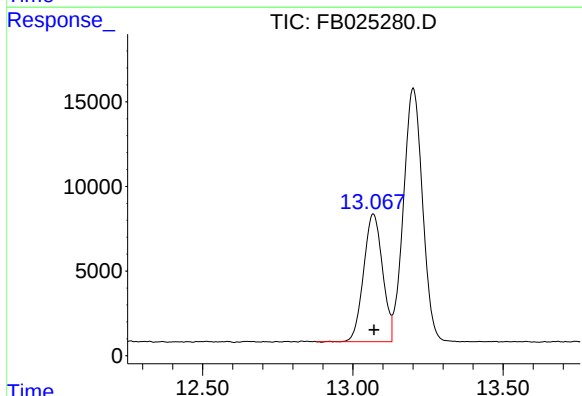


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.002 min
Response: 329167
Conc: 9.59 ng/ml

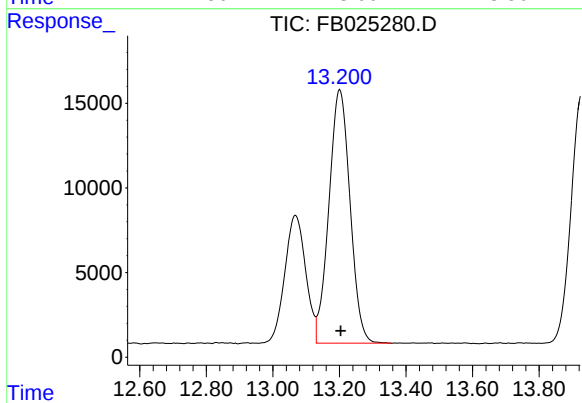

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 661398
Conc: 19.59 ng/ml

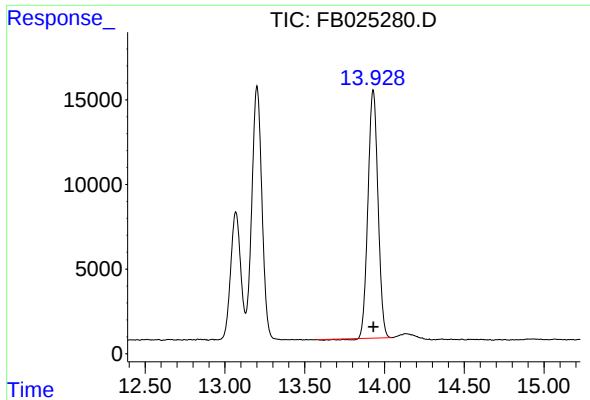

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 637280
Conc: 19.49 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B3-112020-8-10MSD

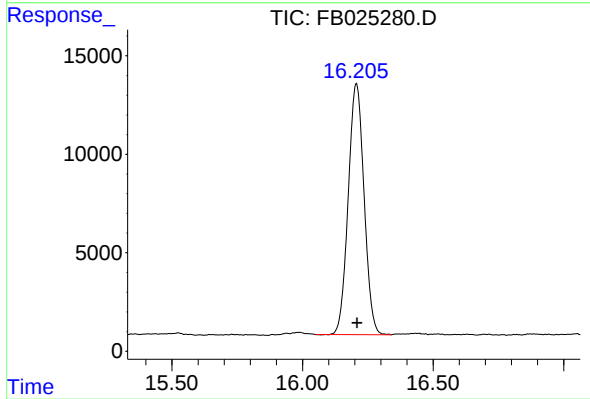

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 536830
Conc: 19.51 ng/ml