

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112619\
 Data File : FB023102.D
 Signal(s) : FID2B.CH
 Acq On : 26 Nov 2019 16:35
 Operator : DD/AJ
 Sample : K5670-10MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 27 00:12:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	564139	22.966 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	998423	30.553 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	1058161	30.345 ng/ml
3) t n-Heptane	7.756	346169	10.068 ng/ml
4) t Benzene	7.891	435719	10.458 ng/ml
6) t Toluene	10.628	1255195	31.159 ng/ml
7) t Ethylbenzene	13.068	393475	10.197 ng/ml
8) t m-Xylene	13.201	736249	20.232 ng/ml
9) t O-Xylene	13.929	701740	20.211 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	576096	20.543 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112619\
Data File : FB023102.D
Signal(s) : FID2B.CH
Acq On : 26 Nov 2019 16:35
Operator : DD/AJ
Sample : K5670-10MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 27 00:12:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

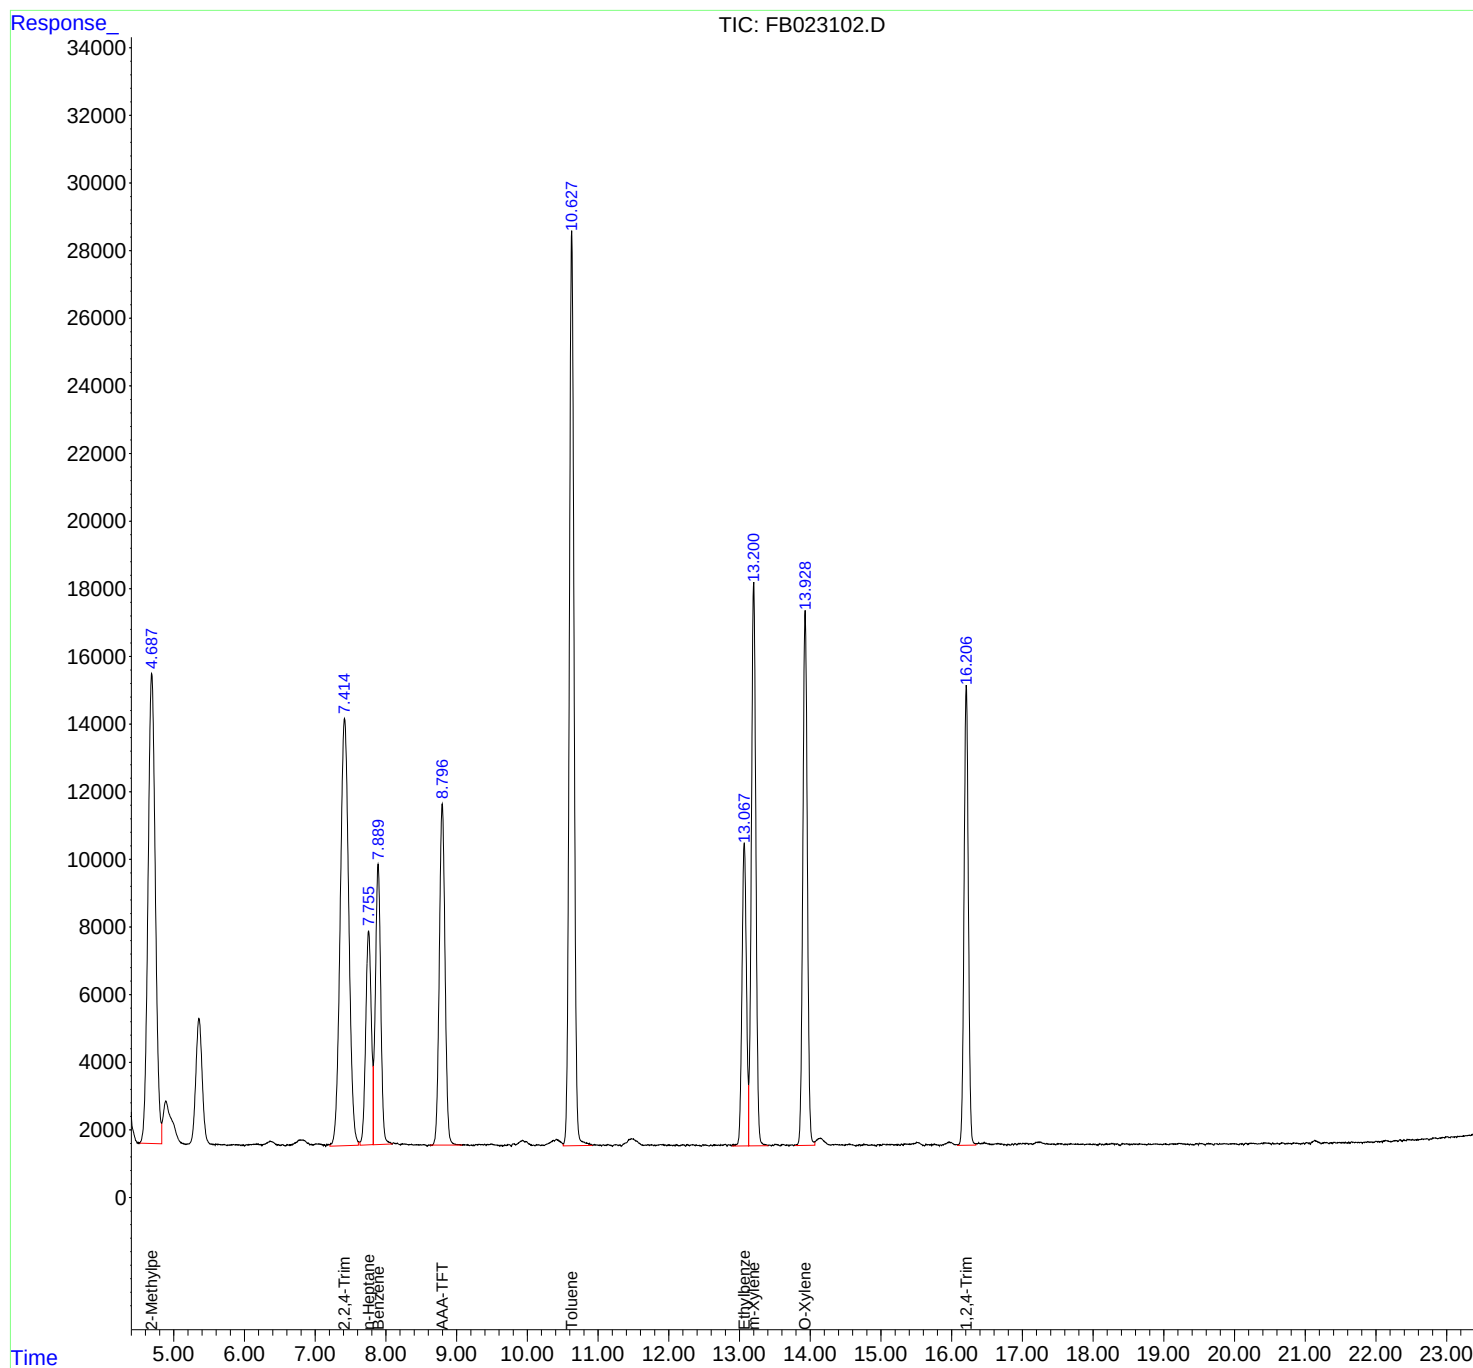

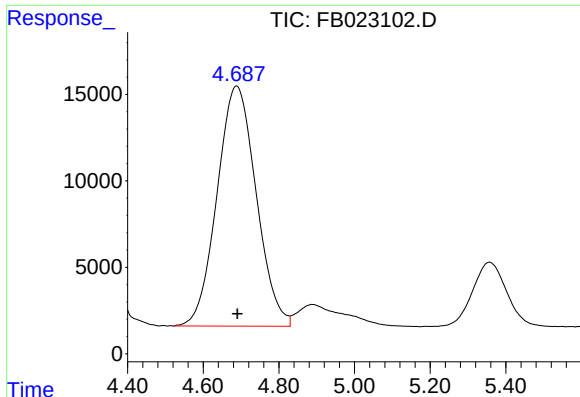


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 998423
Conc: 30.55 ng/ml

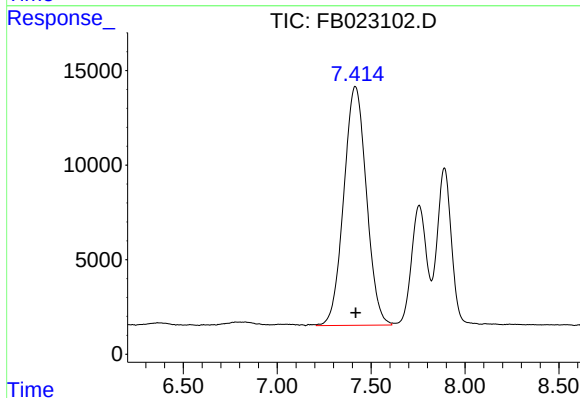


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 1058161
Conc: 30.35 ng/ml

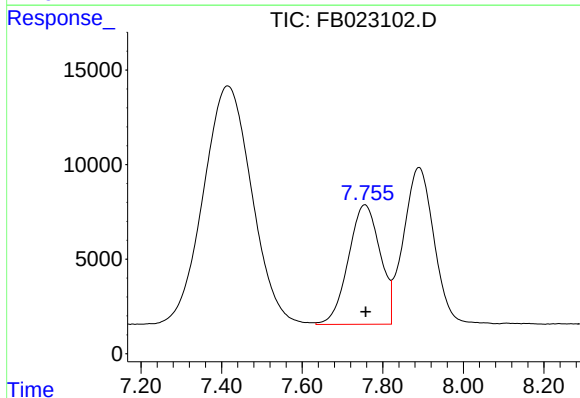


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 346169
Conc: 10.07 ng/ml

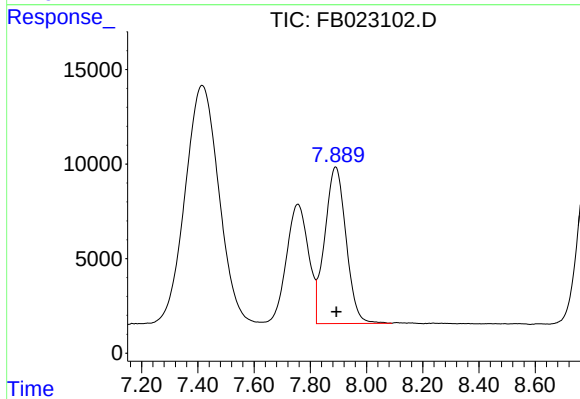


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 435719
Conc: 10.46 ng/ml

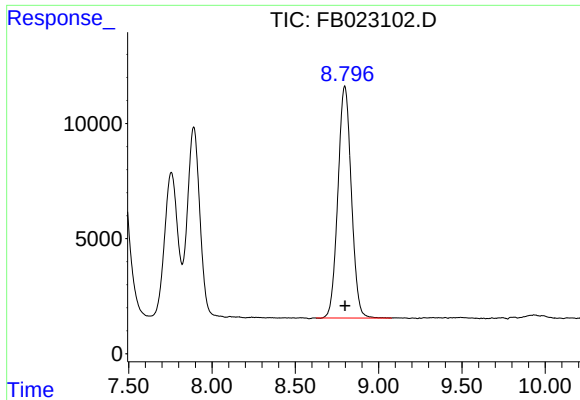


#5 AAA-TFT

R.T.: 8.797 min
 Delta R.T.: -0.002 min
 Response: 564139
 Conc: 22.97 ng/ml

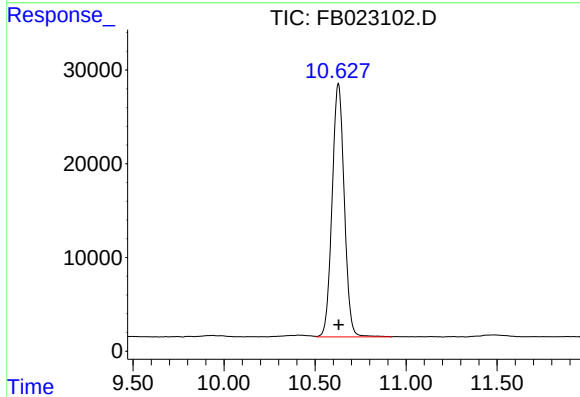


#6 Toluene

R.T.: 10.628 min
 Delta R.T.: -0.002 min
 Response: 1255195
 Conc: 31.16 ng/ml

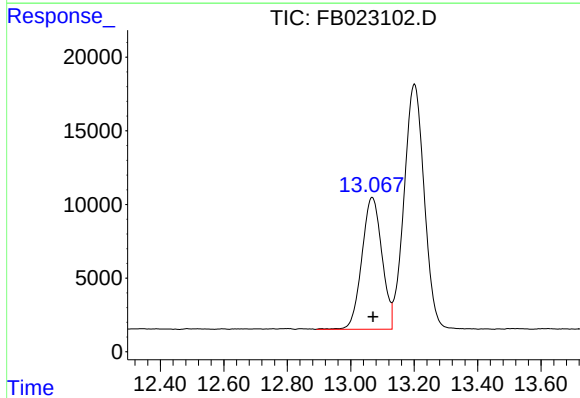


#7 Ethylbenzene

R.T.: 13.068 min
 Delta R.T.: -0.002 min
 Response: 393475
 Conc: 10.20 ng/ml

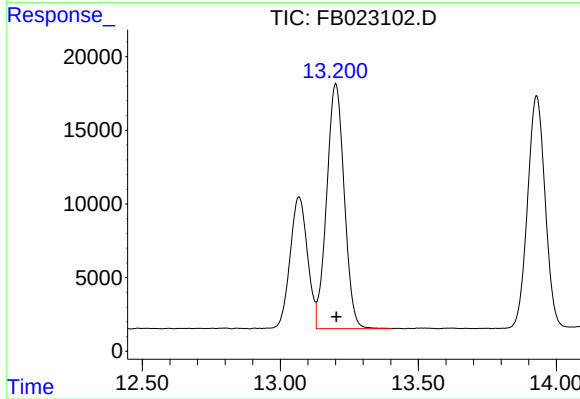


#8 m-Xylene

R.T.: 13.201 min
 Delta R.T.: -0.002 min
 Response: 736249
 Conc: 20.23 ng/ml

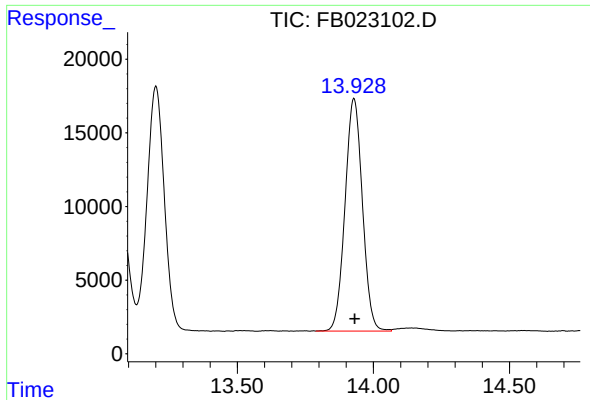

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.003 min
Response: 701740
Conc: 20.21 ng/ml

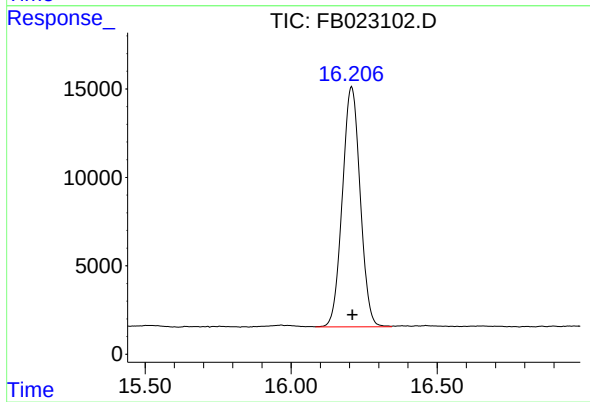

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.003 min
Response: 576096
Conc: 20.54 ng/ml