

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112619\
 Data File : FB023100.D
 Signal(s) : FID2B.CH
 Acq On : 26 Nov 2019 15:35
 Operator : DD/AJ
 Sample : K5670-10MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 27 00:12:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.794	588752	23.968 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.686	979758	29.982 ng/ml
2) t	2,2,4-Trimethylpentane	7.413	1051470	30.153 ng/ml
3) t	n-Heptane	7.753	345320	10.043 ng/ml
4) t	Benzene	7.887	426591	10.239 ng/ml
6) t	Toluene	10.626	1234644	30.649 ng/ml
7) t	Ethylbenzene	13.066	389105	10.084 ng/ml
8) t	m-Xylene	13.199	733971	20.170 ng/ml
9) t	O-Xylene	13.927	696186	20.051 ng/ml
10) t	1,2,4-Trimethylbenzene	16.205	559535	19.952 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112619\
Data File : FB023100.D
Signal(s) : FID2B.CH
Acq On : 26 Nov 2019 15:35
Operator : DD/AJ
Sample : K5670-10MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 27 00:12:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

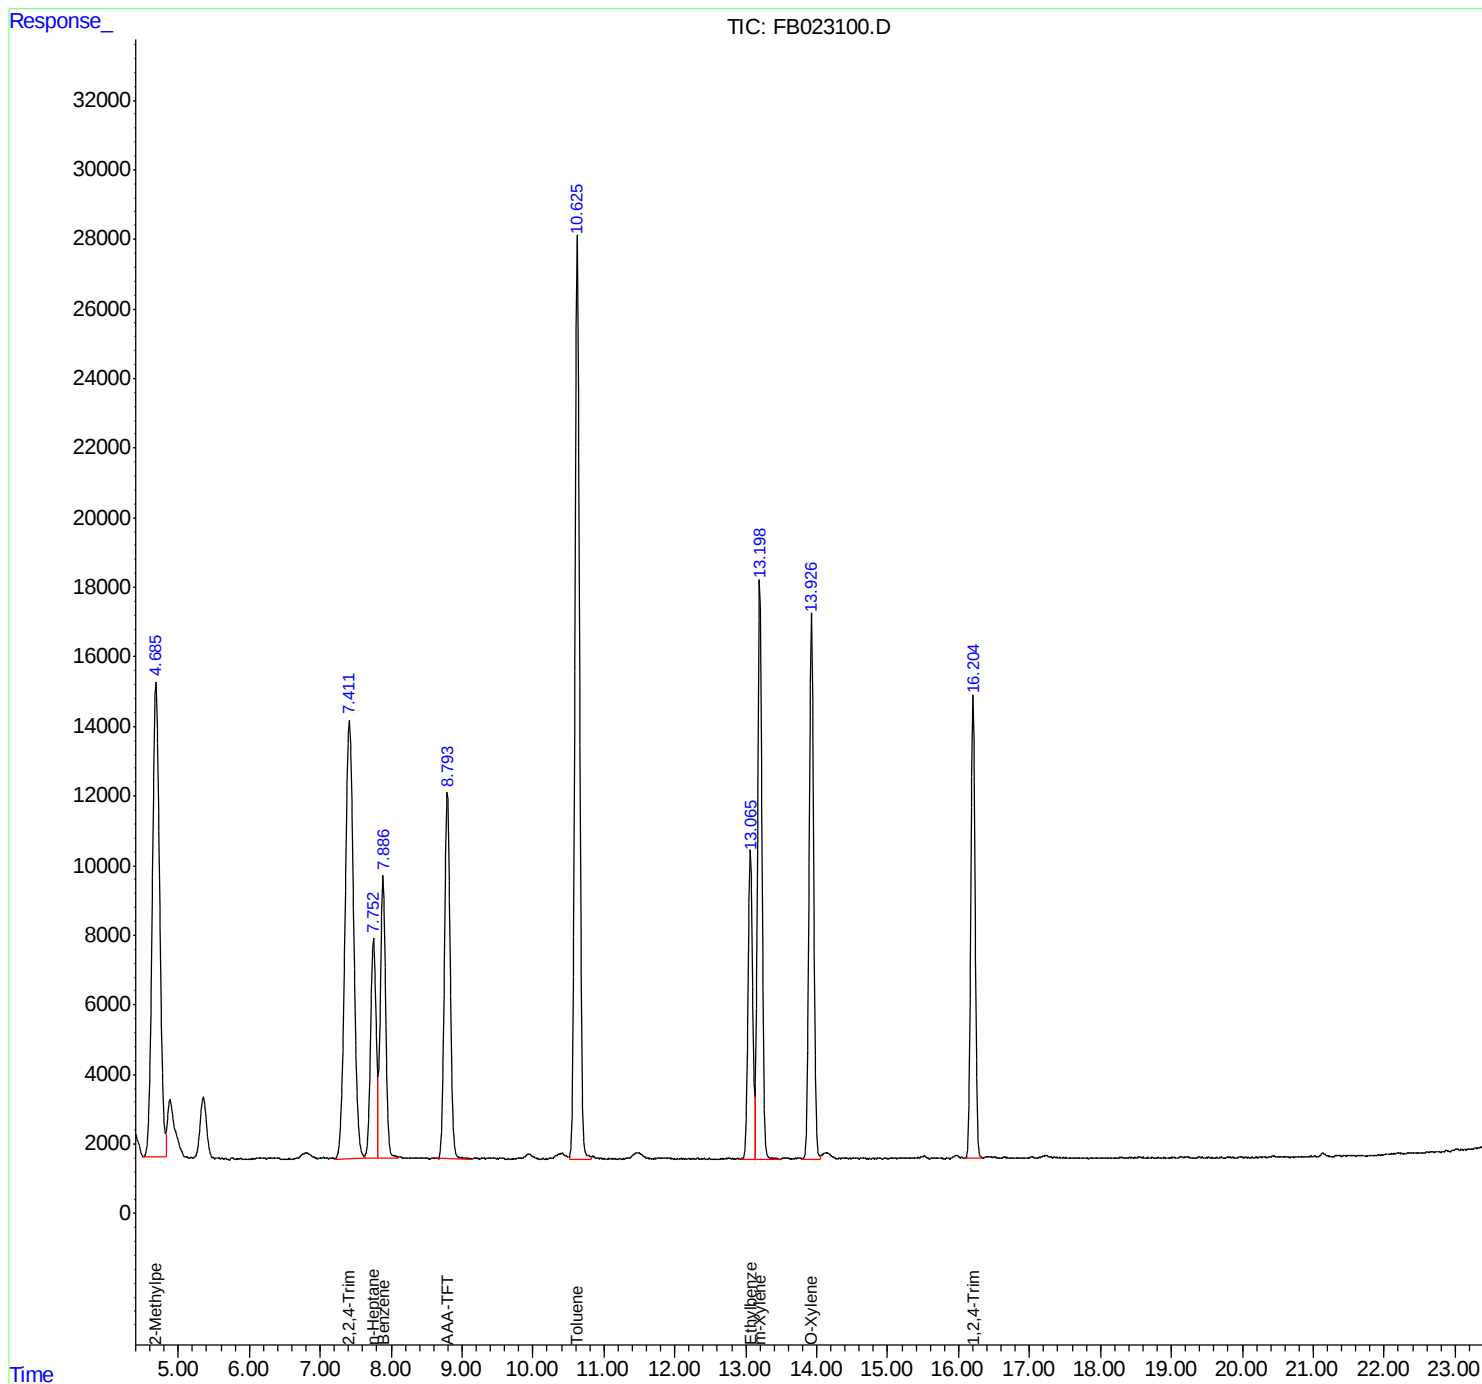

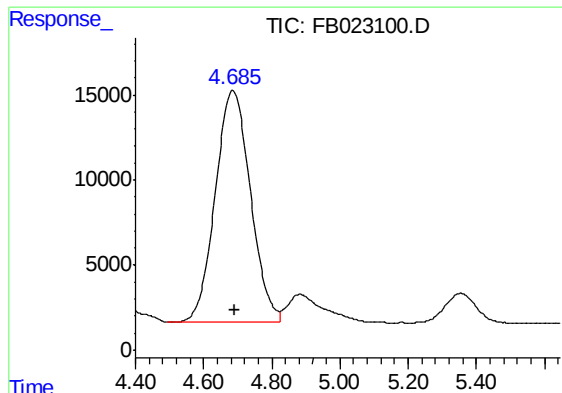


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.005 min
Response: 979758
Conc: 29.98 ng/ml

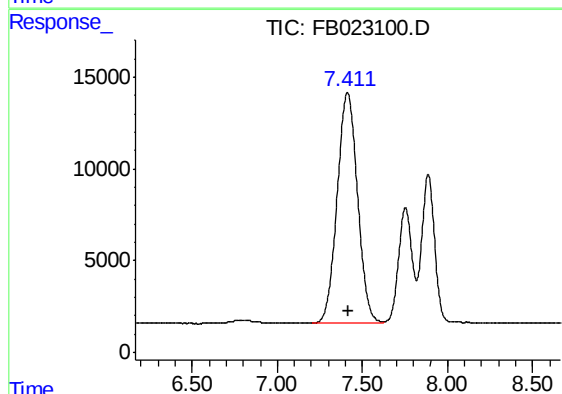


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.005 min
Response: 1051470
Conc: 30.15 ng/ml

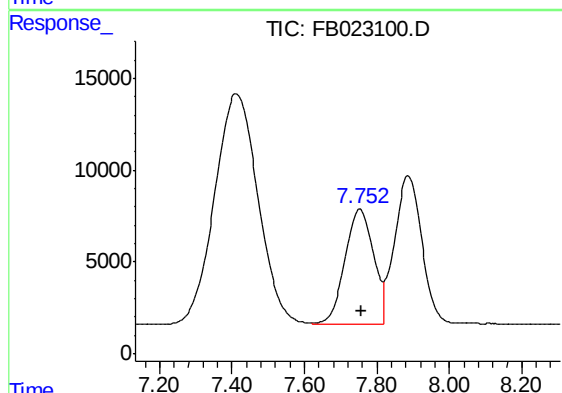


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 345320
Conc: 10.04 ng/ml

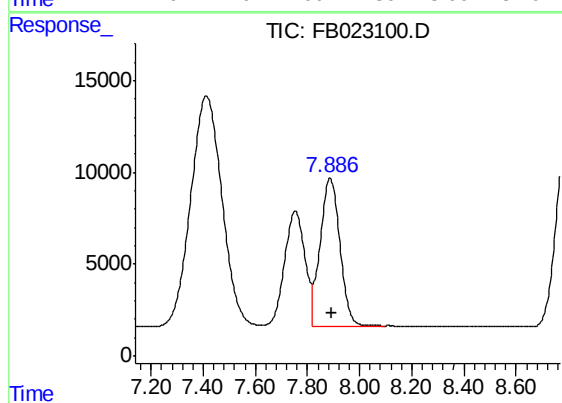


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.005 min
Response: 426591
Conc: 10.24 ng/ml

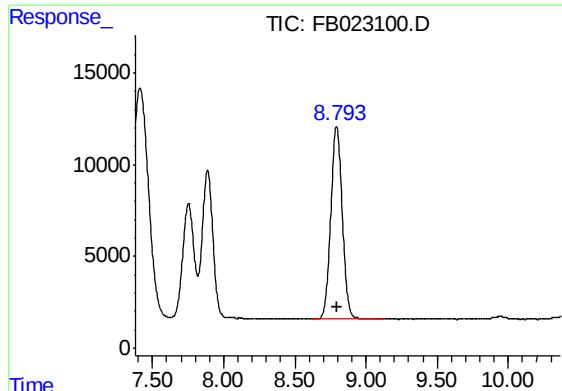


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.005 min
Response: 588752
Conc: 23.97 ng/ml

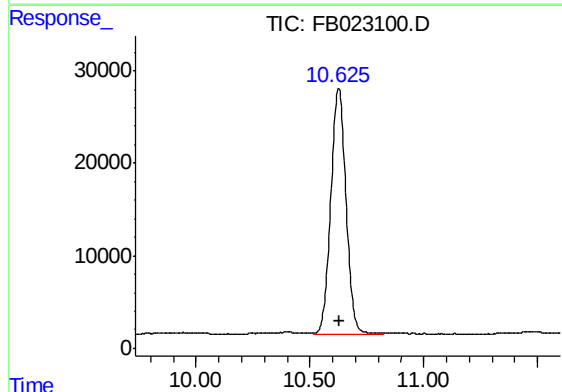


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.005 min
Response: 1234644
Conc: 30.65 ng/ml

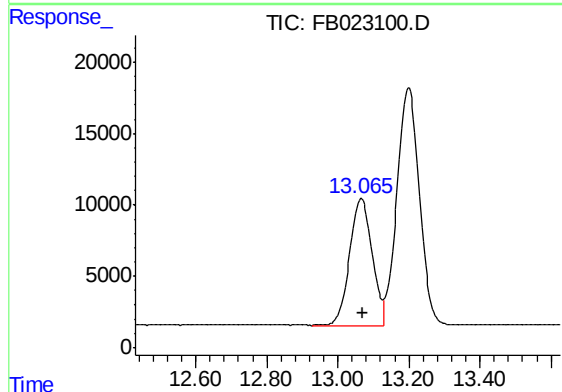


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.004 min
Response: 389105
Conc: 10.08 ng/ml

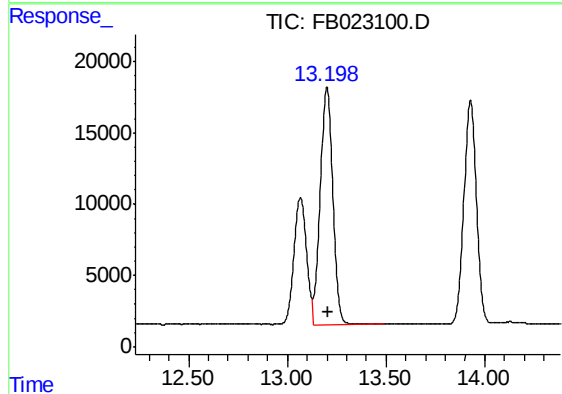


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.004 min
Response: 733971
Conc: 20.17 ng/ml

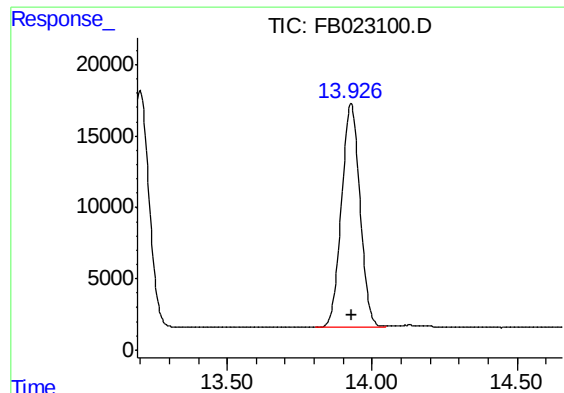

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.004 min
Response: 696186
Conc: 20.05 ng/ml

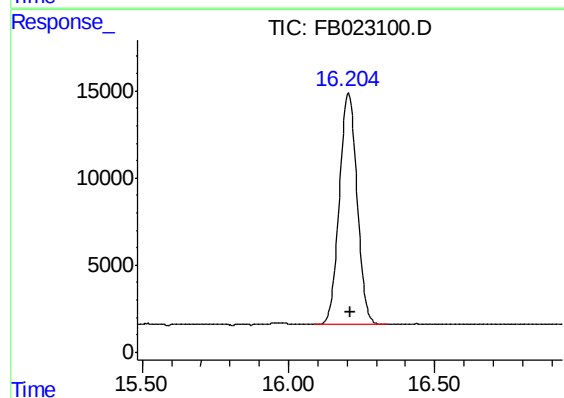

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.005 min
Response: 559535
Conc: 19.95 ng/ml