

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112624\
Data File : FB031266.D
Signal(s) : FID2B.CH
Acq On : 26 Nov 2024 11:04
Operator : YP/AJ
Sample : VBF1126S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 27 00:12:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
Quant Title :
QLast Update : Thu Nov 21 12:34:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	493483	17.532 ng/ml
Target Compounds			
6) t Toluene	10.616	1784	0.036 ng/ml
8) t m-Xylene	13.197	3060	0.065 ng/ml
9) t O-Xylene	13.928	9393	0.216 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	15264	0.428 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112624\
Data File : FB031266.D
Signal(s) : FID2B.CH
Acq On : 26 Nov 2024 11:04
Operator : YP/AJ
Sample : VBF1126S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 27 00:12:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
Quant Title :
QLast Update : Thu Nov 21 12:34:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

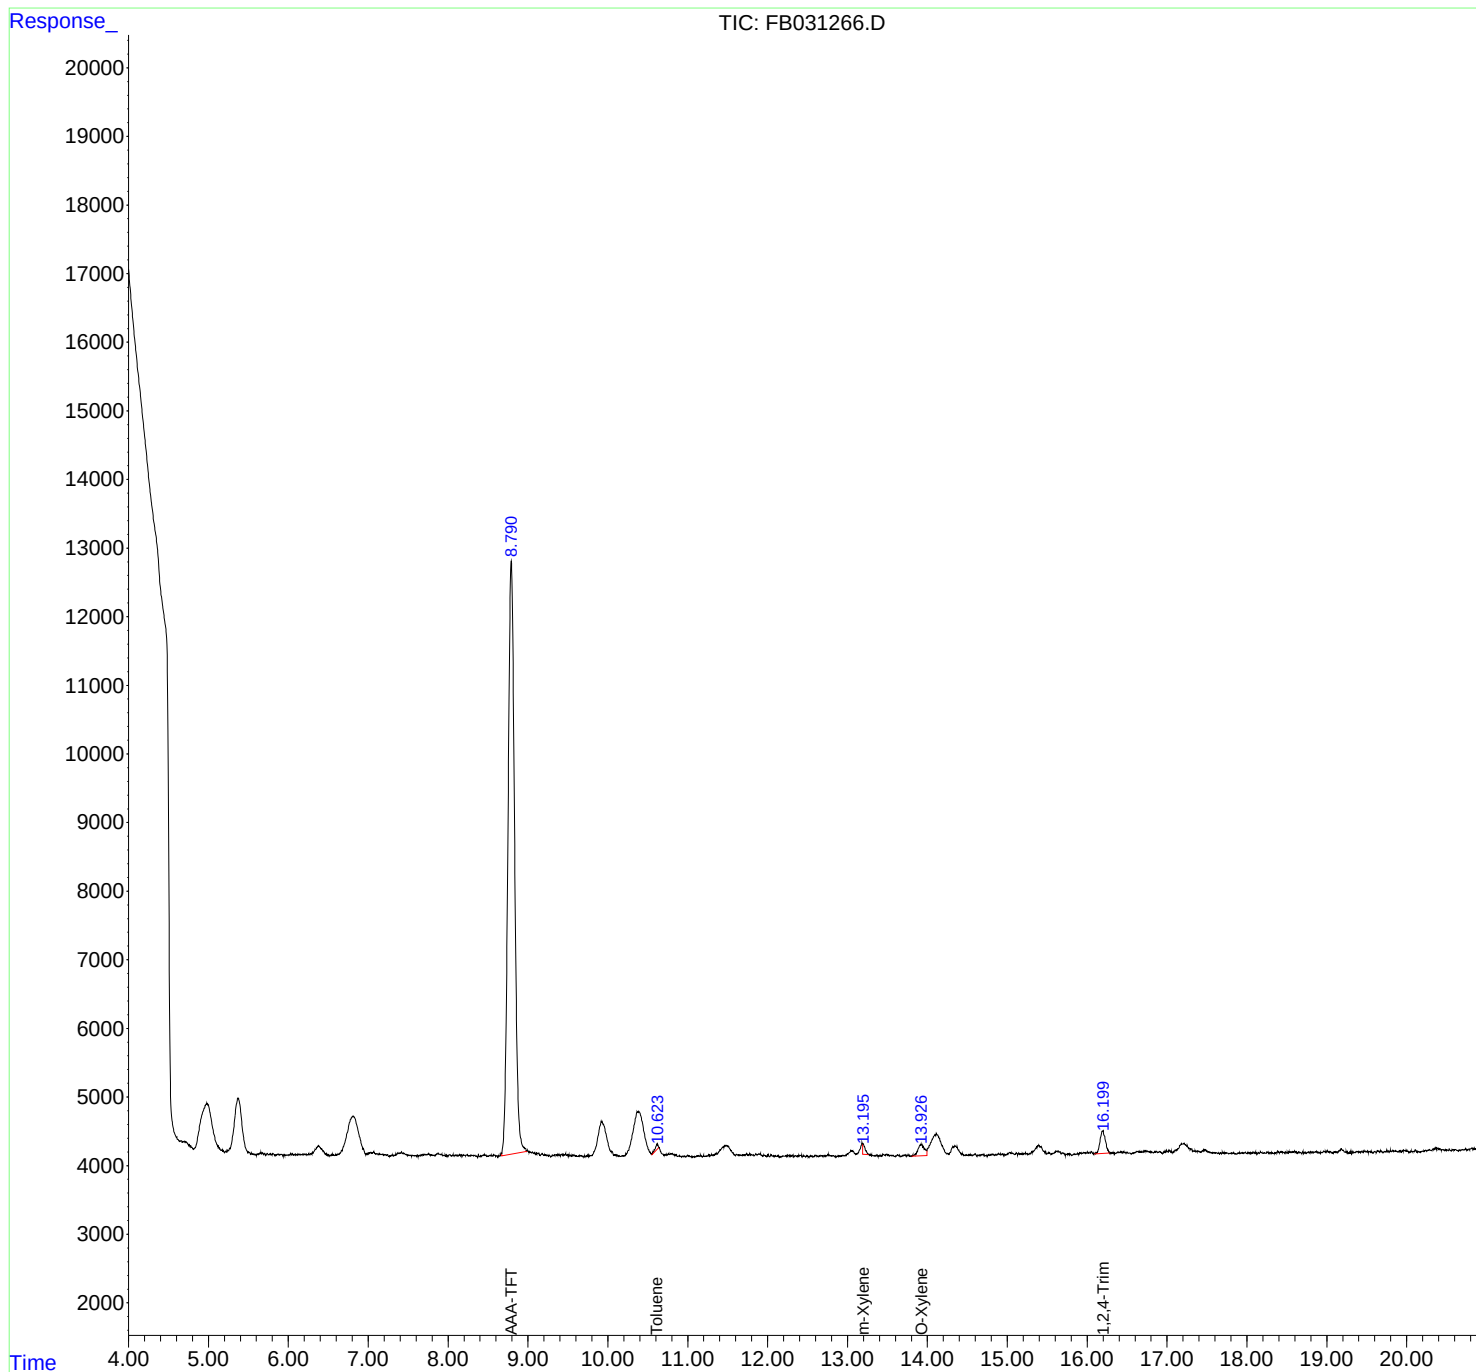


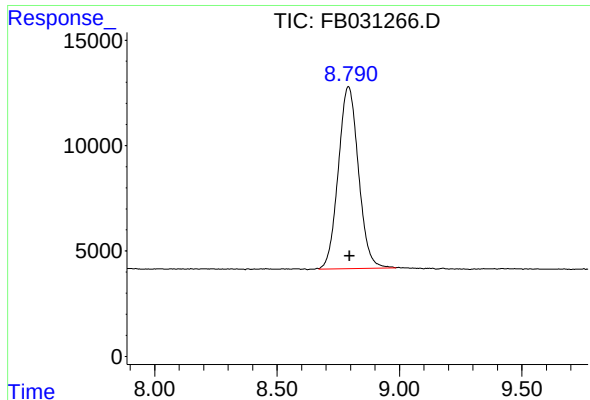

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.005 min
Response: 493483
Conc: 17.53 ng/ml

Instrument :
FID_B
ClientSampleId :

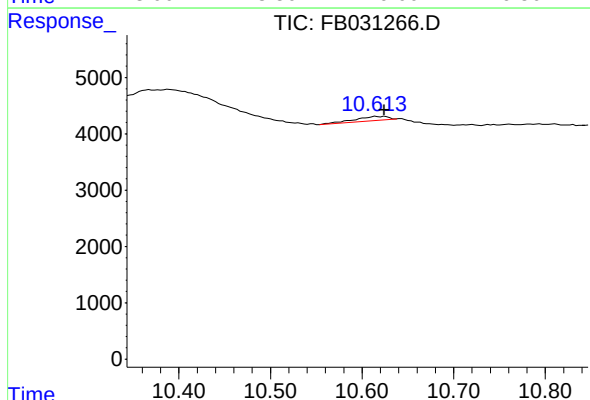


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.009 min
Response: 1784
Conc: 0.04 ng/ml

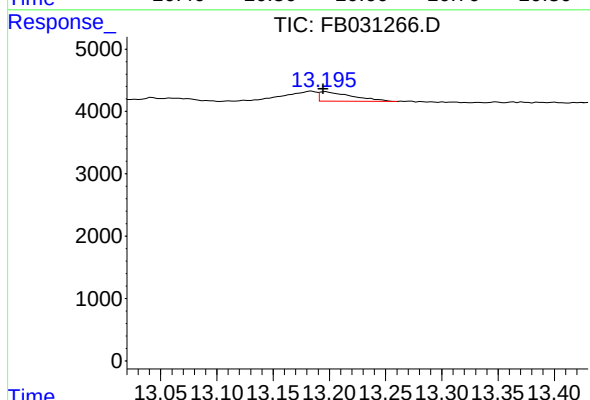


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: 0.002 min
Response: 3060
Conc: 0.06 ng/ml

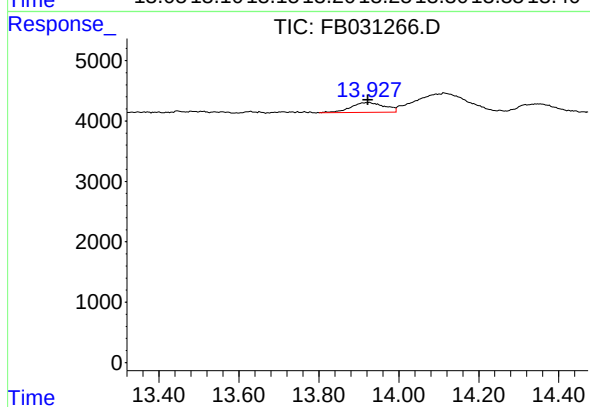

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.005 min
Response: 9393
Conc: 0.22 ng/ml

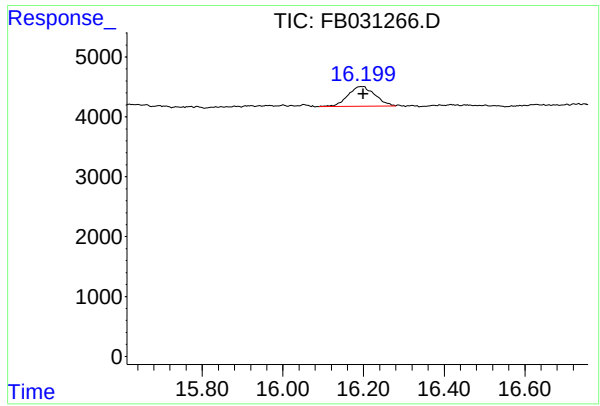

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.002 min
Response: 15264
Conc: 0.43 ng/ml

Instrument :

FID_B

ClientSampleId :