

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112624\
 Data File : FB031268.D
 Signal(s) : FID2B.CH
 Acq On : 26 Nov 2024 11:57
 Operator : YP/AJ
 Sample : BSF1126S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1126S1

Integration File: SAMPLE.e
 Quant Time: Nov 27 00:12:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
 Quant Title :
 QLast Update : Thu Nov 21 12:34:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	467578	16.612 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	1205138	30.558 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	1403899	29.688 ng/ml
3) t n-Heptane	7.755	448588	9.605 ng/ml
4) t Benzene	7.893	531087	9.799 ng/ml
6) t Toluene	10.622	1473933	29.474 ng/ml
7) t Ethylbenzene	13.058	425160	9.691 ng/ml
8) t m-Xylene	13.191	909202	19.284 ng/ml
9) t O-Xylene	13.919	846905	19.445 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	681262	19.085 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112624\
Data File : FB031268.D
Signal(s) : FID2B.CH
Acq On : 26 Nov 2024 11:57
Operator : YP/AJ
Sample : BSF1126S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1126S1

Integration File: SAMPLE.e
Quant Time: Nov 27 00:12:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
Quant Title :
QLast Update : Thu Nov 21 12:34:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

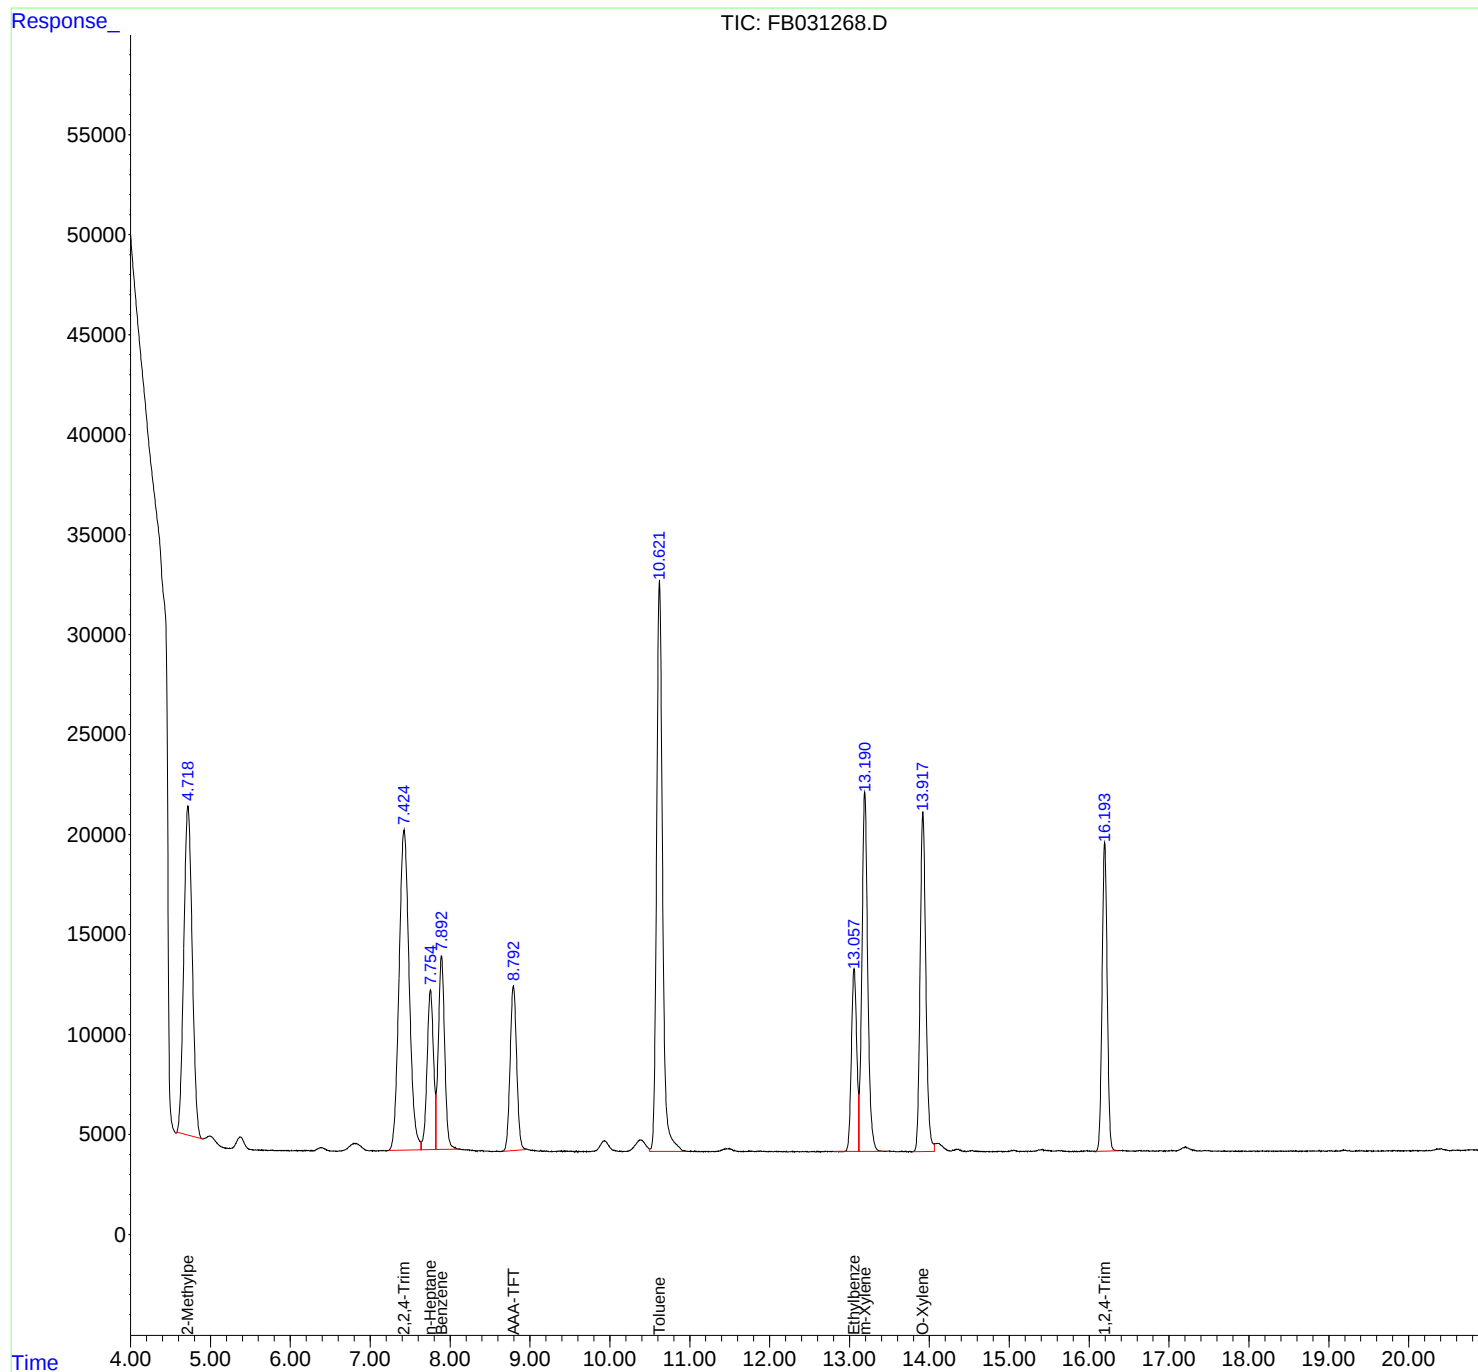


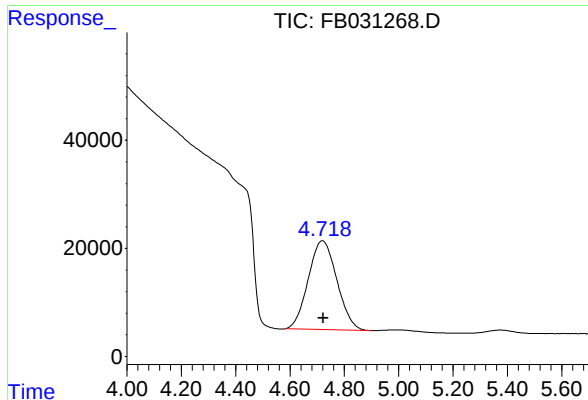

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: -0.003 min
Response: 1205138
Conc: 30.56 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1126S1

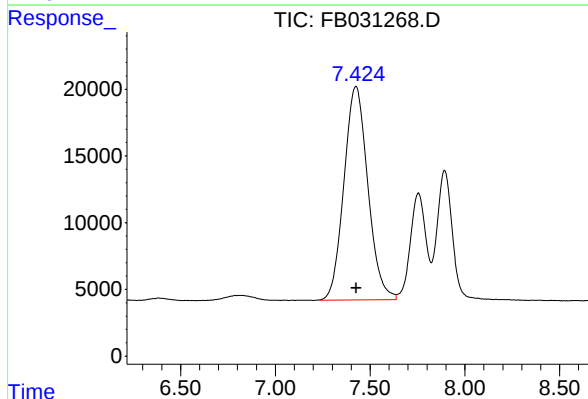


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.002 min
Response: 1403899
Conc: 29.69 ng/ml

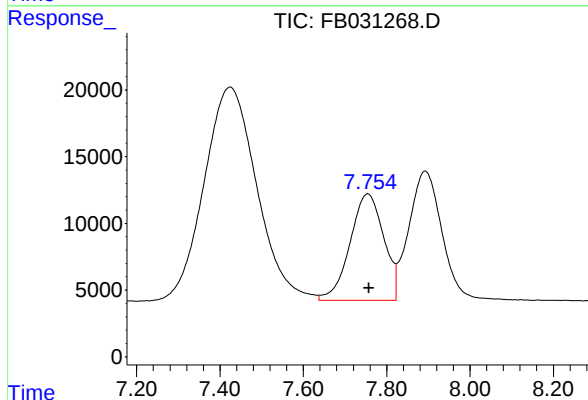


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.002 min
Response: 448588
Conc: 9.61 ng/ml

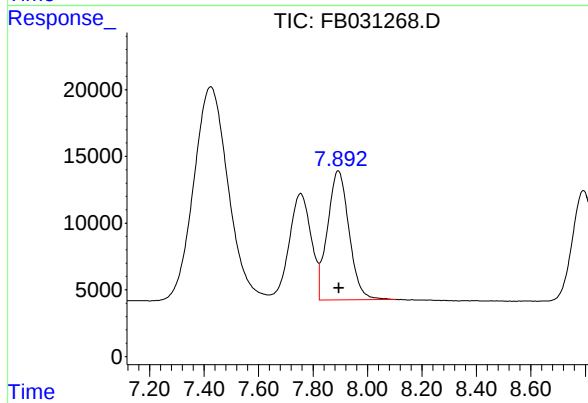

#4 Benzene


R.T.: 7.893 min
Delta R.T.: -0.002 min
Response: 531087
Conc: 9.80 ng/ml

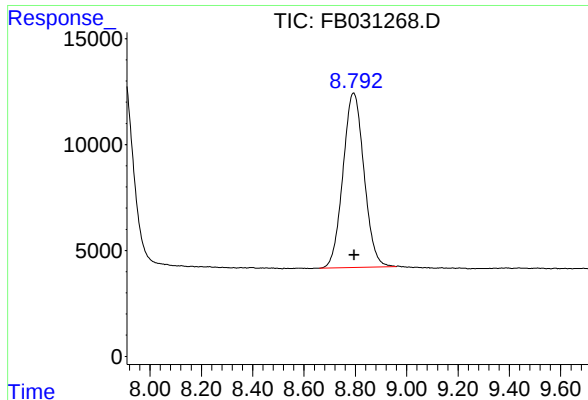

#5 AAA-TFT


R.T.: 8.793 min
 Delta R.T.: -0.003 min
 Response: 467578
 Conc: 16.61 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 BSF1126S1

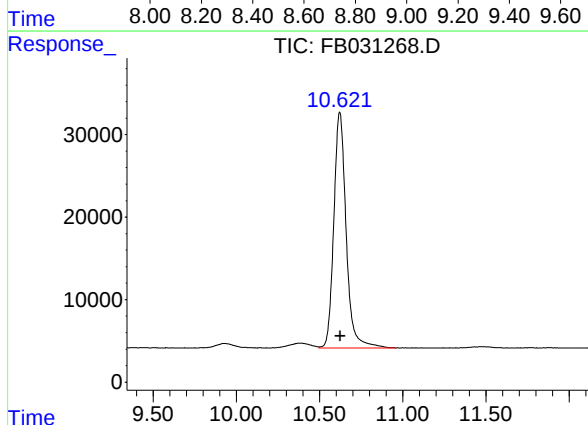


#6 Toluene

R.T.: 10.622 min
 Delta R.T.: -0.002 min
 Response: 1473933
 Conc: 29.47 ng/ml

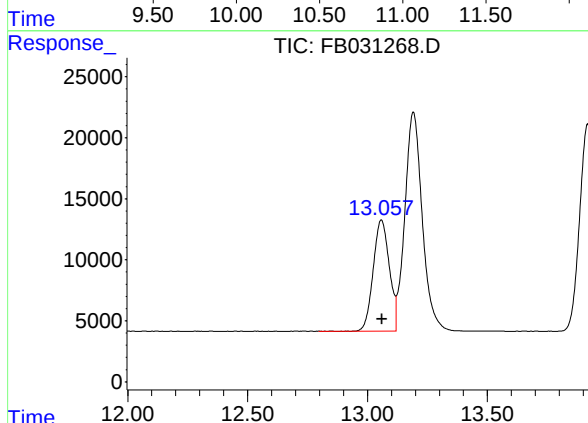


#7 Ethylbenzene

R.T.: 13.058 min
 Delta R.T.: -0.003 min
 Response: 425160
 Conc: 9.69 ng/ml

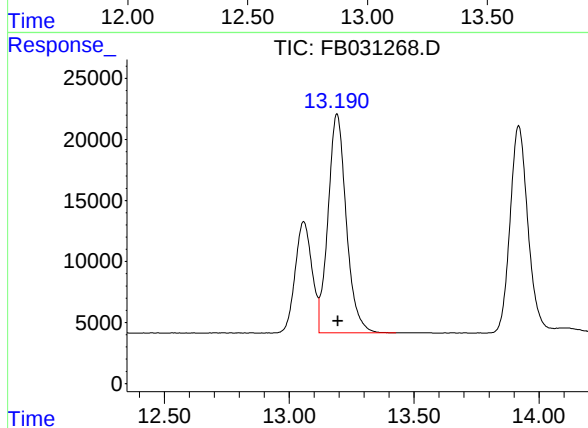

#8 m-Xylene


R.T.: 13.191 min
 Delta R.T.: -0.003 min
 Response: 909202
 Conc: 19.28 ng/ml

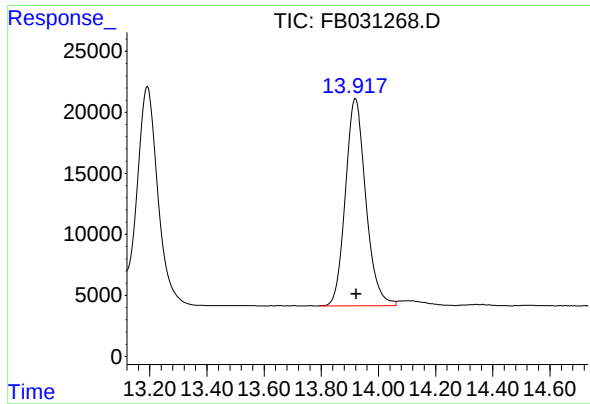

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.004 min
Response: 846905
Conc: 19.44 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1126S1

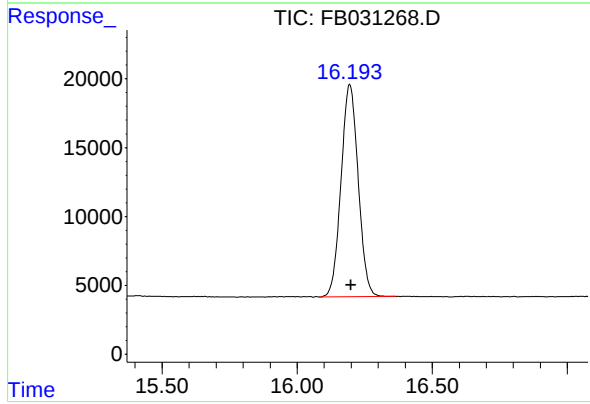

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.004 min
Response: 681262
Conc: 19.08 ng/ml