

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112624\
 Data File : FB031272.D
 Signal(s) : FID2B.CH
 Acq On : 26 Nov 2024 14:28
 Operator : YP/AJ
 Sample : BSF1126S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1126S2

Integration File: SAMPLE.e
 Quant Time: Nov 27 00:13:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
 Quant Title :
 QLast Update : Thu Nov 21 12:34:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	572096	20.325 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.722	1258838	31.920 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	1461004	30.896 ng/ml
3) t n-Heptane	7.757	478198	10.239 ng/ml
4) t Benzene	7.896	555252	10.245 ng/ml
6) t Toluene	10.624	1534686	30.689 ng/ml
7) t Ethylbenzene	13.060	440424	10.039 ng/ml
8) t m-Xylene	13.194	943213	20.006 ng/ml
9) t O-Xylene	13.922	877871	20.156 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	694321	19.451 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112624\
Data File : FB031272.D
Signal(s) : FID2B.CH
Acq On : 26 Nov 2024 14:28
Operator : YP/AJ
Sample : BSF1126S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1126S2

Integration File: SAMPLE.e
Quant Time: Nov 27 00:13:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
Quant Title :
QLast Update : Thu Nov 21 12:34:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

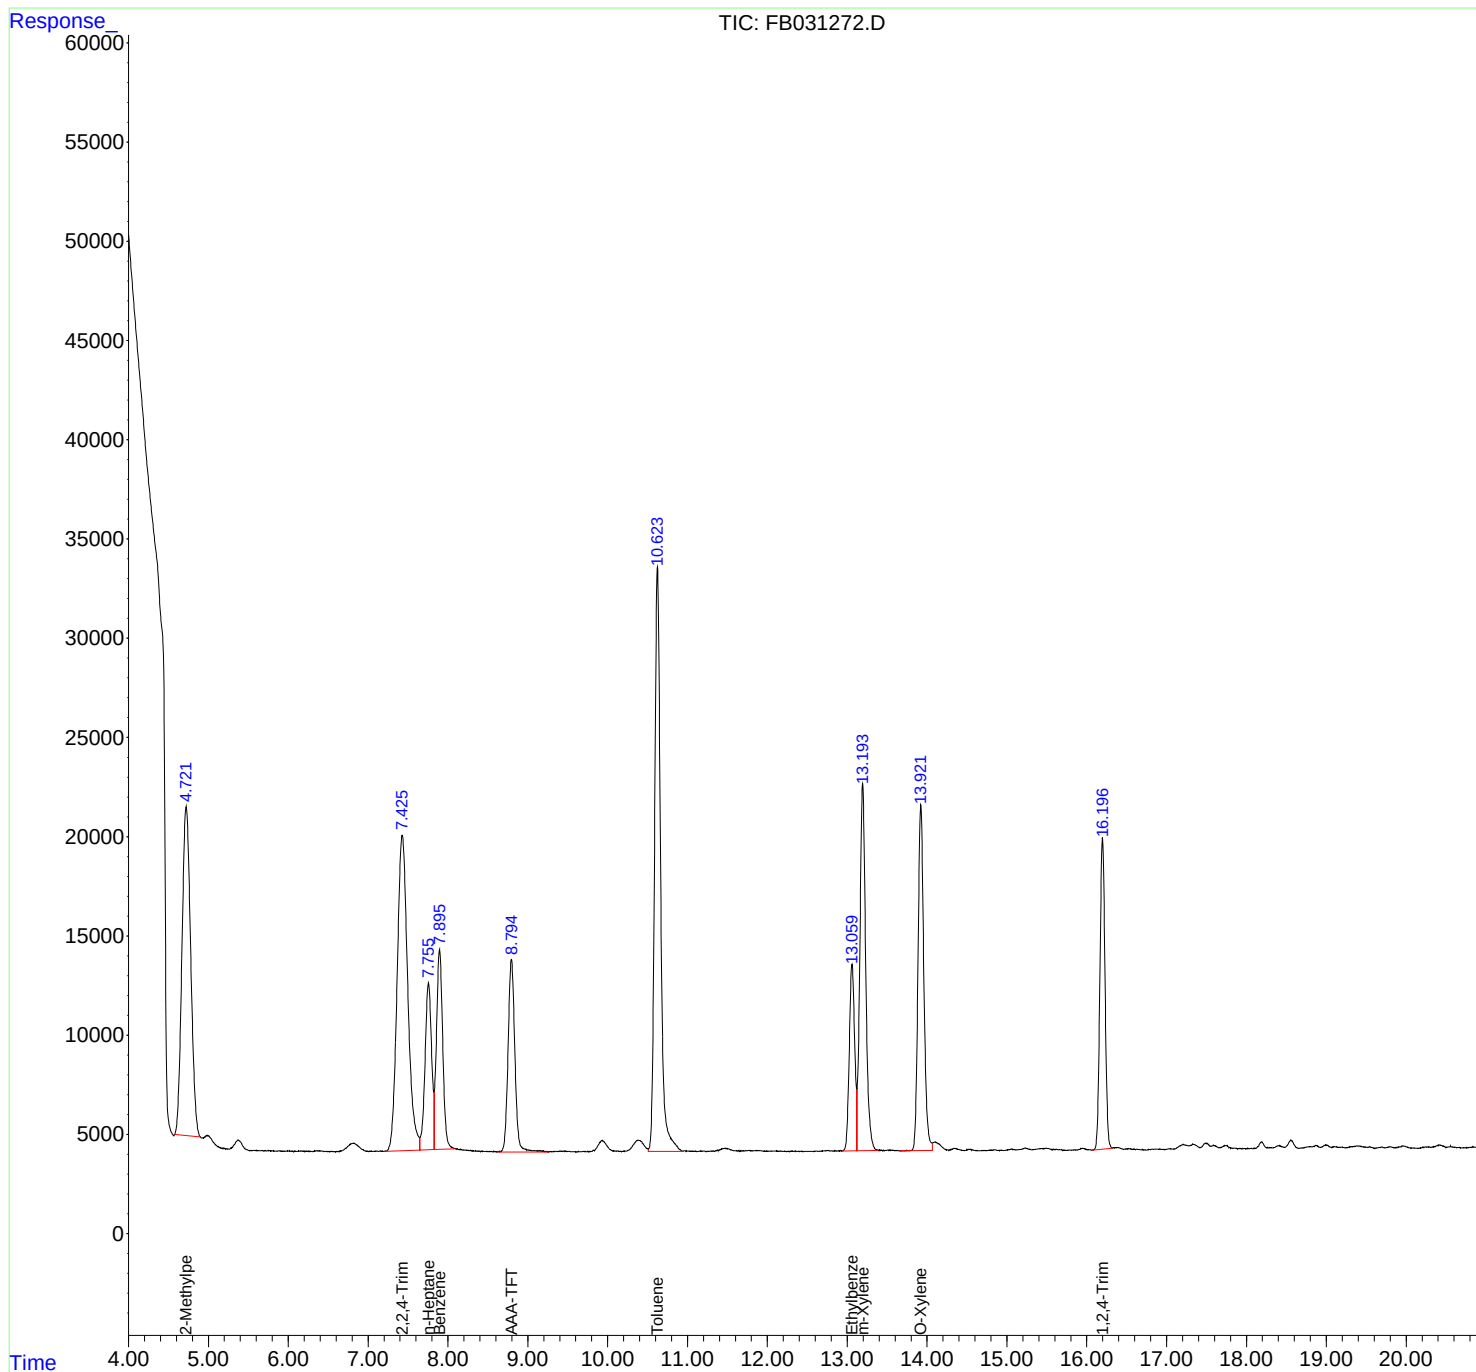


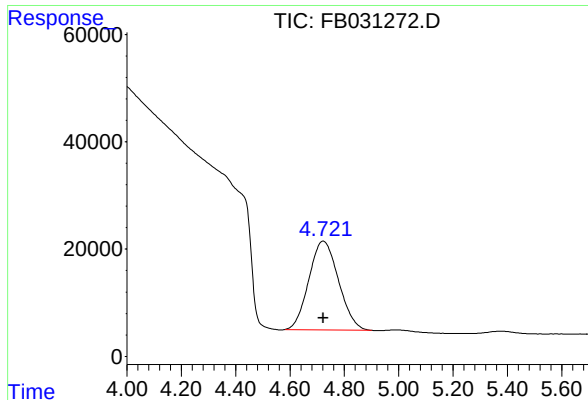

#1 2-Methylpentane


R.T.: 4.722 min
Delta R.T.: 0.000 min
Response: 1258838
Conc: 31.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1126S2

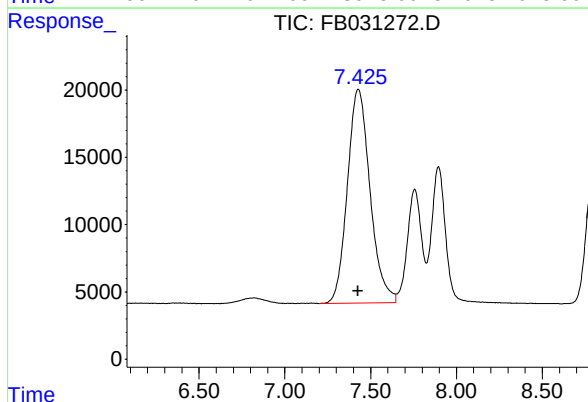


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.000 min
Response: 1461004
Conc: 30.90 ng/ml

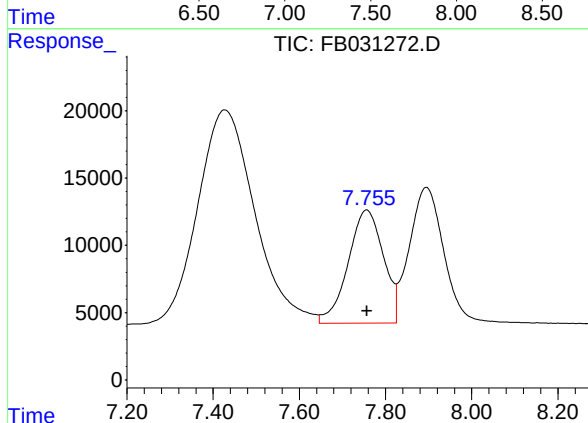


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 478198
Conc: 10.24 ng/ml

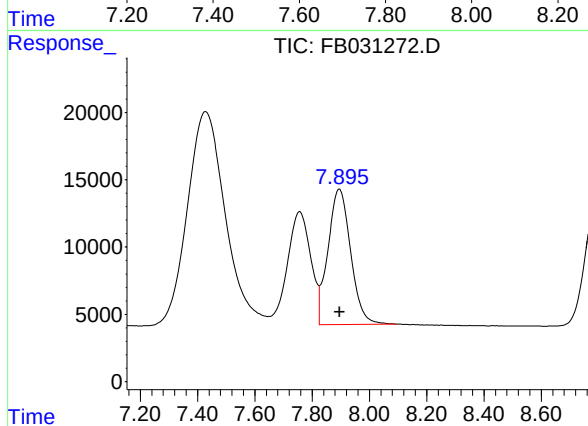

#4 Benzene


R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 555252
Conc: 10.24 ng/ml

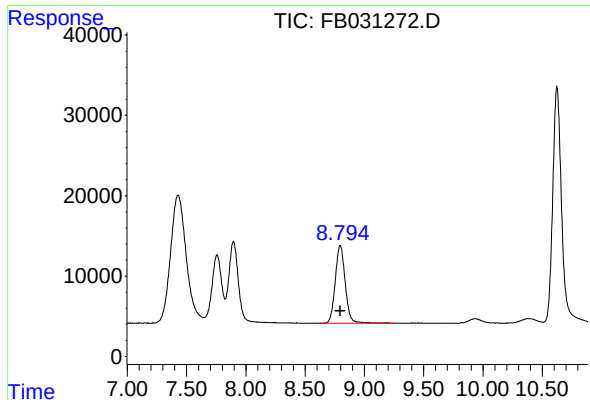

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 572096
Conc: 20.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1126S2

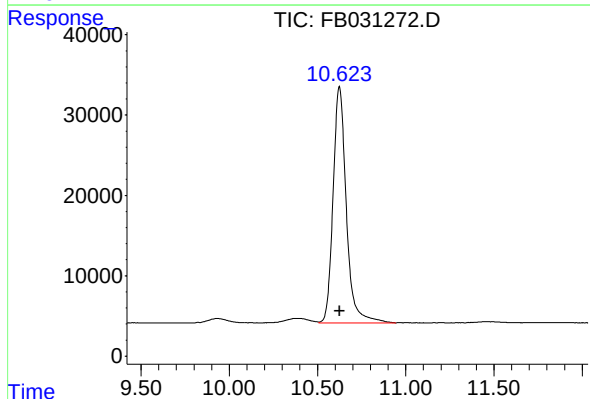


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.000 min
Response: 1534686
Conc: 30.69 ng/ml

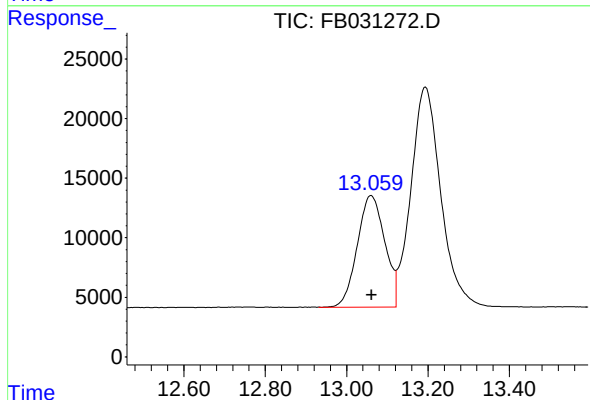


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.001 min
Response: 440424
Conc: 10.04 ng/ml

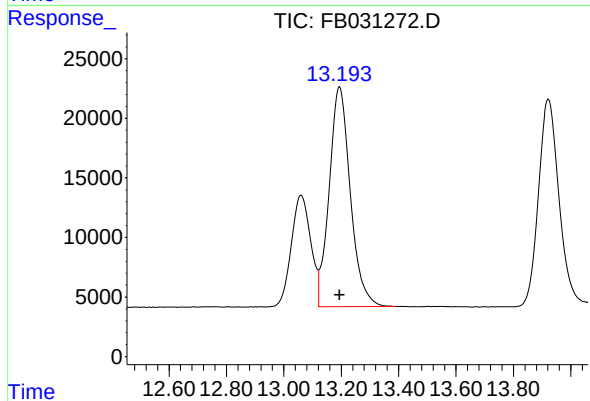

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.000 min
Response: 943213
Conc: 20.01 ng/ml

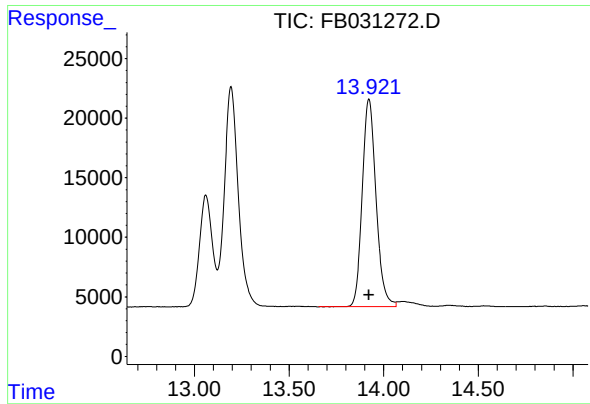

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.000 min
Response: 877871
Conc: 20.16 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1126S2

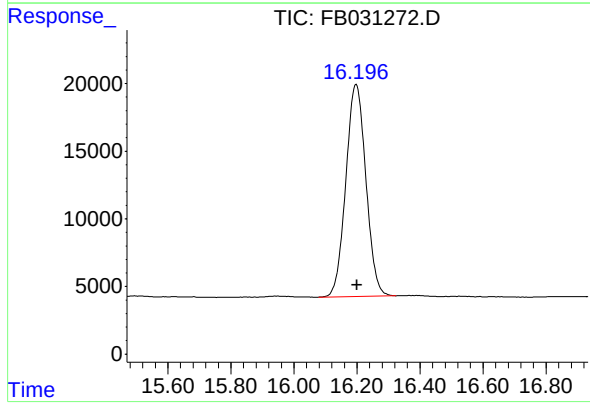

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.002 min
Response: 694321
Conc: 19.45 ng/ml