

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112719\
 Data File : FB023110.D
 Signal(s) : FID2B.CH
 Acq On : 27 Nov 2019 12:14
 Operator : DD/AJ
 Sample : BSF1127S1
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 27 21:50:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.794	523486	21.311 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.684	972771	29.768 ng/ml
2) t	2,2,4-Trimethylpentane	7.412	1084981	31.114 ng/ml
3) t	n-Heptane	7.752	358318	10.421 ng/ml
4) t	Benzene	7.887	429312	10.304 ng/ml
6) t	Toluene	10.626	1254641	31.145 ng/ml
7) t	Ethylbenzene	13.066	402310	10.426 ng/ml
8) t	m-Xylene	13.200	766183	21.055 ng/ml
9) t	O-Xylene	13.927	729295	21.005 ng/ml
10) t	1,2,4-Trimethylbenzene	16.206	614994	21.930 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112719\
Data File : FB023110.D
Signal(s) : FID2B.CH
Acq On : 27 Nov 2019 12:14
Operator : DD/AJ
Sample : BSF1127S1
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 27 21:50:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

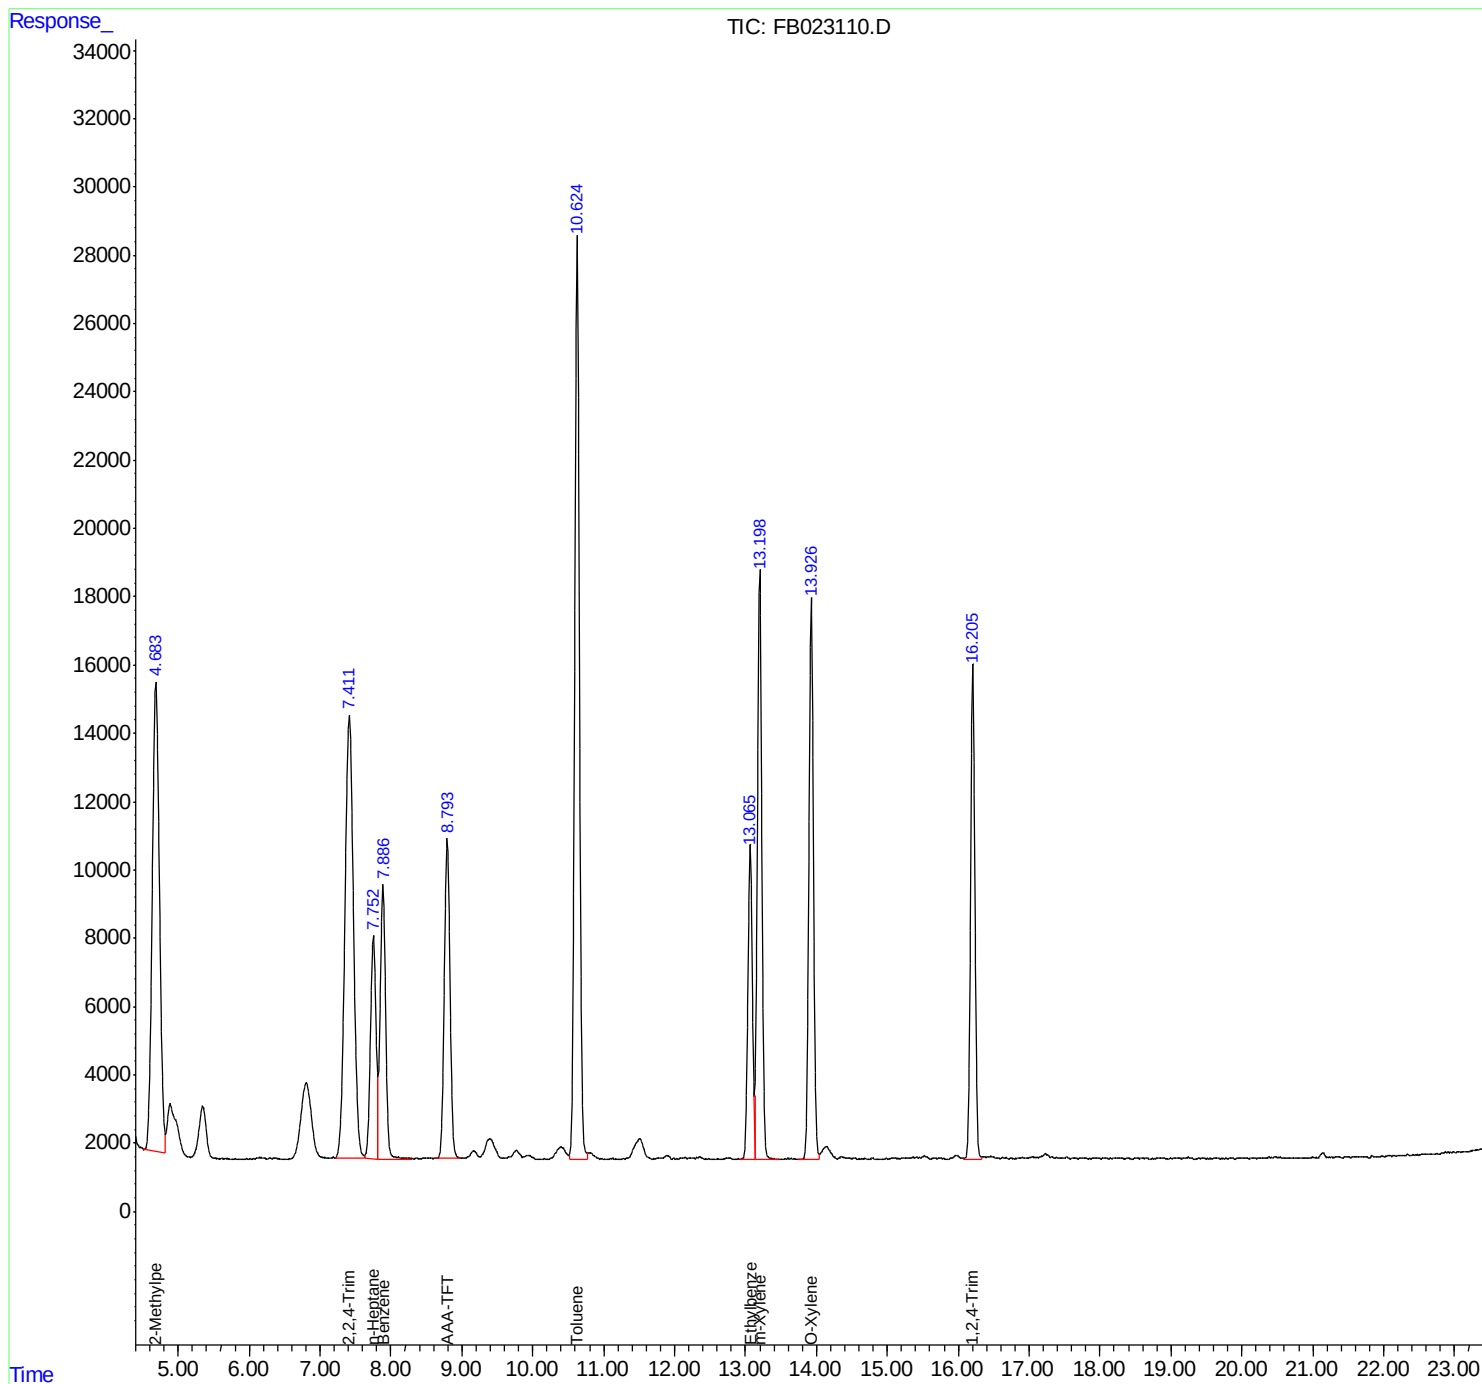

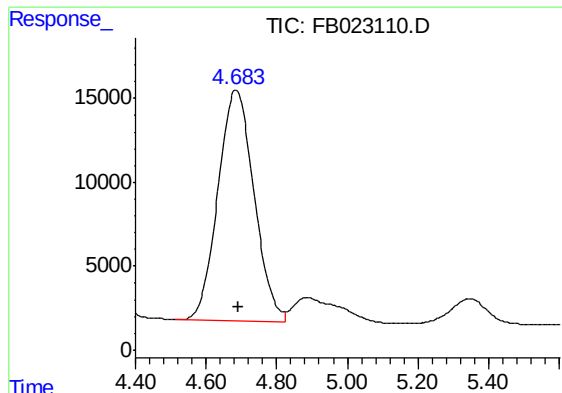


#1 2-Methylpentane

R.T.: 4.684 min
Delta R.T.: -0.007 min
Response: 972771
Conc: 29.77 ng/ml

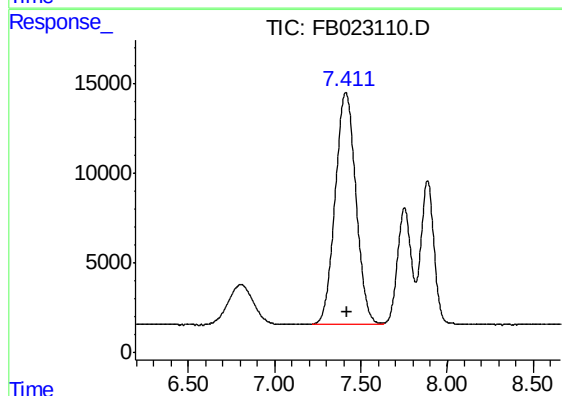


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.006 min
Response: 1084981
Conc: 31.11 ng/ml

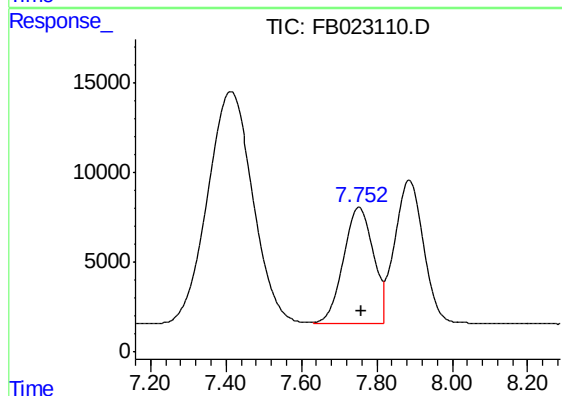


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.005 min
Response: 358318
Conc: 10.42 ng/ml

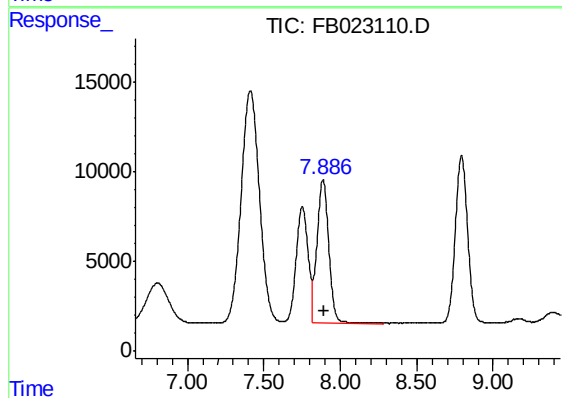


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.005 min
Response: 429312
Conc: 10.30 ng/ml

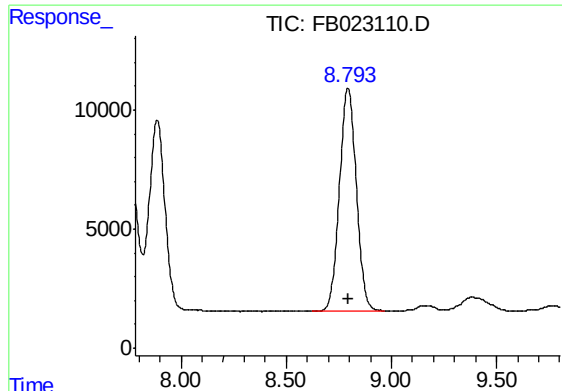


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.005 min
Response: 523486
Conc: 21.31 ng/ml

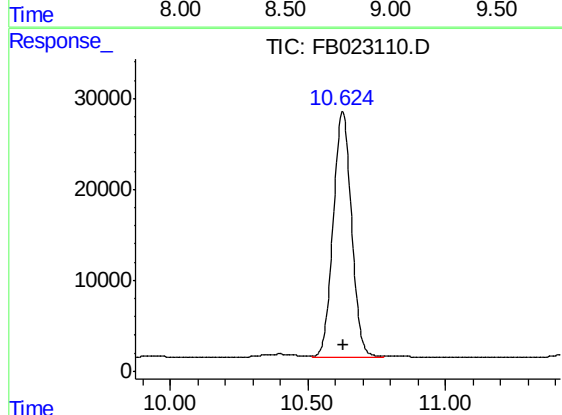


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.005 min
Response: 1254641
Conc: 31.15 ng/ml

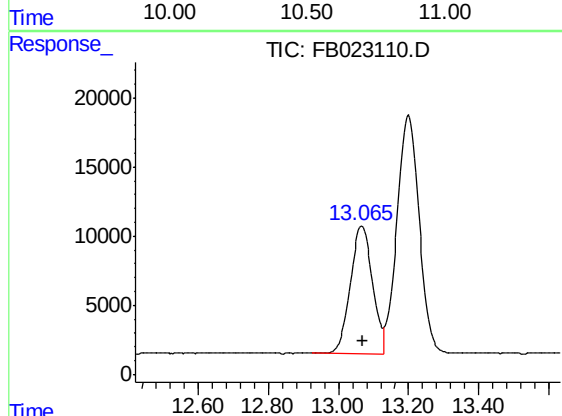


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.004 min
Response: 402310
Conc: 10.43 ng/ml

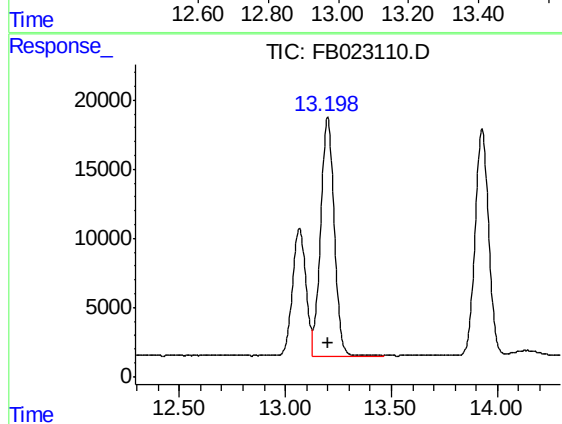


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.004 min
Response: 766183
Conc: 21.05 ng/ml

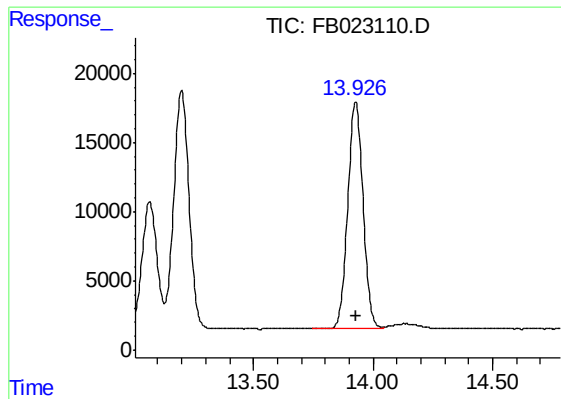

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.004 min
Response: 729295
Conc: 21.00 ng/ml

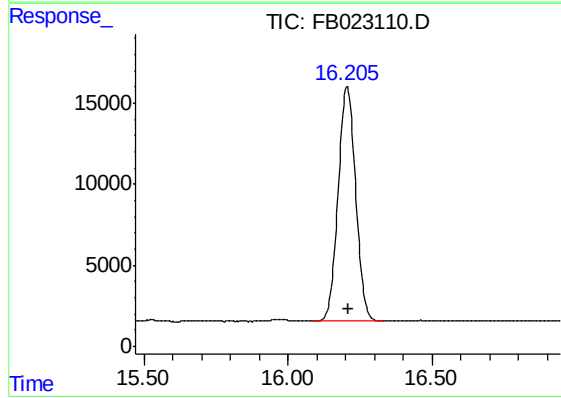

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.004 min
Response: 614994
Conc: 21.93 ng/ml