

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112720\
 Data File : FB025293.D
 Signal(s) : FID2B.CH
 Acq On : 27 Nov 2020 13:21
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 27 22:59:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	457724	20.272 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	987717	30.601 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	1065422	32.112 ng/ml
3) t n-Heptane	7.758	343812	10.468 ng/ml
4) t Benzene	7.892	424629	10.680 ng/ml
6) t Toluene	10.630	1203572	32.189 ng/ml
7) t Ethylbenzene	13.071	362297	10.550 ng/ml
8) t m-Xylene	13.203	729326	21.600 ng/ml
9) t O-Xylene	13.931	708174	21.659 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	619572	22.518 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112720\
Data File : FB025293.D
Signal(s) : FID2B.CH
Acq On : 27 Nov 2020 13:21
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 27 22:59:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

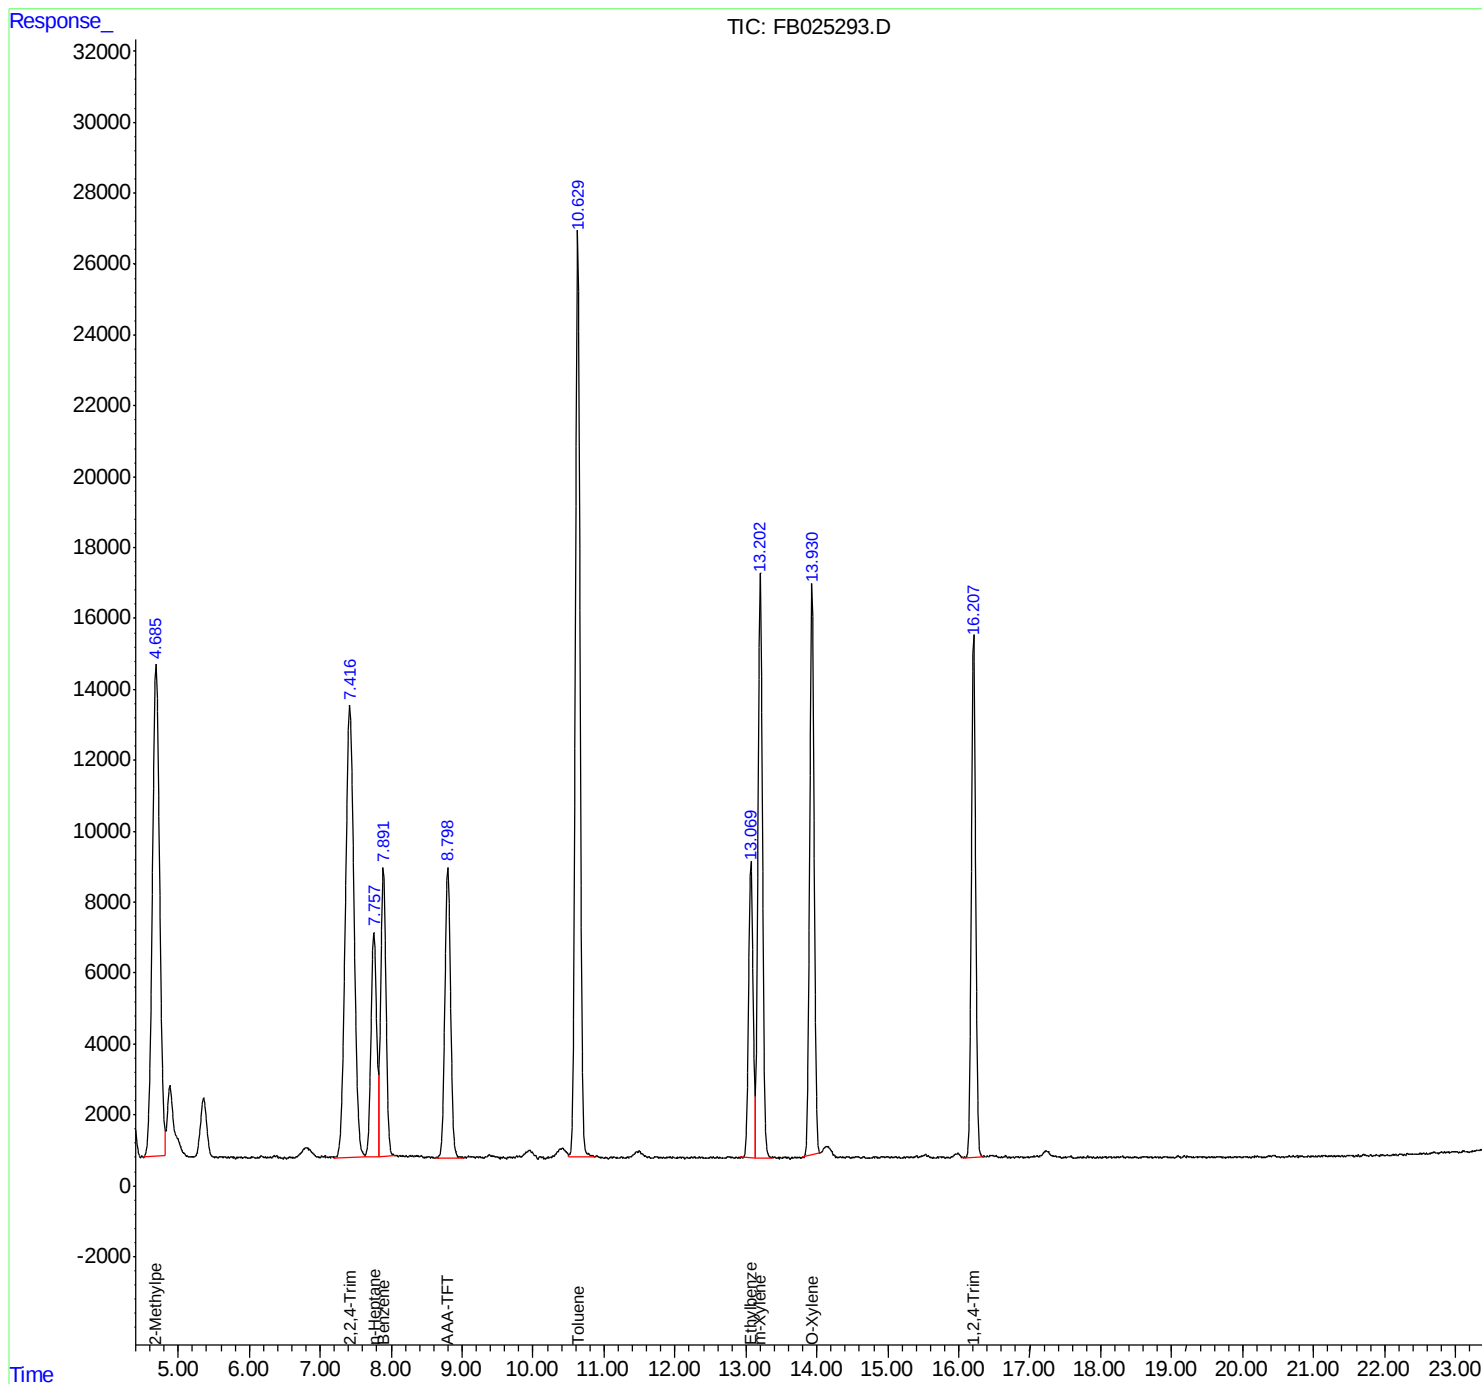

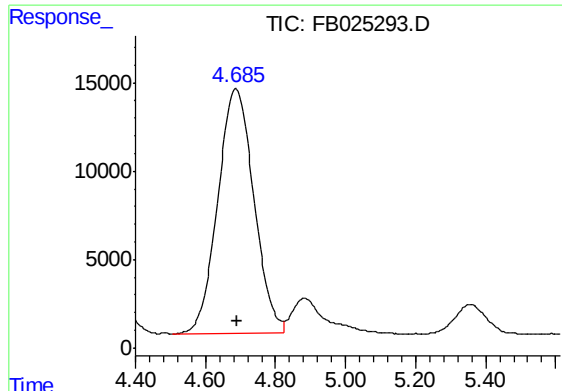


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 987717
Conc: 30.60 ng/ml

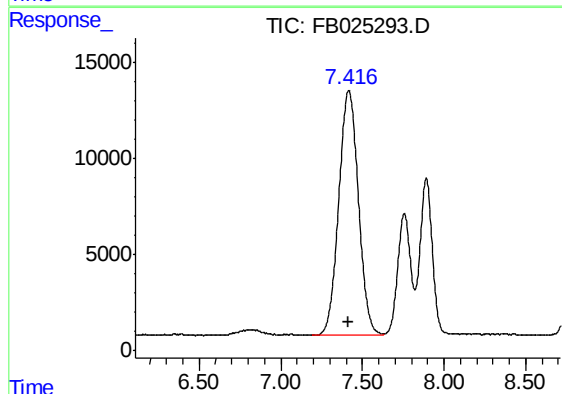


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.001 min
Response: 1065422
Conc: 32.11 ng/ml

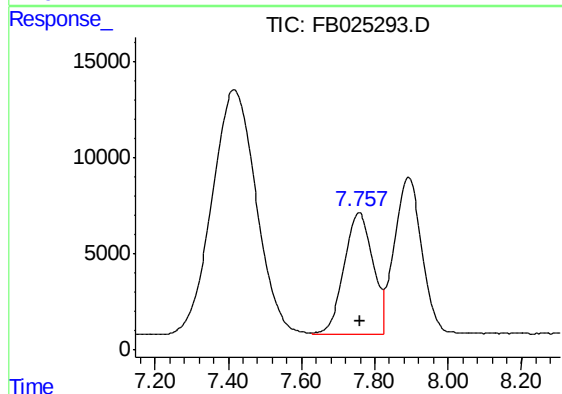


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 343812
Conc: 10.47 ng/ml

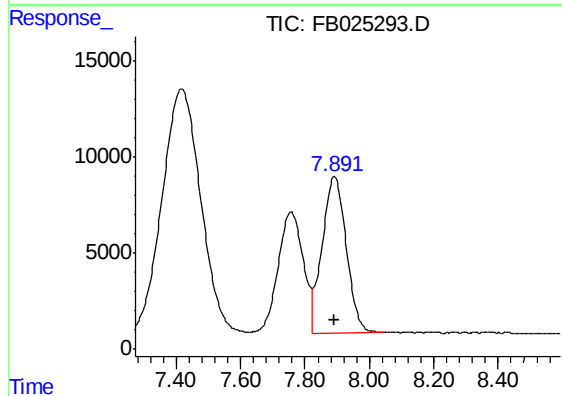


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.001 min
Response: 424629
Conc: 10.68 ng/ml

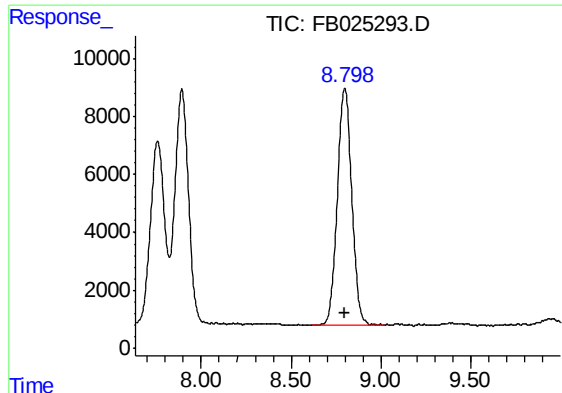


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 457724
Conc: 20.27 ng/ml

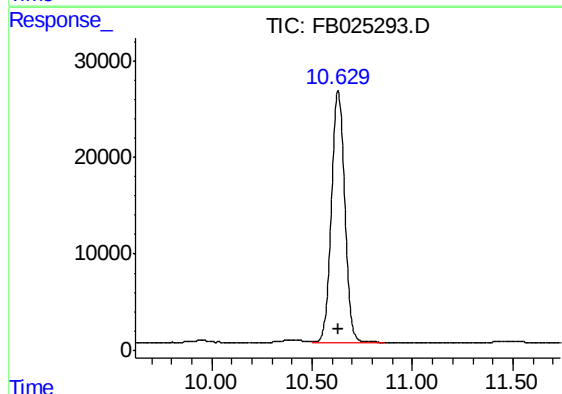


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1203572
Conc: 32.19 ng/ml

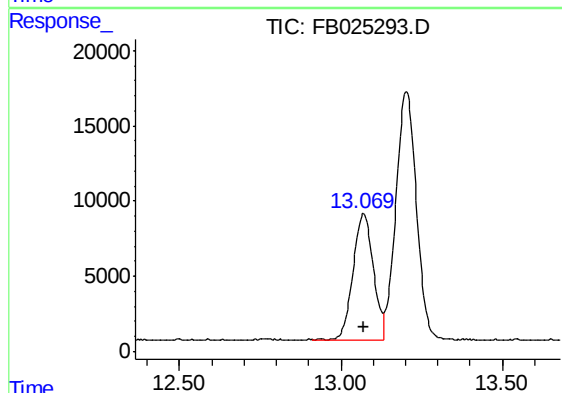


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 362297
Conc: 10.55 ng/ml

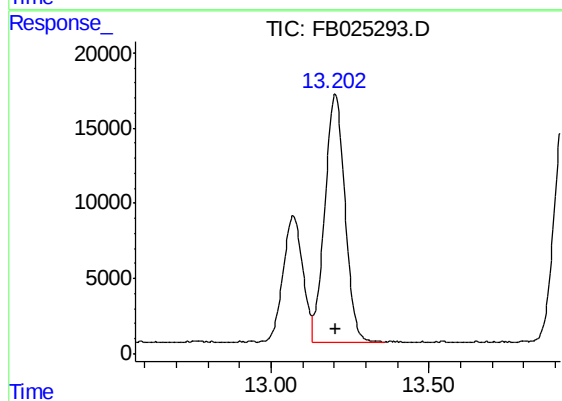


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 729326
Conc: 21.60 ng/ml

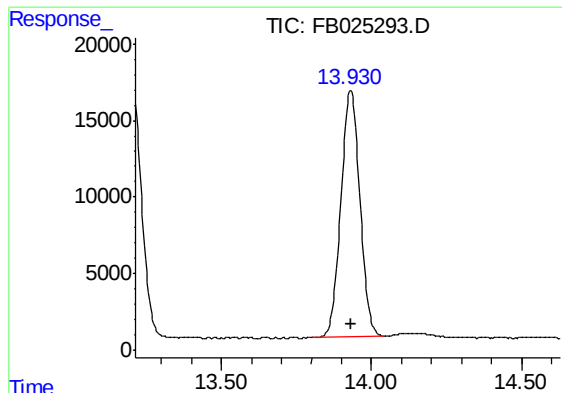

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 708174
Conc: 21.66 ng/ml

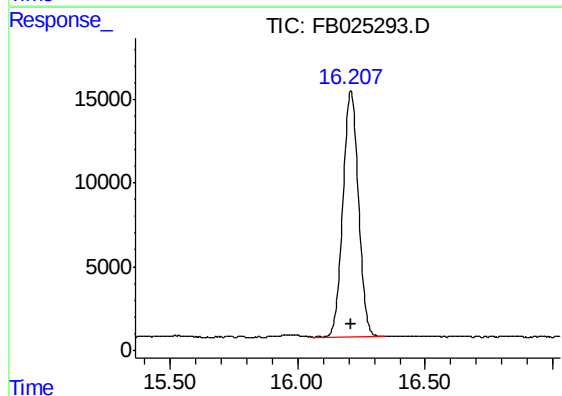

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 619572
Conc: 22.52 ng/ml