

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112720\
 Data File : FB025291.D
 Signal(s) : FID2B.CH
 Acq On : 27 Nov 2020 12:20
 Operator : DD/AJ
 Sample : L4900-05MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 27 22:59:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	450853	19.967 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	870165	26.959 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	897736	27.058 ng/ml
3) t n-Heptane	7.758	254265	7.741 ng/ml
4) t Benzene	7.892	396225	9.965 ng/ml
6) t Toluene	10.631	1085617	29.034 ng/ml
7) t Ethylbenzene	13.071	326809	9.517 ng/ml
8) t m-Xylene	13.204	649992	19.251 ng/ml
9) t O-Xylene	13.932	632290	19.338 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	525556	19.101 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112720\
Data File : FB025291.D
Signal(s) : FID2B.CH
Acq On : 27 Nov 2020 12:20
Operator : DD/AJ
Sample : L4900-05MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 27 22:59:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

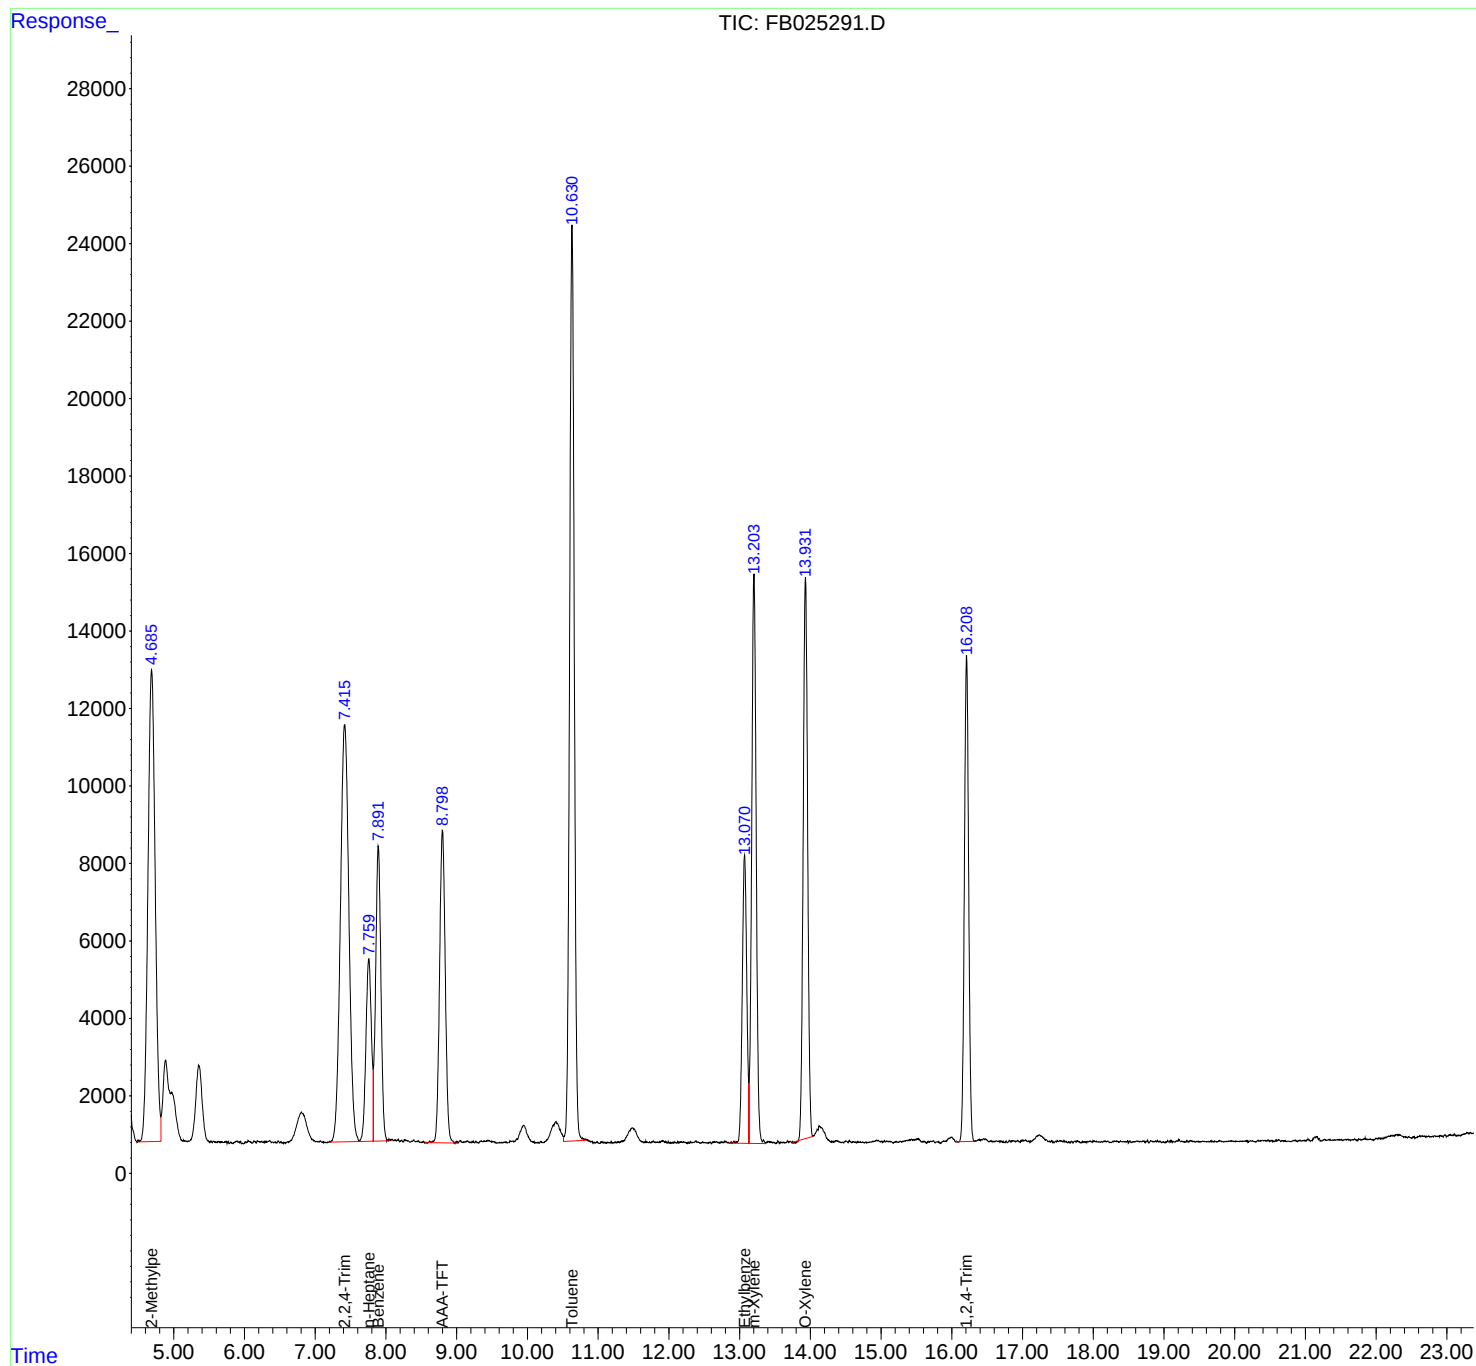

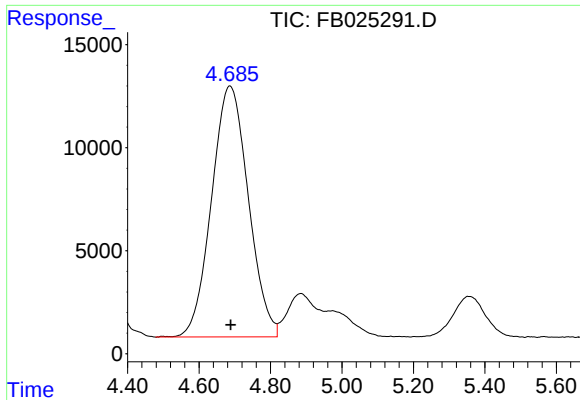


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 870165
Conc: 26.96 ng/ml

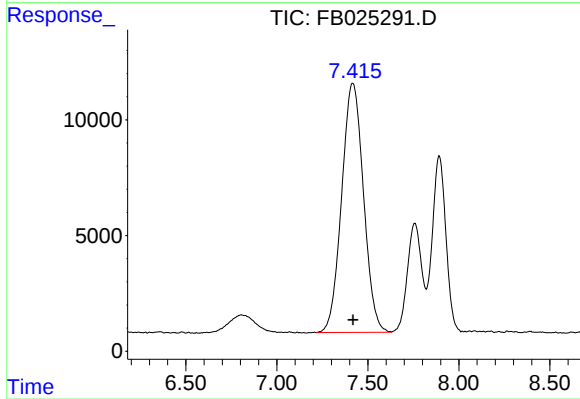


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.001 min
Response: 897736
Conc: 27.06 ng/ml

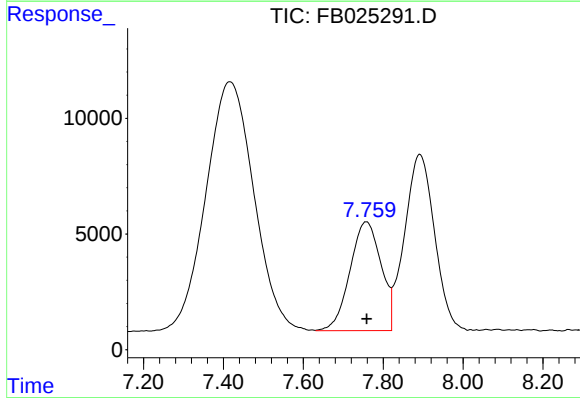


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 254265
Conc: 7.74 ng/ml

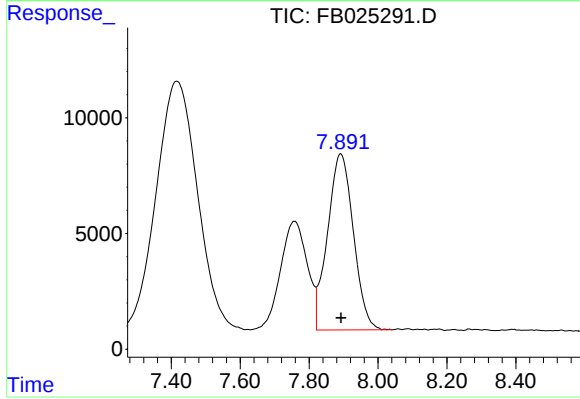


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 396225
Conc: 9.97 ng/ml

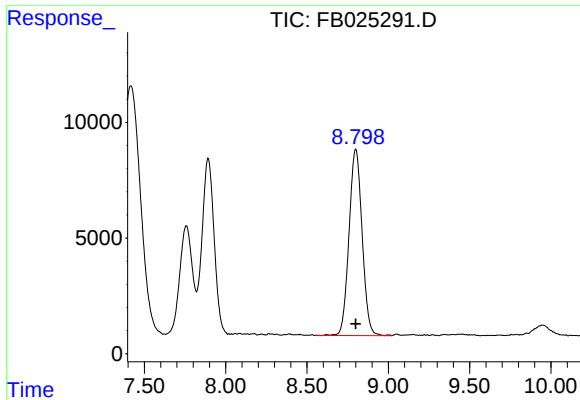


#5 AAA-TFT

R.T.: 8.800 min
 Delta R.T.: 0.000 min
 Response: 450853
 Conc: 19.97 ng/ml

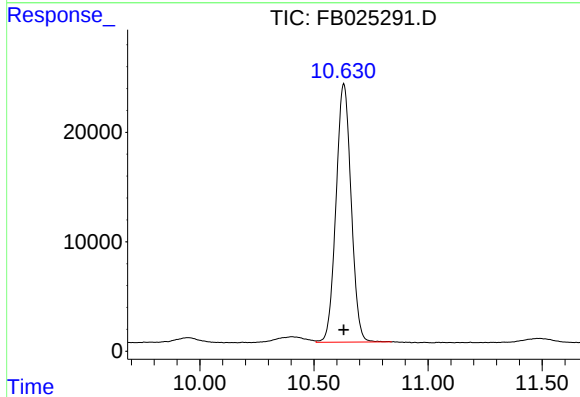


#6 Toluene

R.T.: 10.631 min
 Delta R.T.: 0.000 min
 Response: 1085617
 Conc: 29.03 ng/ml

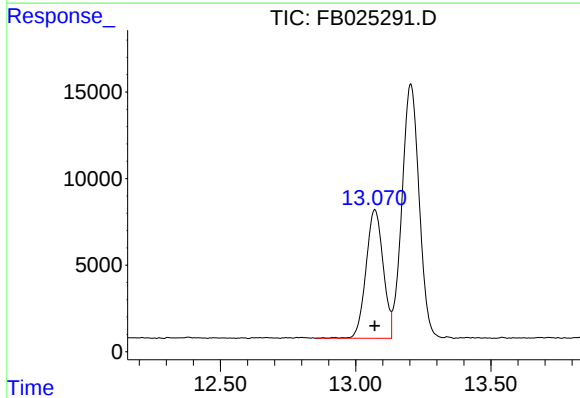


#7 Ethylbenzene

R.T.: 13.071 min
 Delta R.T.: 0.000 min
 Response: 326809
 Conc: 9.52 ng/ml

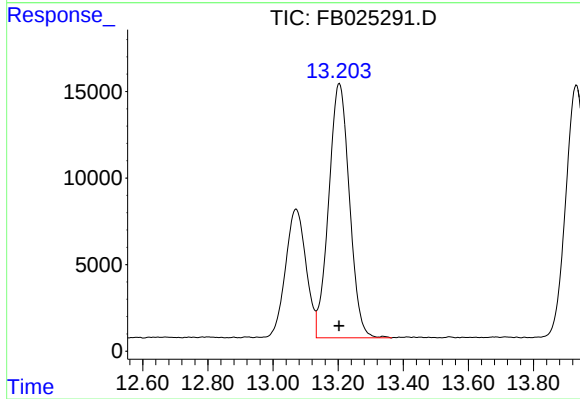


#8 m-Xylene

R.T.: 13.204 min
 Delta R.T.: 0.000 min
 Response: 649992
 Conc: 19.25 ng/ml

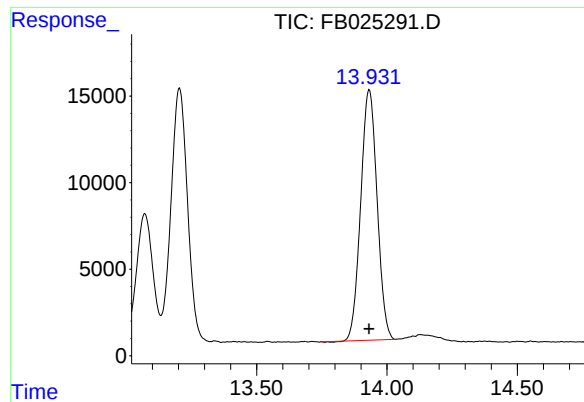

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 632290
Conc: 19.34 ng/ml

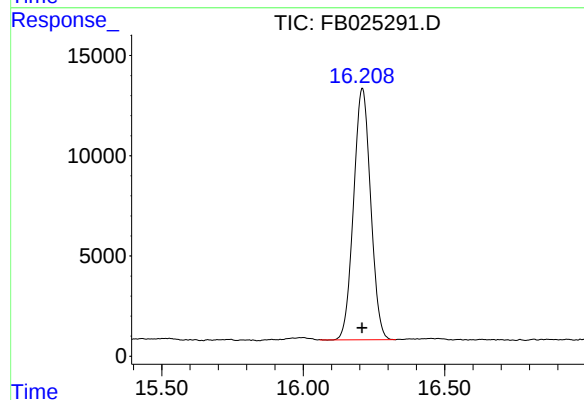

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 525556
Conc: 19.10 ng/ml