

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112822\
 Data File : FB029055.D
 Signal(s) : FID2B.CH
 Acq On : 28 Nov 2022 9:21
 Operator : AJ/MA
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 5 GRO STD

Integration File: Calibration.e
 Quant Time: Nov 28 10:49:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112822.M
 Quant Title :
 QLast Update : Mon Nov 28 10:47:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	76331	6.668 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	87688	7.853 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	91299	6.640 ng/ml
3) t n-Heptane	7.749	34333	3.213 ng/ml
4) t Benzene	7.884	40396	2.666 ng/ml
6) t Toluene	10.614	122726	8.081 ng/ml
7) t Ethylbenzene	13.052	39192	2.601 ng/ml
8) t m-Xylene	13.184	77401	5.117 ng/ml
9) t O-Xylene	13.910	84369	5.477 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	90903	5.454 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112822\
Data File : FB029055.D
Signal(s) : FID2B.CH
Acq On : 28 Nov 2022 9:21
Operator : AJ/MA
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
5 GRO STD

Integration File: Calibration.e
Quant Time: Nov 28 10:49:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112822.M
Quant Title :
QLast Update : Mon Nov 28 10:47:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

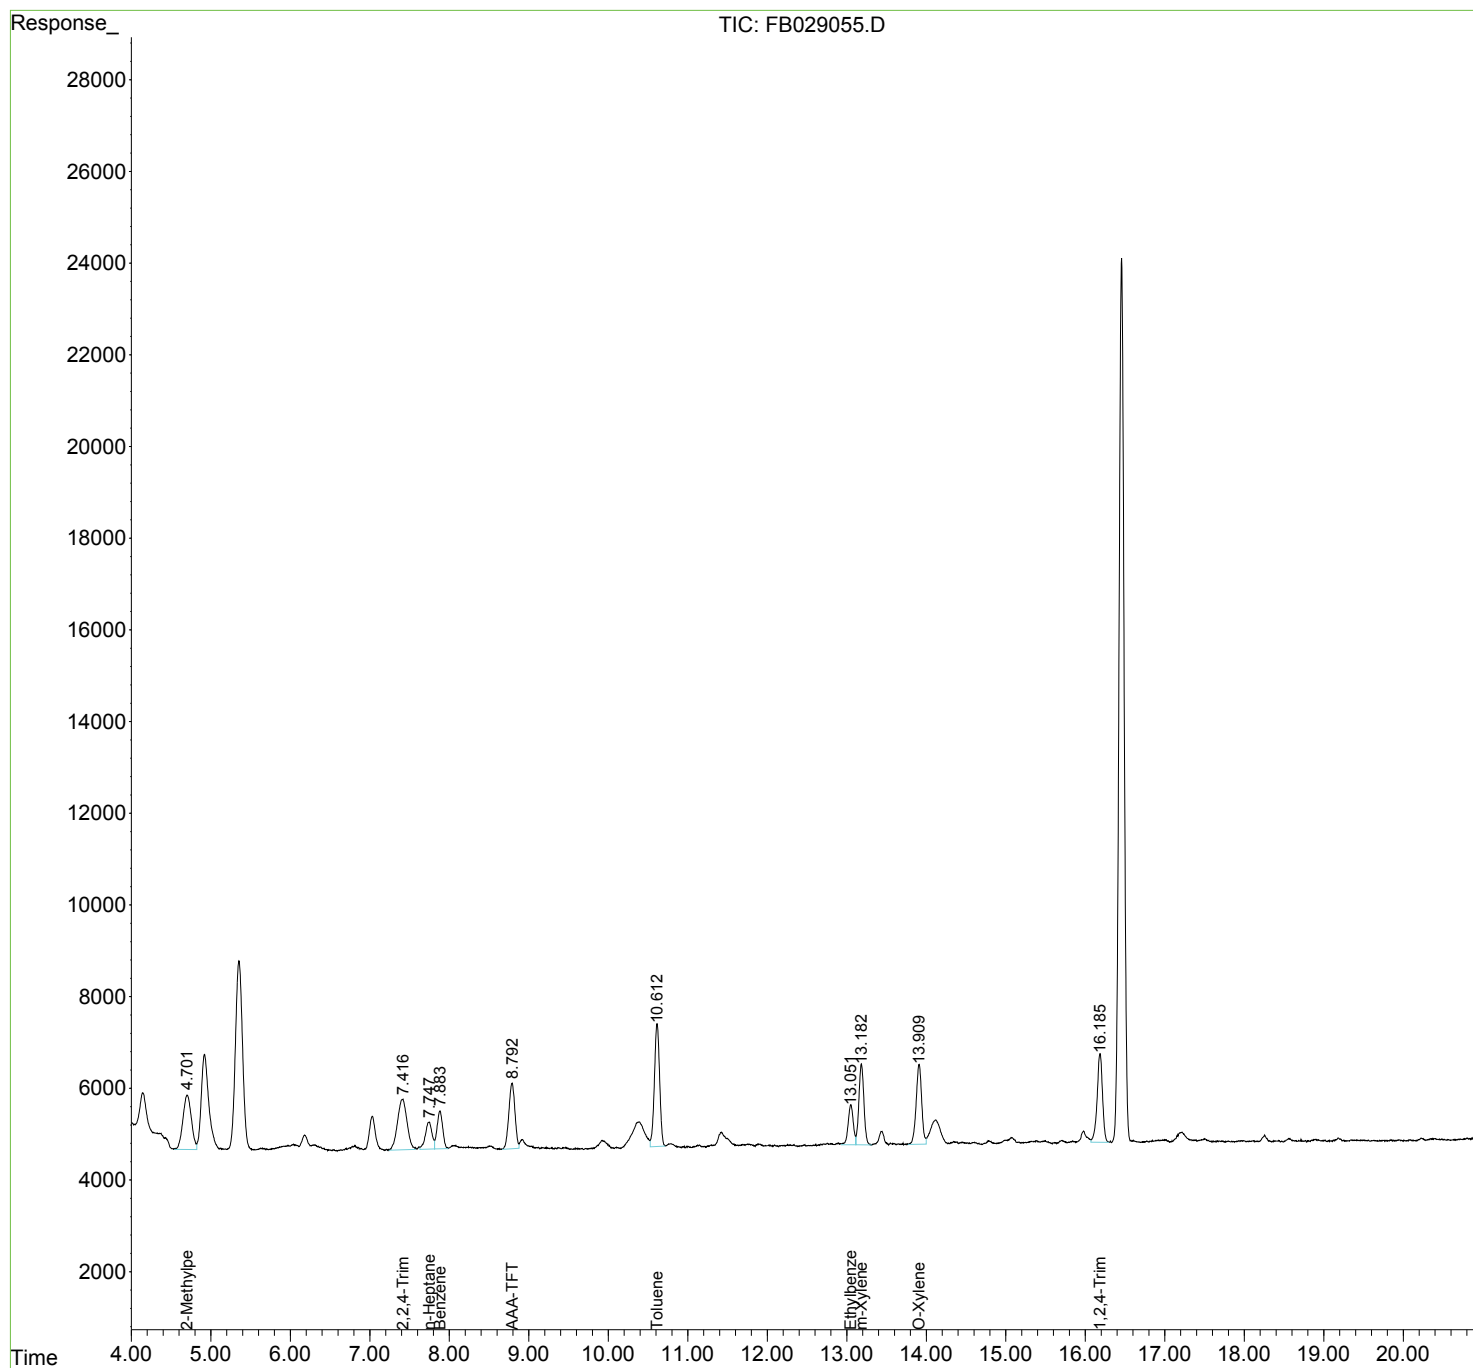


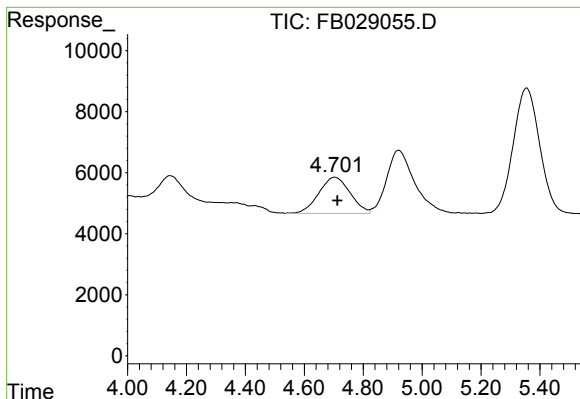

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.011 min
Response: 87688
Conc: 7.85 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

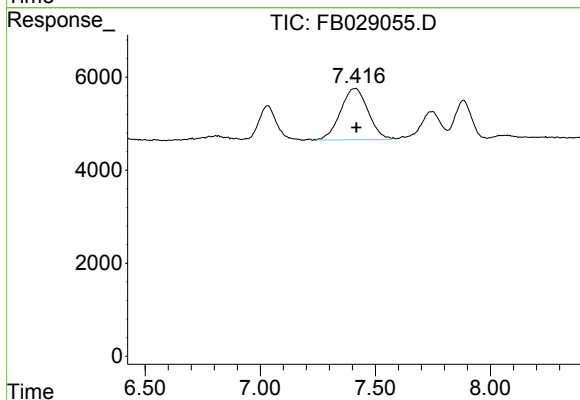


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 91299
Conc: 6.64 ng/ml

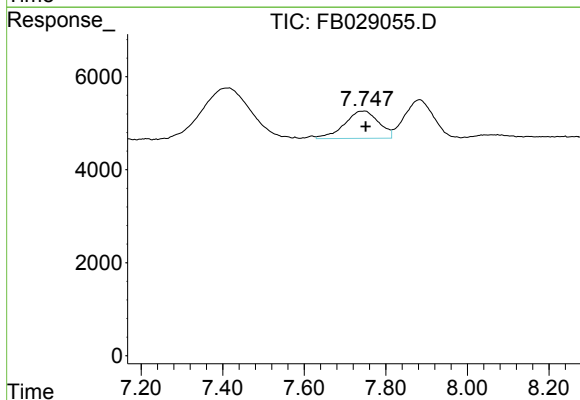


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 34333
Conc: 3.21 ng/ml

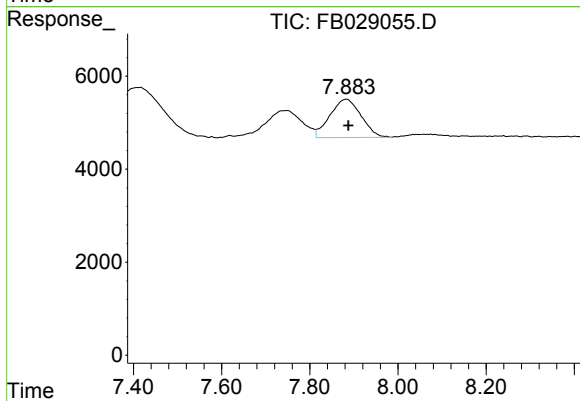

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.003 min
Response: 40396
Conc: 2.67 ng/ml

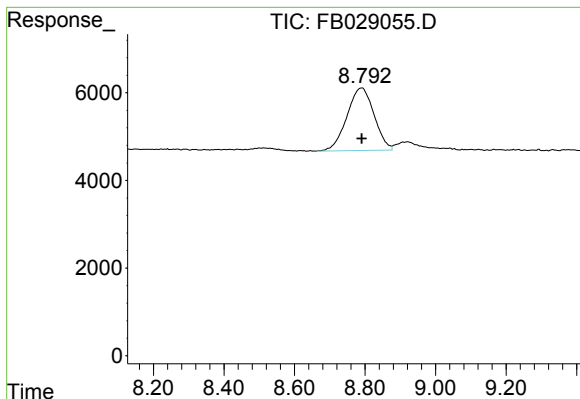

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 76331
Conc: 6.67 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

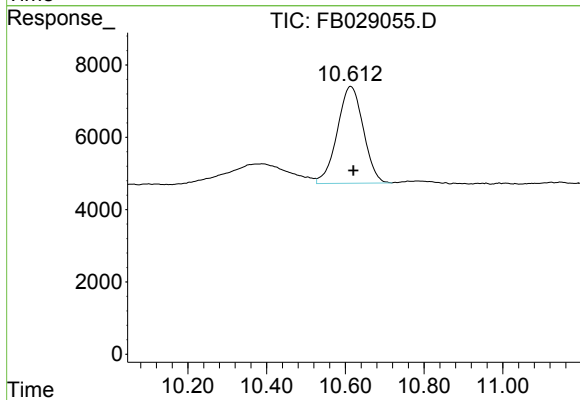


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.006 min
Response: 122726
Conc: 8.08 ng/ml

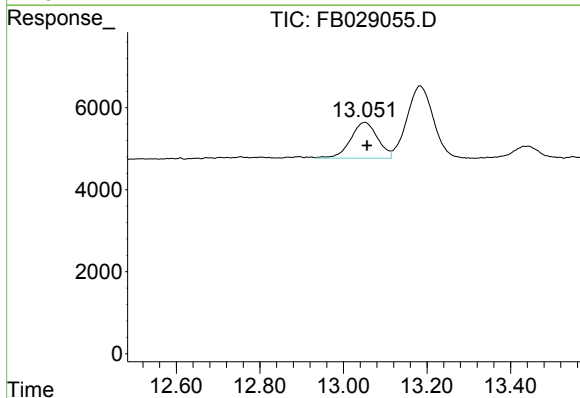


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.004 min
Response: 39192
Conc: 2.60 ng/ml

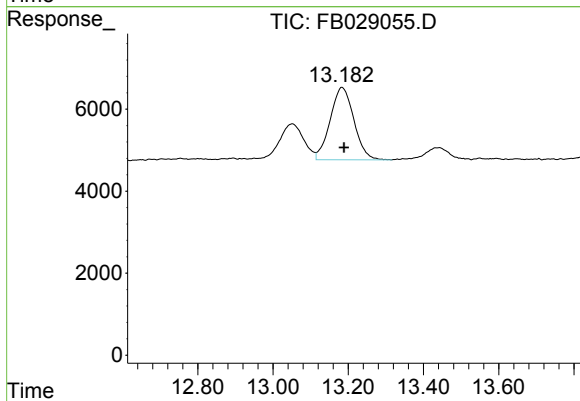

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: -0.005 min
Response: 77401
Conc: 5.12 ng/ml

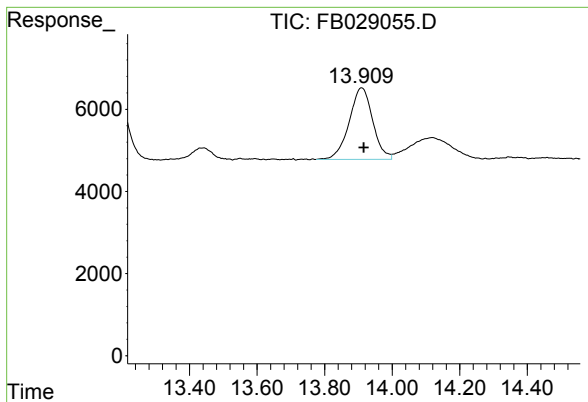

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.005 min
Response: 84369
Conc: 5.48 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

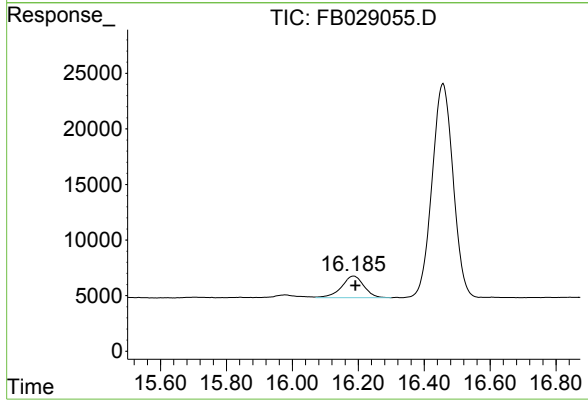

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.004 min
Response: 90903
Conc: 5.45 ng/ml