

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120120\
 Data File : FB025296.D
 Signal(s) : FID2B.CH
 Acq On : 1 Dec 2020 9:27
 Operator : DD/AJ
 Sample : BSF1201S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1201S1

Integration File: Calibration.e
 Quant Time: Dec 02 00:19:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	460840	20.410 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	976427	30.251 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1063805	32.064 ng/ml
3) t n-Heptane	7.760	342664	10.433 ng/ml
4) t Benzene	7.895	425004	10.689 ng/ml
6) t Toluene	10.634	1209857	32.357 ng/ml
7) t Ethylbenzene	13.074	379559	11.053 ng/ml
8) t m-Xylene	13.207	753279	22.310 ng/ml
9) t O-Xylene	13.935	727985	22.265 ng/ml
10) t 1,2,4-Trimethylbenzene	16.213	642423	23.348 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120120\
Data File : FB025296.D
Signal(s) : FID2B.CH
Acq On : 1 Dec 2020 9:27
Operator : DD/AJ
Sample : BSF1201S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1201S1

Integration File: Calibration.e
Quant Time: Dec 02 00:19:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

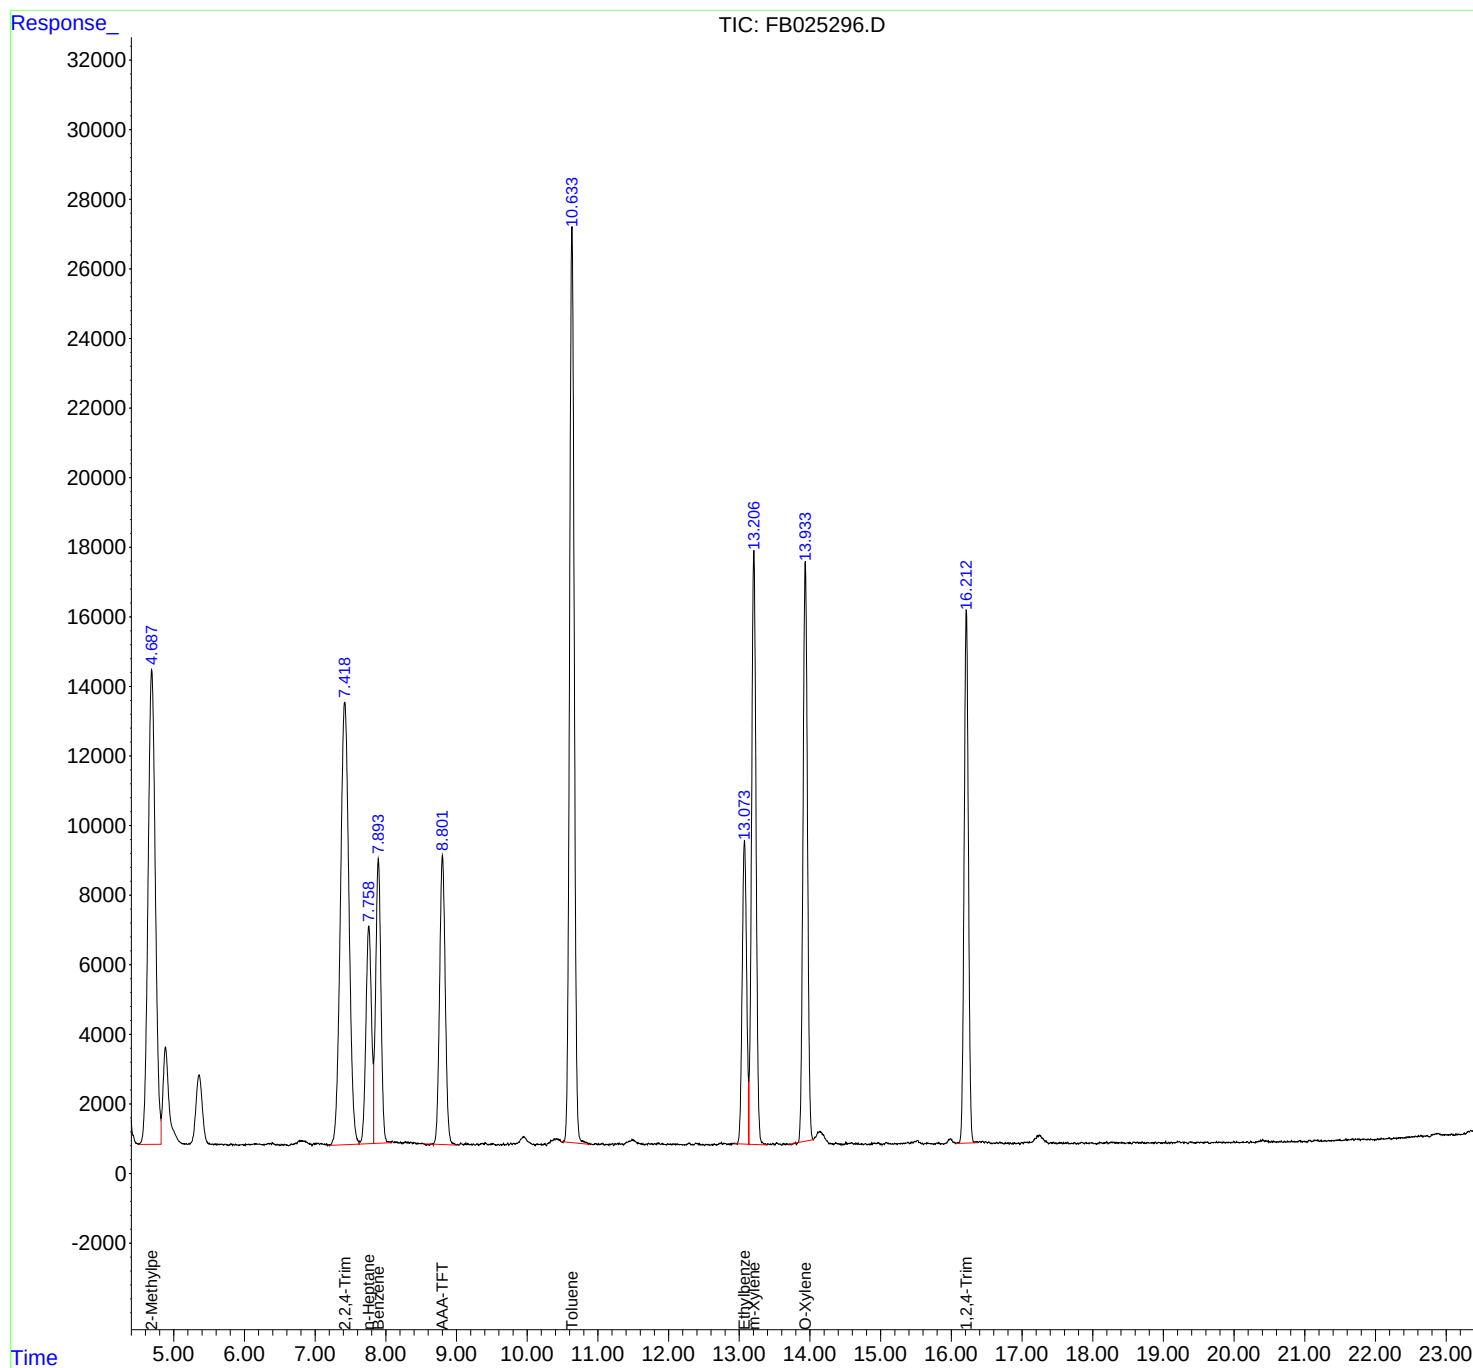


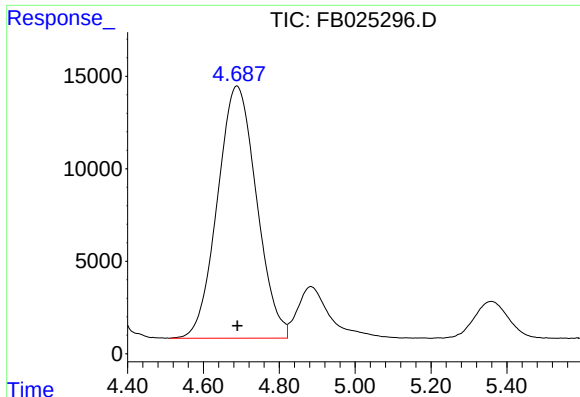

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 976427
Conc: 30.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1201S1

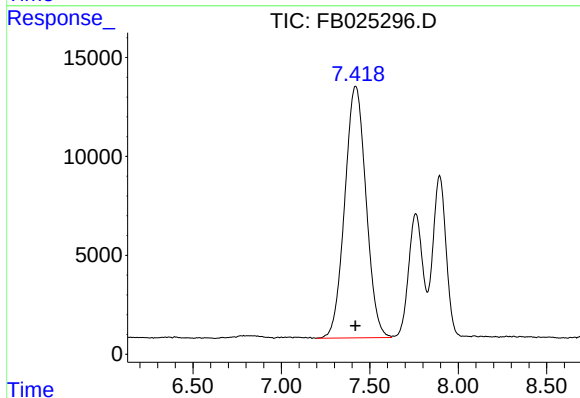


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.001 min
Response: 1063805
Conc: 32.06 ng/ml

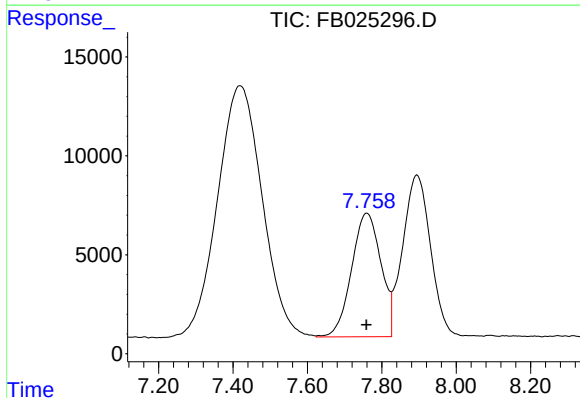


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.001 min
Response: 342664
Conc: 10.43 ng/ml

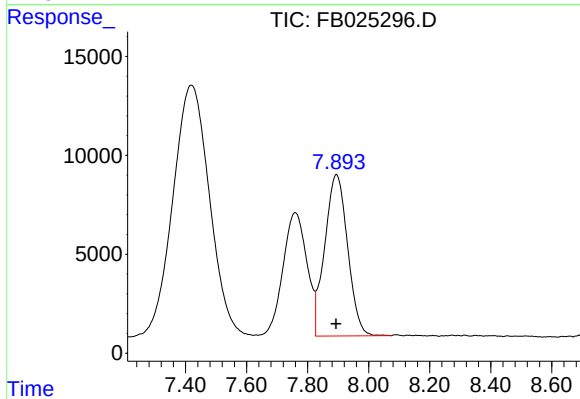

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.002 min
Response: 425004
Conc: 10.69 ng/ml

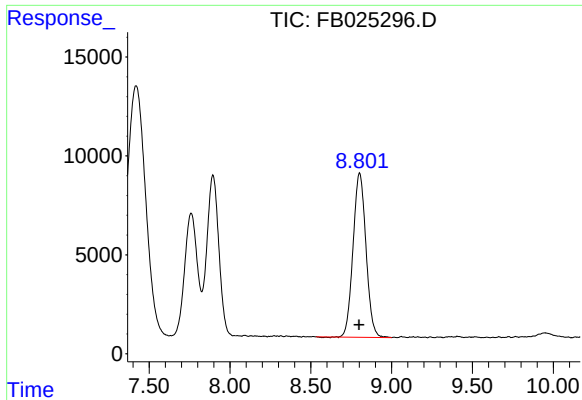

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.003 min
Response: 460840
Conc: 20.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1201S1

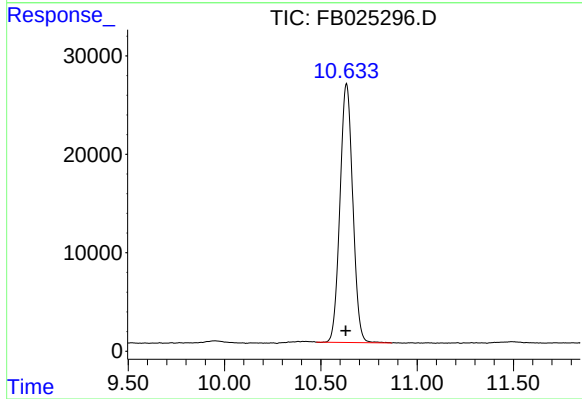


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.003 min
Response: 1209857
Conc: 32.36 ng/ml

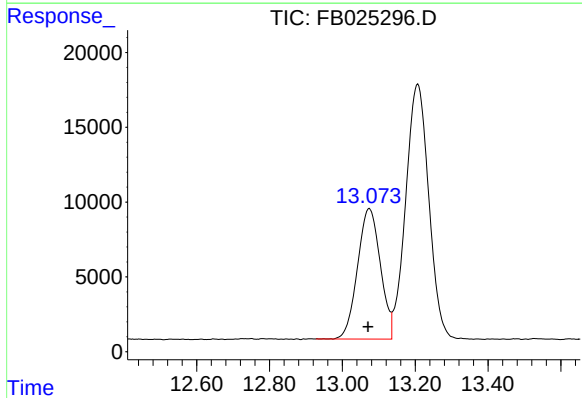


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.004 min
Response: 379559
Conc: 11.05 ng/ml

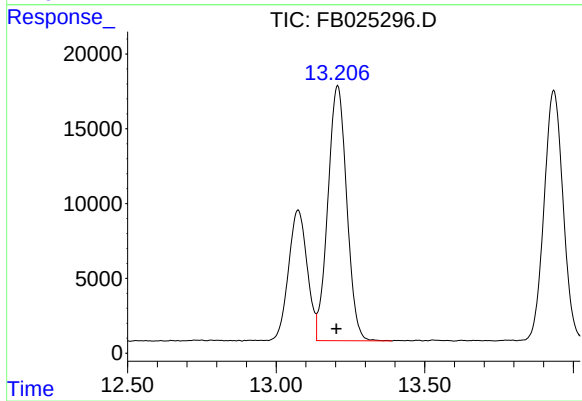

#8 m-Xylene


R.T.: 13.207 min
Delta R.T.: 0.004 min
Response: 753279
Conc: 22.31 ng/ml

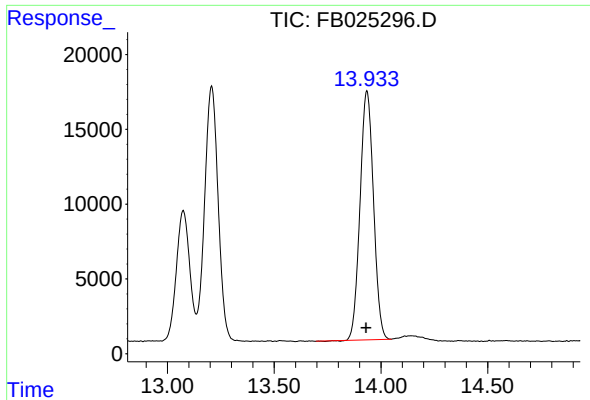

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.004 min
Response: 727985
Conc: 22.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1201S1

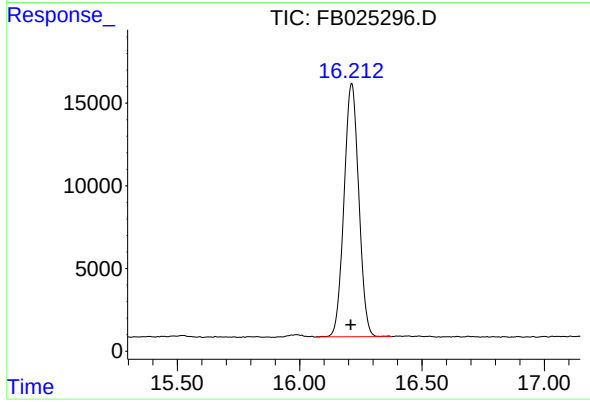

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.004 min
Response: 642423
Conc: 23.35 ng/ml