

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120120\
 Data File : FB025301.D
 Signal(s) : FID2B.CH
 Acq On : 1 Dec 2020 12:06
 Operator : DD/AJ
 Sample : L4900-03MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 PAV-B2-112520-0-10MS

Integration File: Calibration.e
 Quant Time: Dec 02 00:19:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	479659	21.243 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	894798	27.722 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	933082	28.123 ng/ml
3) t n-Heptane	7.761	201028	6.120 ng/ml
4) t Benzene	7.895	417419	10.498 ng/ml
6) t Toluene	10.634	1113659	29.784 ng/ml
7) t Ethylbenzene	13.074	321070	9.350 ng/ml
8) t m-Xylene	13.207	643019	19.044 ng/ml
9) t O-Xylene	13.935	646896	19.785 ng/ml
10) t 1,2,4-Trimethylbenzene	16.213	513282	18.655 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120120\
Data File : FB025301.D
Signal(s) : FID2B.CH
Acq On : 1 Dec 2020 12:06
Operator : DD/AJ
Sample : L4900-03MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
PAV-B2-112520-0-10MS

Integration File: Calibration.e
Quant Time: Dec 02 00:19:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

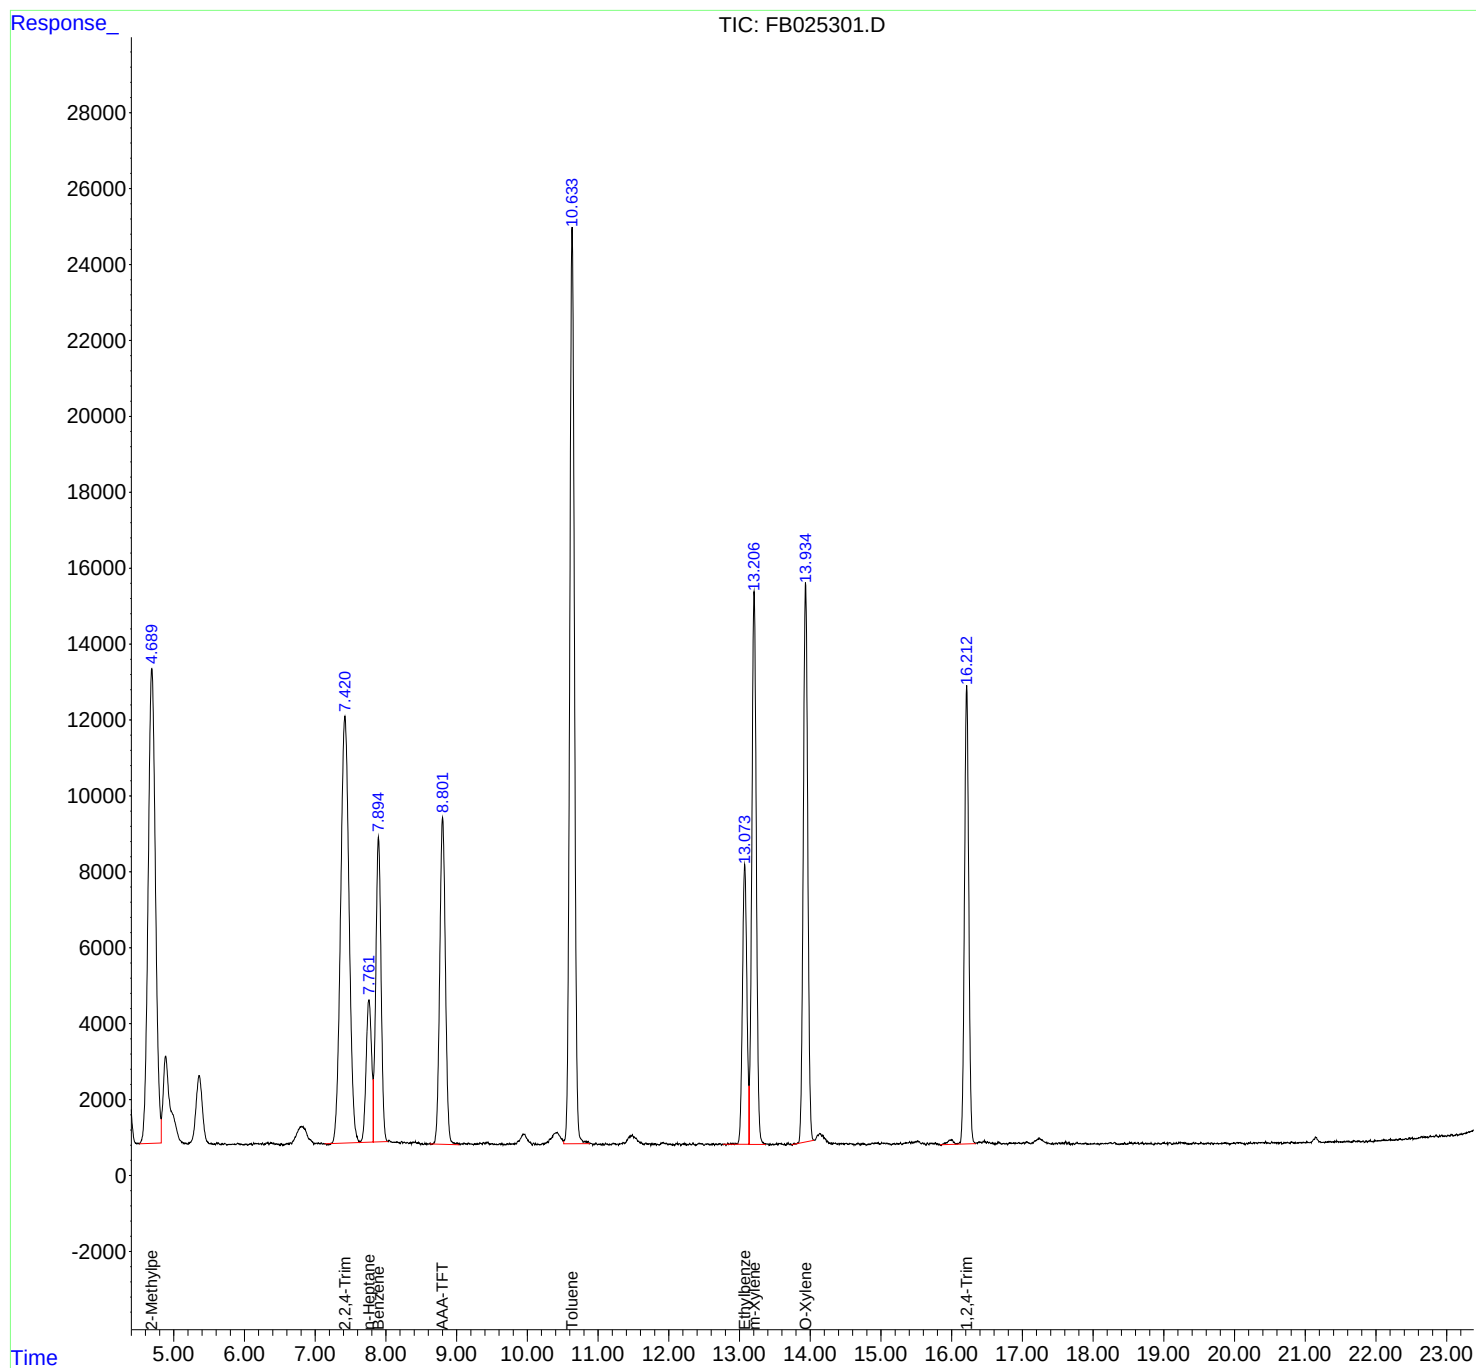


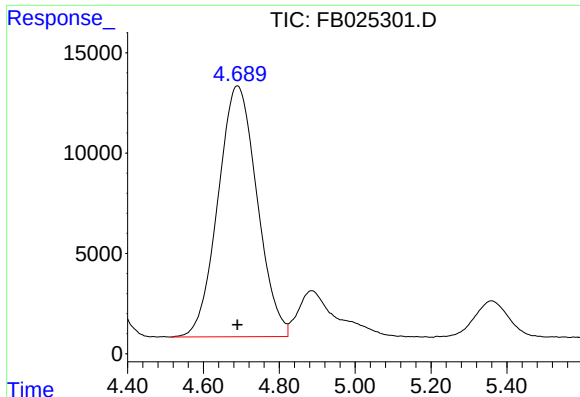

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.002 min
Response: 894798
Conc: 27.72 ng/ml

Instrument :
FID_B
ClientSampleId :
PAV-B2-112520-0-10MS

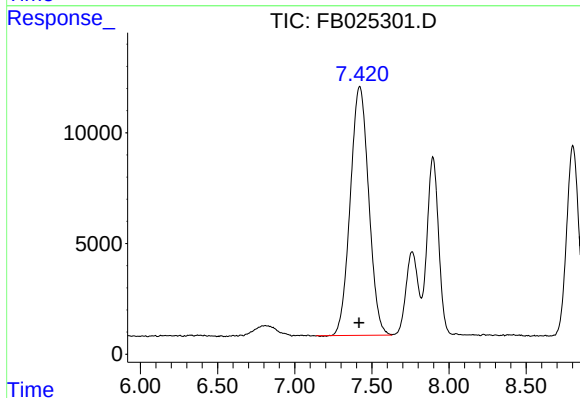


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.004 min
Response: 933082
Conc: 28.12 ng/ml

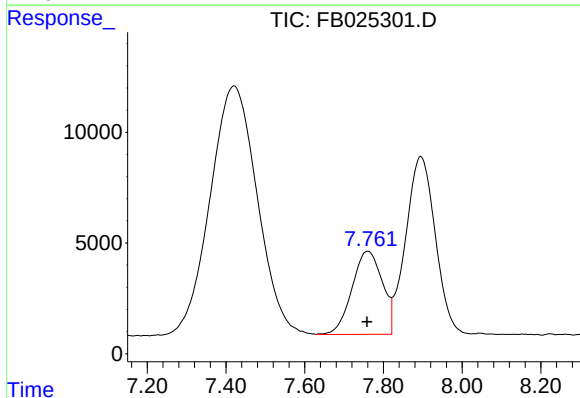


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.002 min
Response: 201028
Conc: 6.12 ng/ml

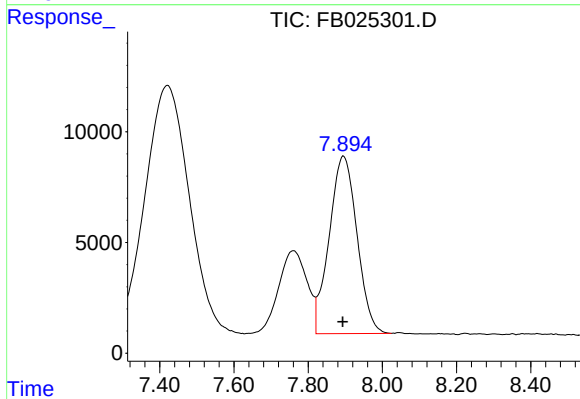

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.002 min
Response: 417419
Conc: 10.50 ng/ml

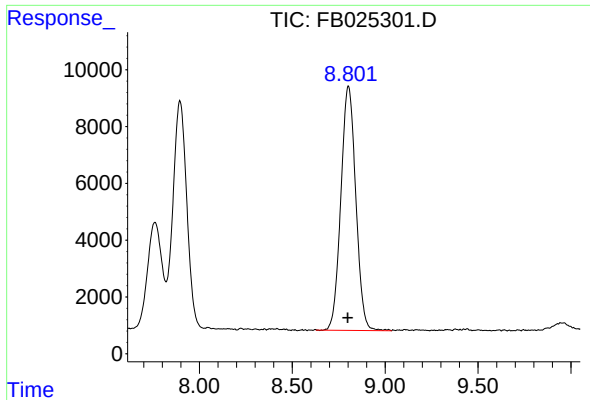

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.003 min
Response: 479659
Conc: 21.24 ng/ml

Instrument :
FID_B
ClientSampleId :
PAV-B2-112520-0-10MS

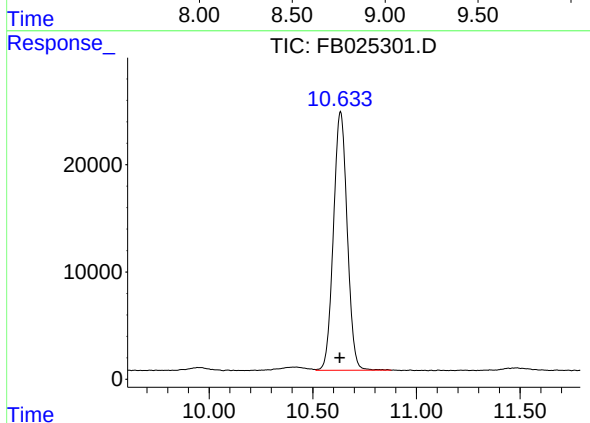


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.004 min
Response: 1113659
Conc: 29.78 ng/ml

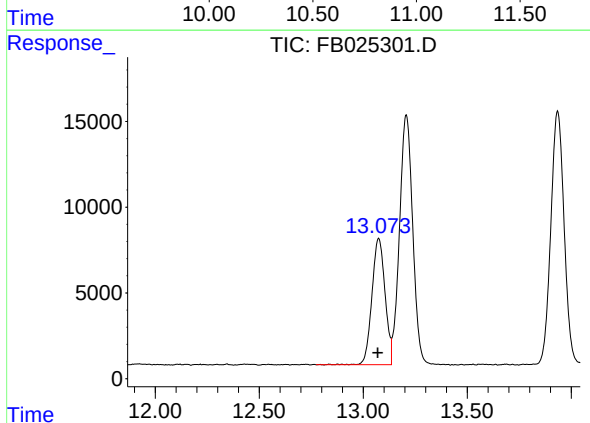


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.004 min
Response: 321070
Conc: 9.35 ng/ml

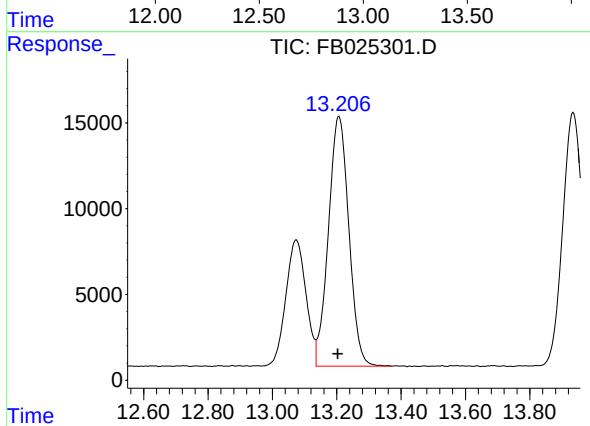

#8 m-Xylene


R.T.: 13.207 min
Delta R.T.: 0.004 min
Response: 643019
Conc: 19.04 ng/ml

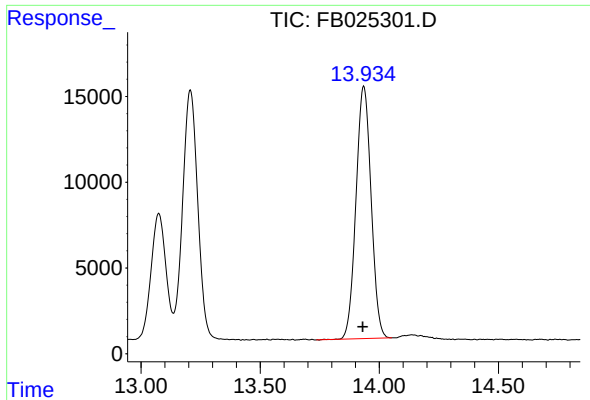

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.004 min
Response: 646896
Conc: 19.78 ng/ml

Instrument :
FID_B
ClientSampleId :
PAV-B2-112520-0-10MS

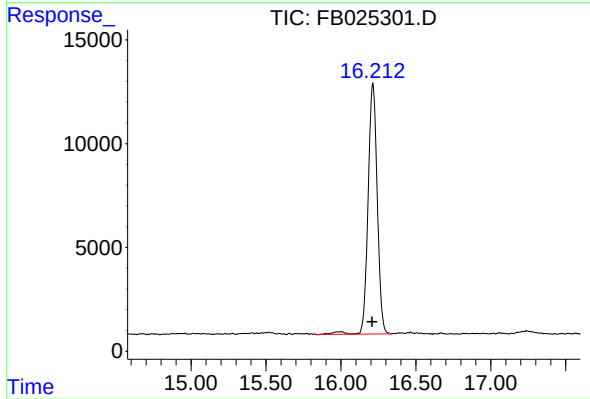

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.005 min
Response: 513282
Conc: 18.65 ng/ml