

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120120\
 Data File : FB025302.D
 Signal(s) : FID2B.CH
 Acq On : 1 Dec 2020 12:37
 Operator : DD/AJ
 Sample : L4900-03MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 PAV-B2-112520-0-10MSD

Integration File: Calibration.e
 Quant Time: Dec 02 00:20:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	510585	22.613 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	863632	26.756 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	949139	28.607 ng/ml
3) t n-Heptane	7.760	245518	7.475 ng/ml
4) t Benzene	7.895	422931	10.637 ng/ml
6) t Toluene	10.633	1154282	30.871 ng/ml
7) t Ethylbenzene	13.074	346844	10.100 ng/ml
8) t m-Xylene	13.207	690585	20.453 ng/ml
9) t O-Xylene	13.935	672119	20.556 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	556934	20.241 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120120\
Data File : FB025302.D
Signal(s) : FID2B.CH
Acq On : 1 Dec 2020 12:37
Operator : DD/AJ
Sample : L4900-03MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
PAV-B2-112520-0-10MSD

Integration File: Calibration.e
Quant Time: Dec 02 00:20:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

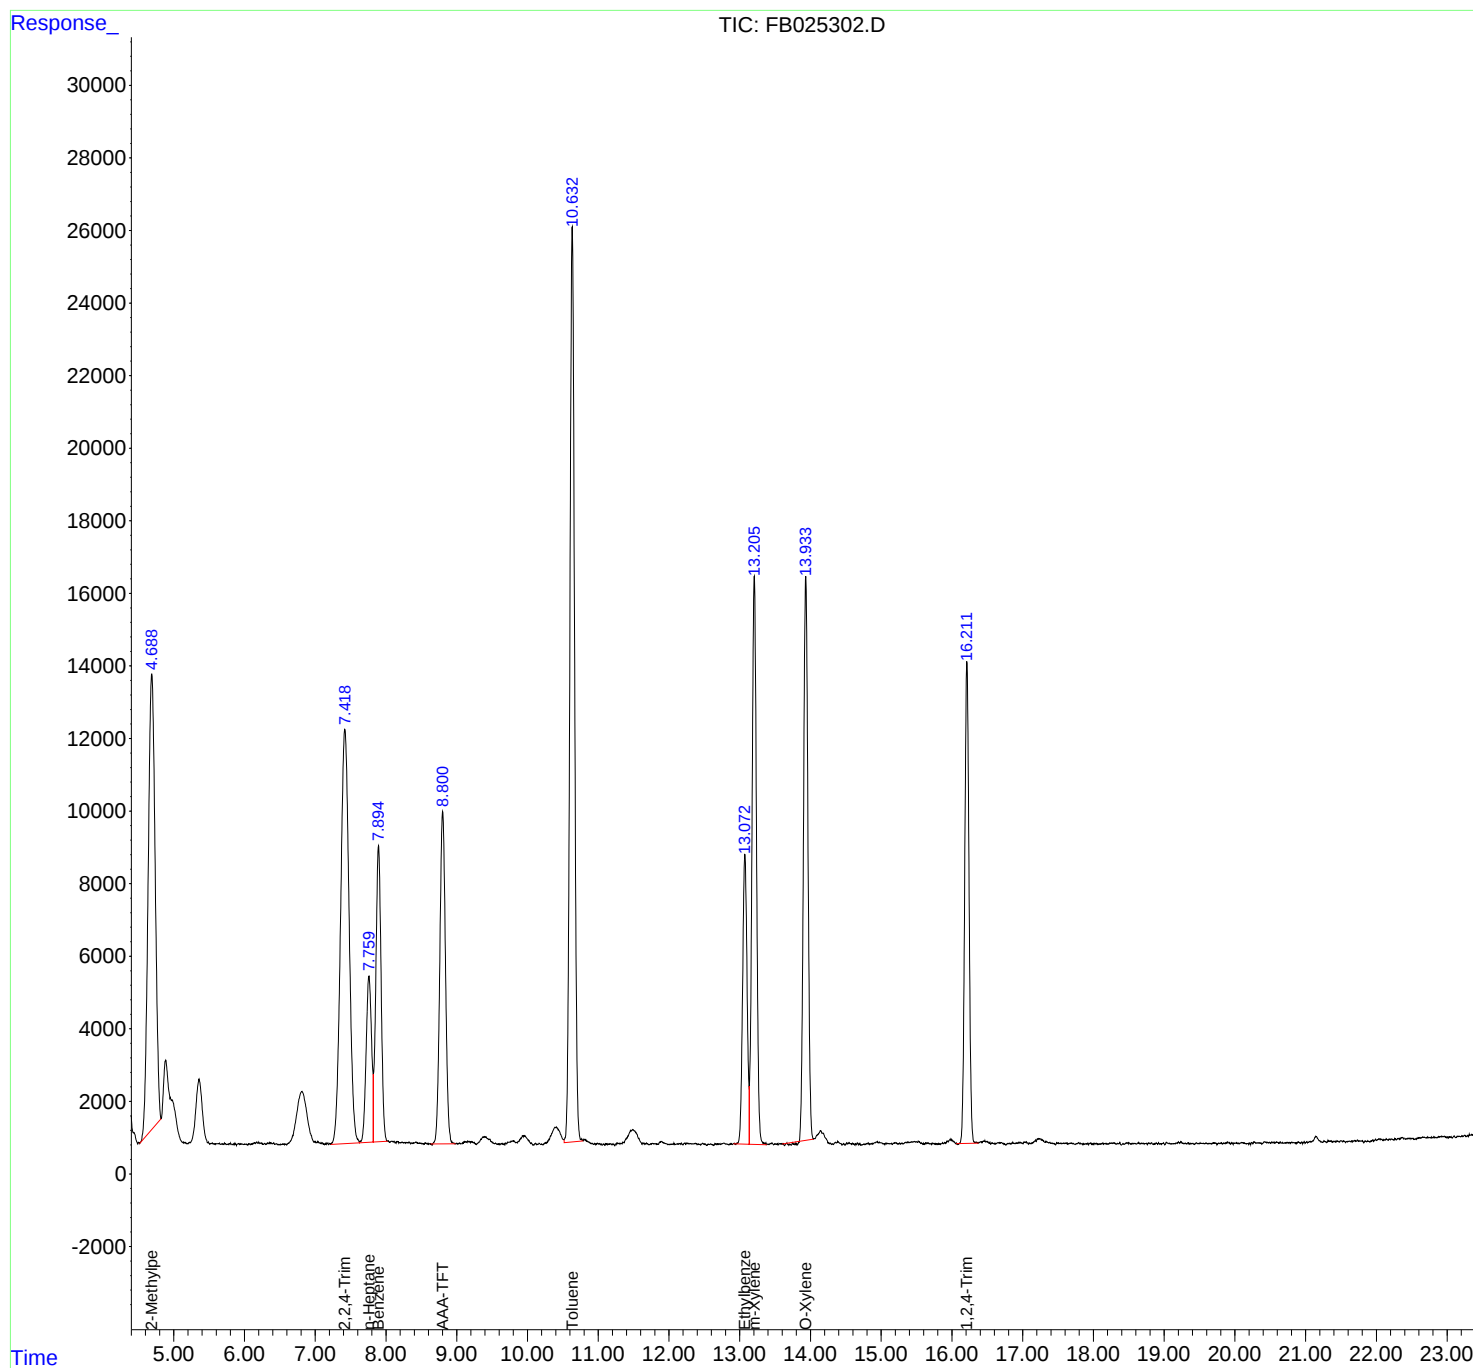


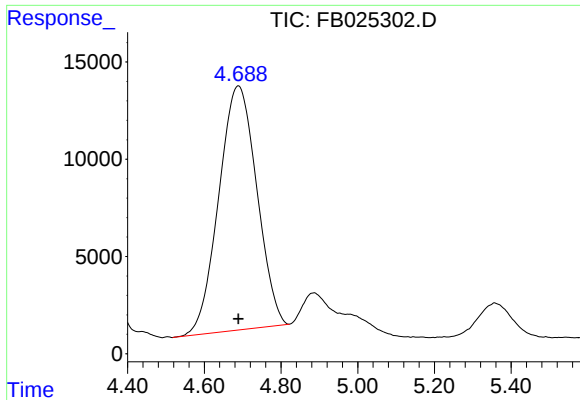

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 863632
Conc: 26.76 ng/ml

Instrument :
FID_B
ClientSampleId :
PAV-B2-112520-0-10MSD

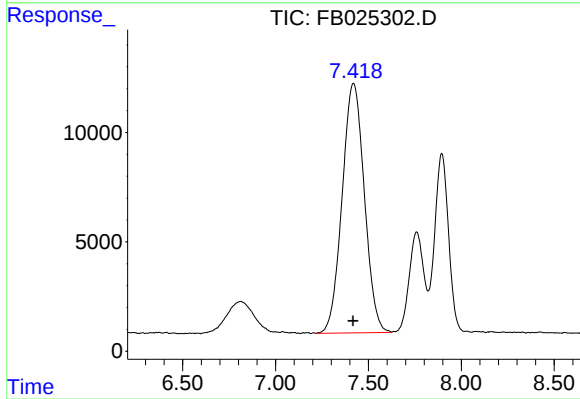


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.001 min
Response: 949139
Conc: 28.61 ng/ml

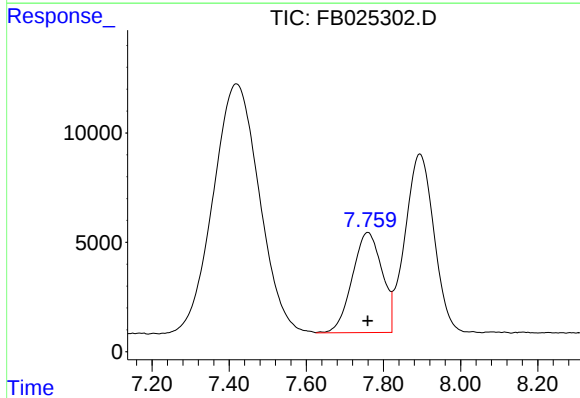


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.001 min
Response: 245518
Conc: 7.48 ng/ml

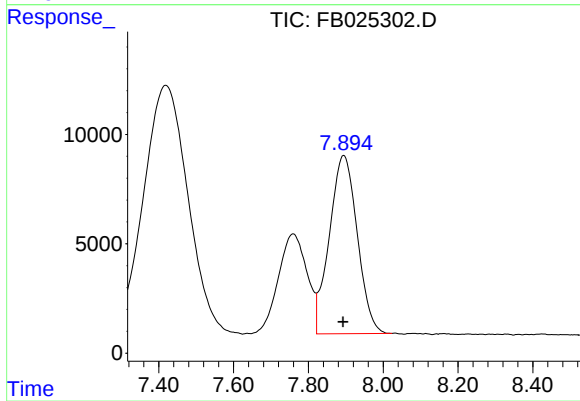

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.002 min
Response: 422931
Conc: 10.64 ng/ml

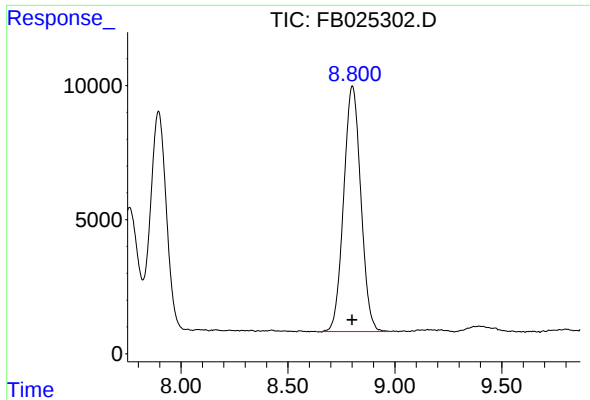

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.003 min
Response: 510585
Conc: 22.61 ng/ml

Instrument :
FID_B
ClientSampleId :
PAV-B2-112520-0-10MSD

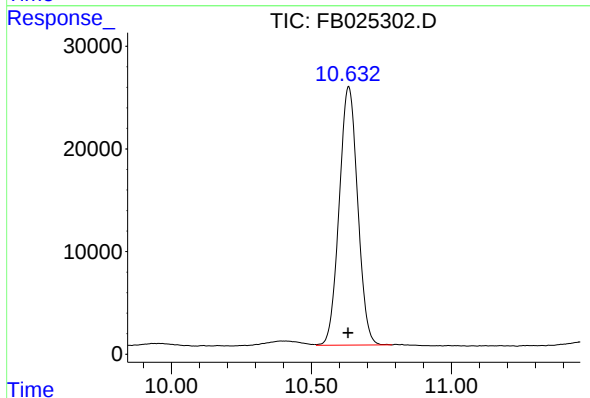


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.003 min
Response: 1154282
Conc: 30.87 ng/ml

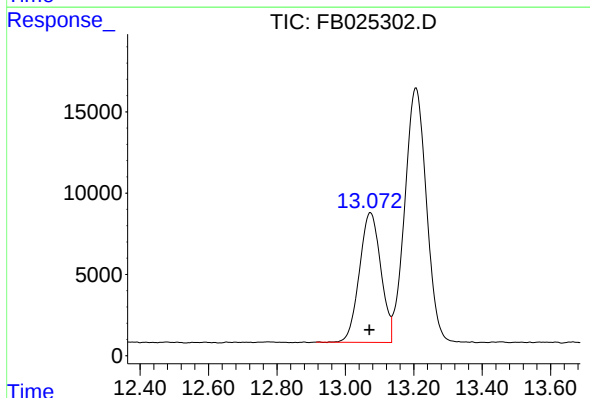


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.003 min
Response: 346844
Conc: 10.10 ng/ml

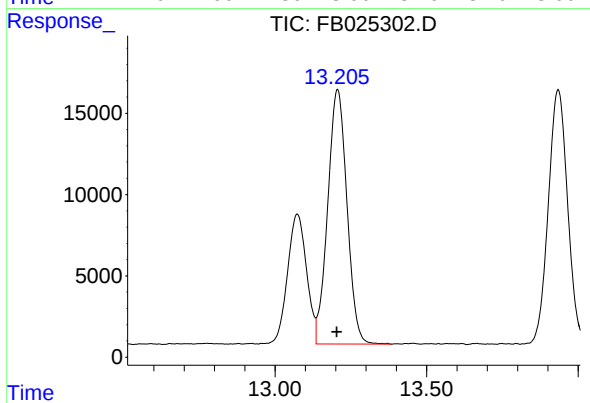

#8 m-Xylene


R.T.: 13.207 min
Delta R.T.: 0.003 min
Response: 690585
Conc: 20.45 ng/ml

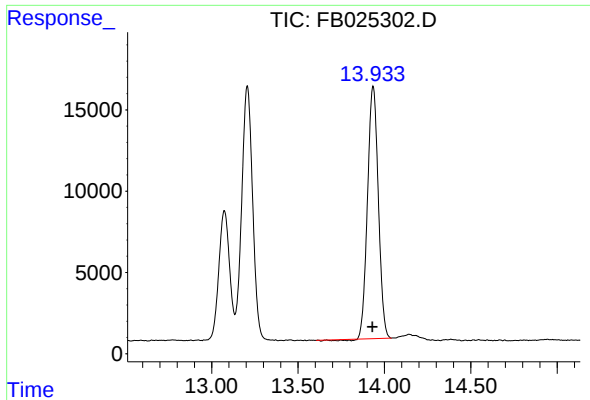

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.003 min
Response: 672119
Conc: 20.56 ng/ml

Instrument :
FID_B
ClientSampleId :
PAV-B2-112520-0-10MSD

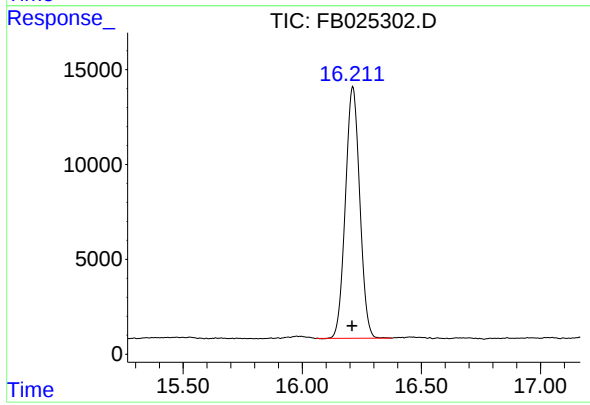

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.003 min
Response: 556934
Conc: 20.24 ng/ml