

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120219\
 Data File : FB023121.D
 Signal(s) : FID2B.CH
 Acq On : 2 Dec 2019 13:42
 Operator : DD/AJ
 Sample : K5948-02
 Misc : 7.11g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 02 13:11:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	519231	21.138 ng/ml
Target Compounds			
6) t Toluene	10.625	1922	0.048 ng/ml
9) t O-Xylene	13.872	212	0.006 ng/ml
10) t 1,2,4-Trimethylbenzene	16.164	2674	0.095 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120219\
Data File : FB023121.D
Signal(s) : FID2B.CH
Acq On : 2 Dec 2019 13:42
Operator : DD/AJ
Sample : K5948-02
Misc : 7.11g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 02 13:11:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

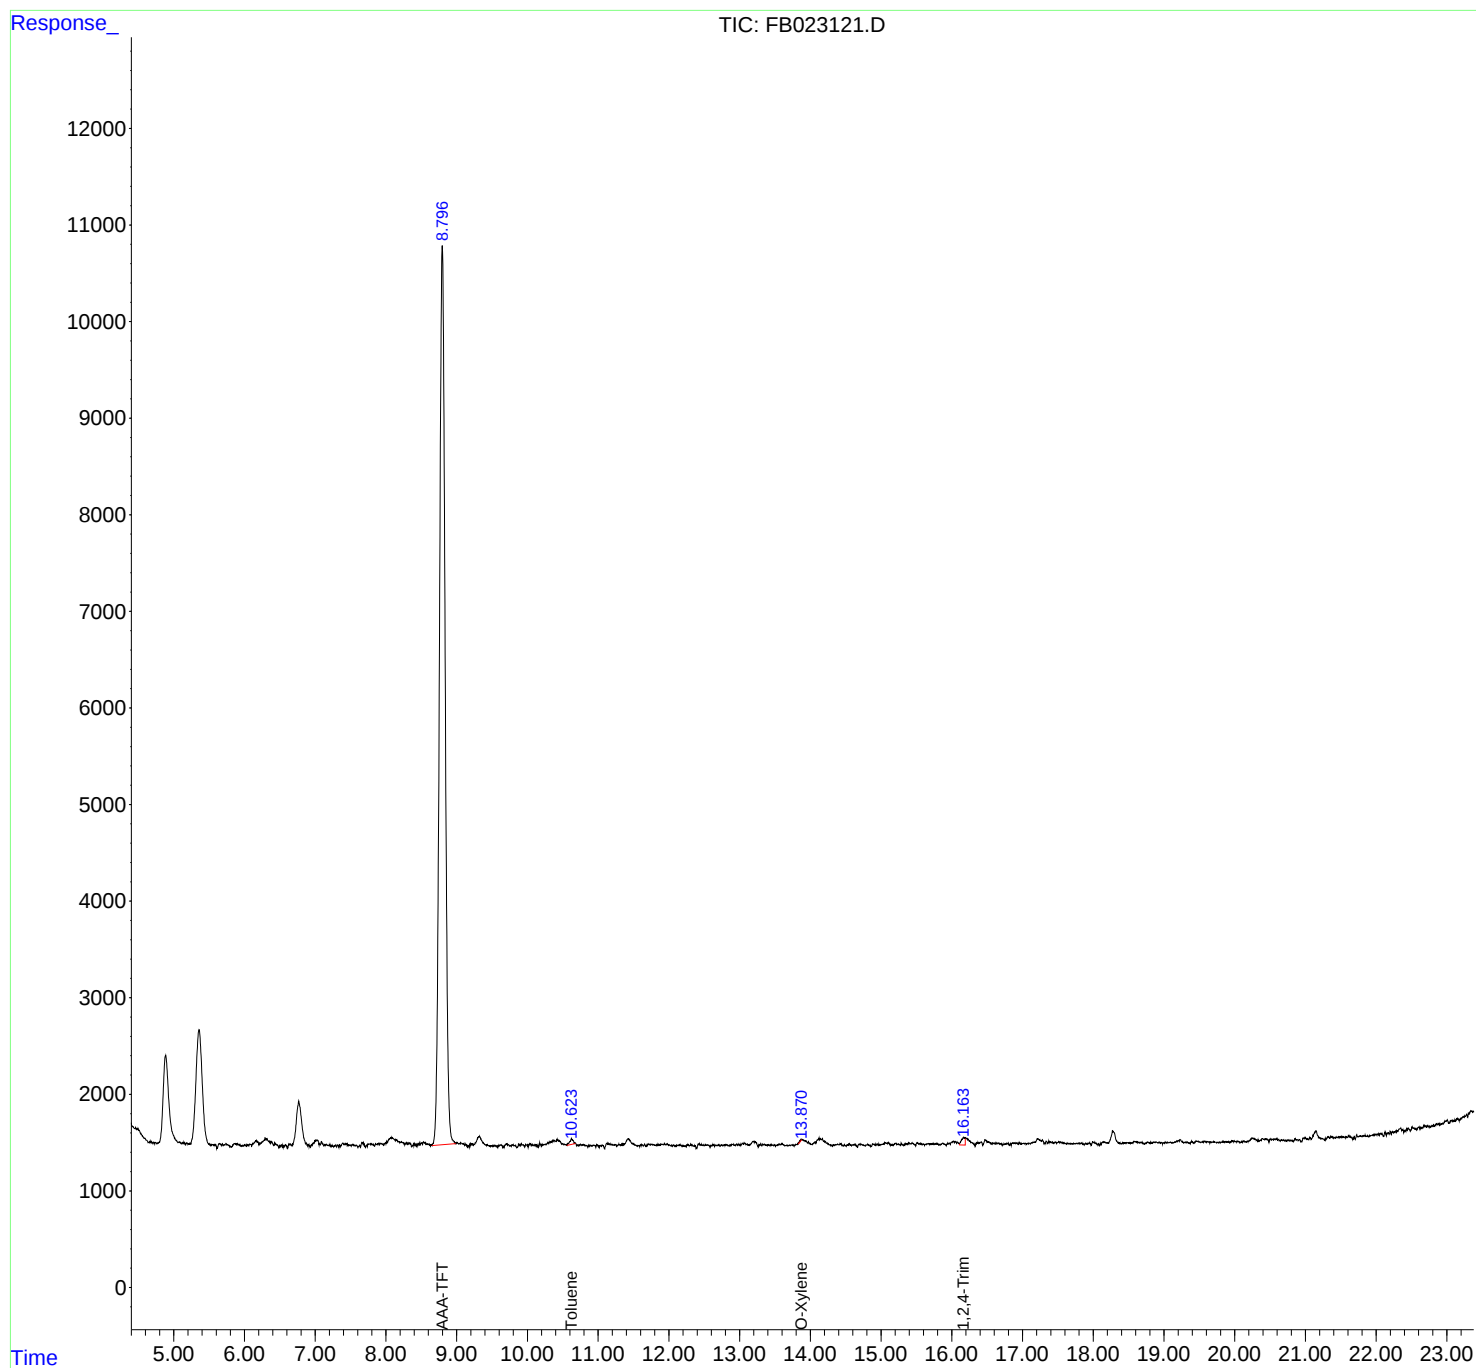


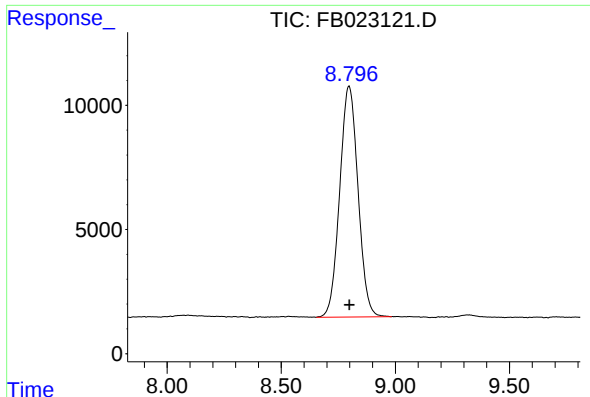

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 519231
Conc: 21.14 ng/ml

Instrument :
FID_B
ClientSampleId :

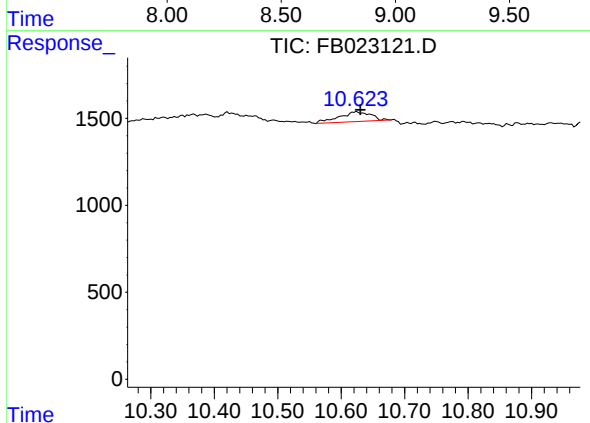


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.006 min
Response: 1922
Conc: 0.05 ng/ml

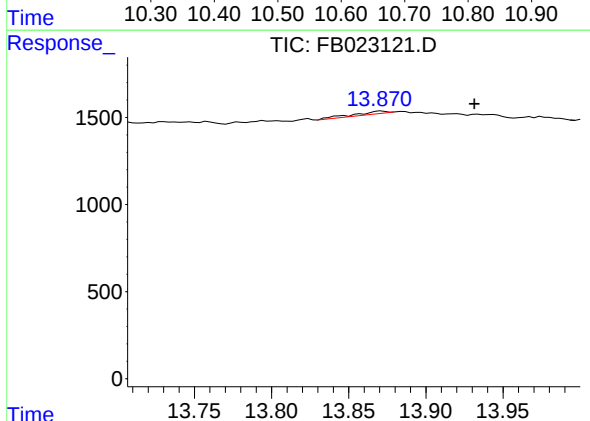

#9 O-Xylene

R.T.: 13.872 min
Delta R.T.: -0.060 min
Response: 212
Conc: 0.01 ng/ml

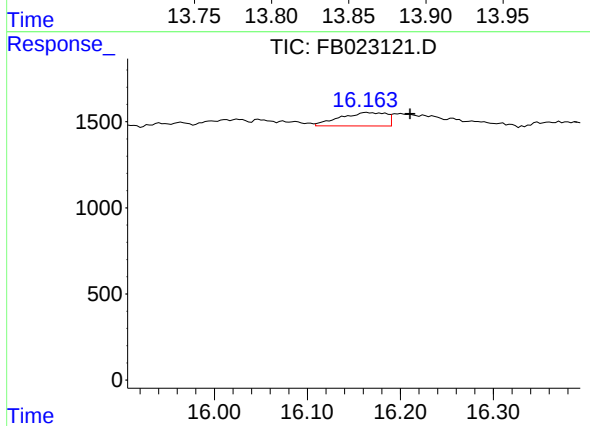

#10 1,2,4-Trimethylbenzene

R.T.: 16.164 min
Delta R.T.: -0.046 min
Response: 2674
Conc: 0.10 ng/ml