

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120219\
 Data File : FB023124.D
 Signal(s) : FID2B.CH
 Acq On : 2 Dec 2019 14:59
 Operator : DD/AJ
 Sample : K6013-02MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 02 14:37:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	523083	21.295 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	1014642	31.049 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1143918	32.805 ng/ml
3) t n-Heptane	7.758	374633	10.896 ng/ml
4) t Benzene	7.893	442200	10.613 ng/ml
6) t Toluene	10.631	1290351	32.031 ng/ml
7) t Ethylbenzene	13.072	410280	10.632 ng/ml
8) t m-Xylene	13.205	783063	21.519 ng/ml
9) t O-Xylene	13.933	750301	21.610 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	620996	22.144 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120219\
Data File : FB023124.D
Signal(s) : FID2B.CH
Acq On : 2 Dec 2019 14:59
Operator : DD/AJ
Sample : K6013-02MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 02 14:37:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

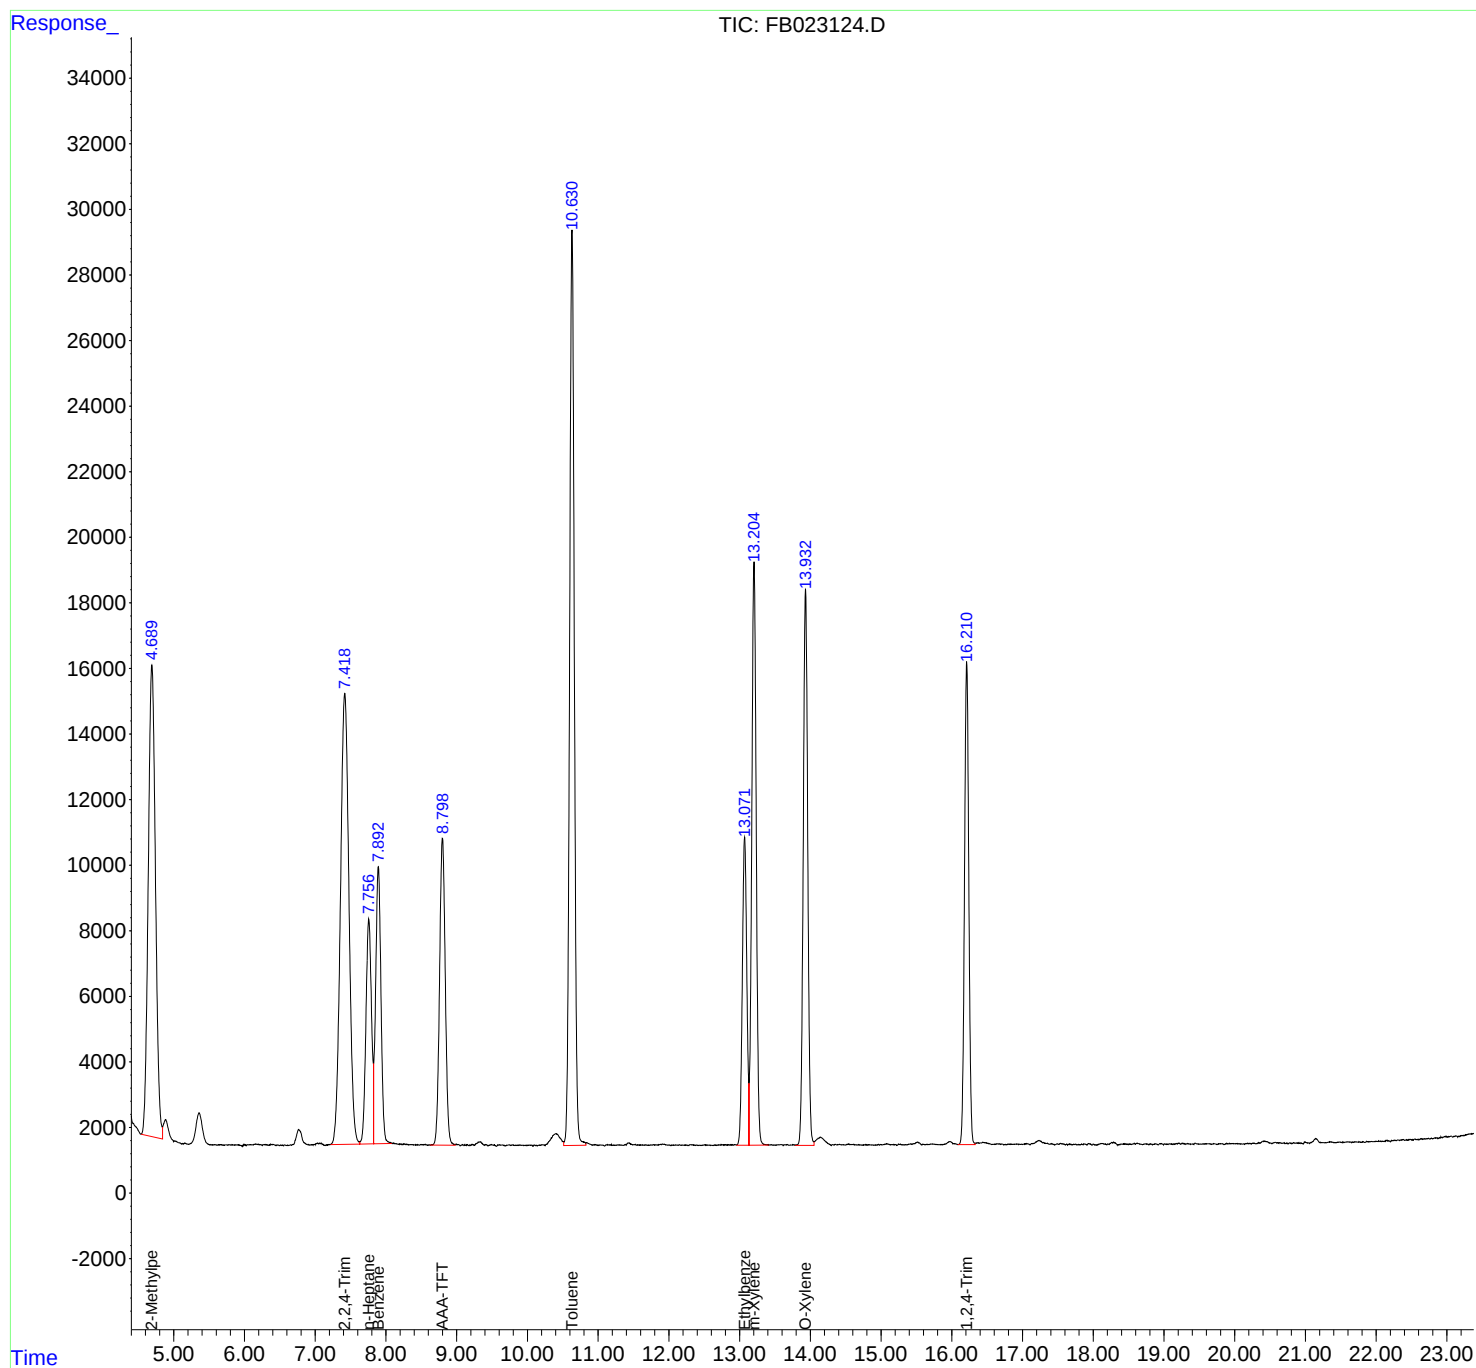


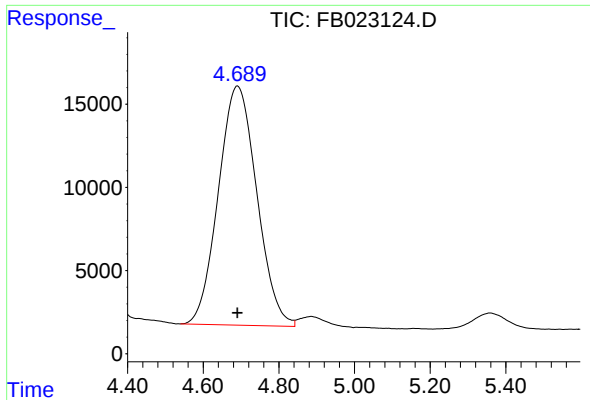

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 1014642
Conc: 31.05 ng/ml

Instrument :
FID_B
ClientSampleId :

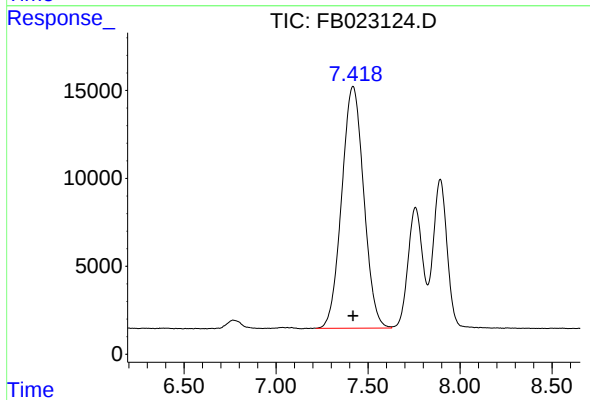


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 1143918
Conc: 32.80 ng/ml

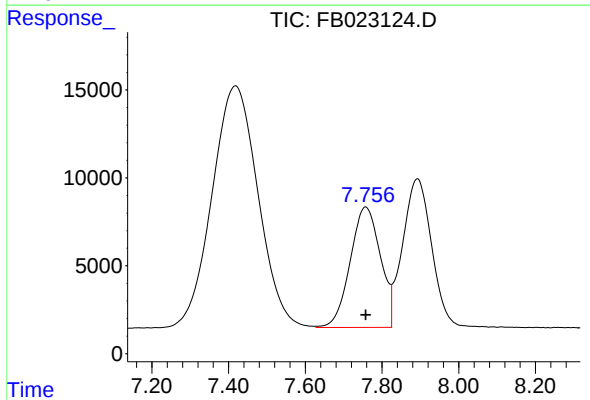


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 374633
Conc: 10.90 ng/ml

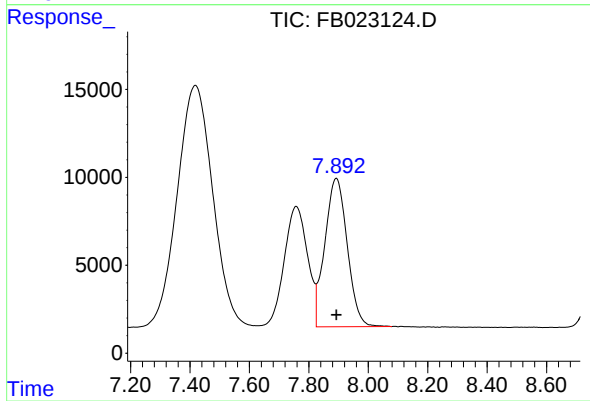

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 442200
Conc: 10.61 ng/ml

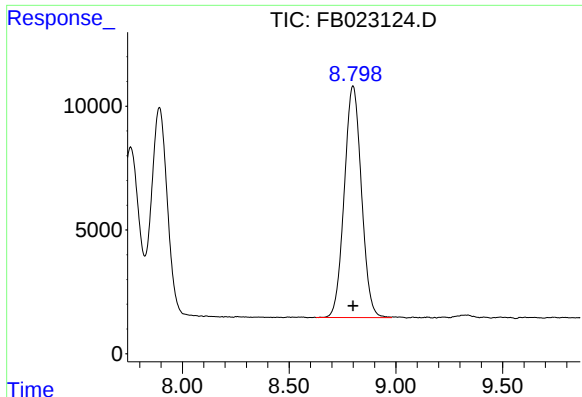

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 523083
Conc: 21.29 ng/ml

Instrument :
FID_B
ClientSampleId :

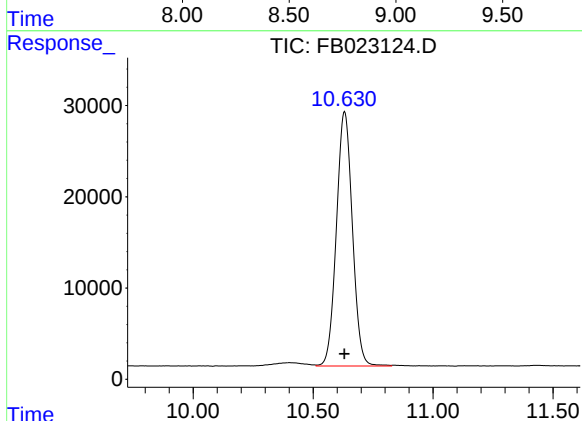


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1290351
Conc: 32.03 ng/ml

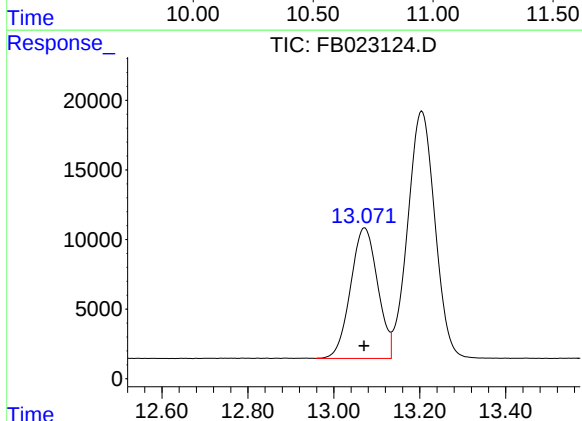


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.001 min
Response: 410280
Conc: 10.63 ng/ml

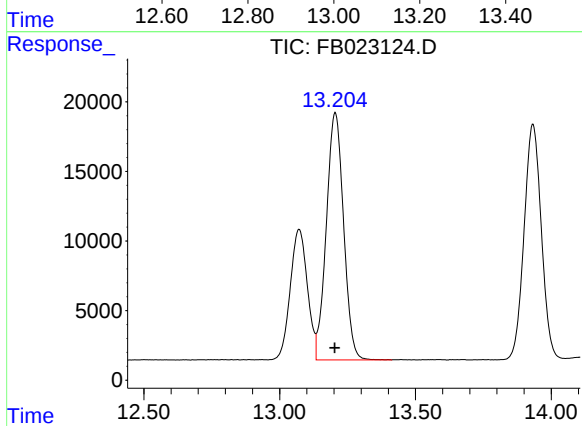

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.002 min
Response: 783063
Conc: 21.52 ng/ml

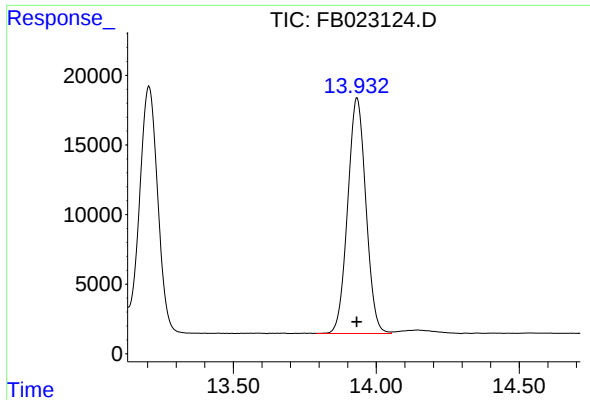

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.001 min
Response: 750301
Conc: 21.61 ng/ml

Instrument :
FID_B
ClientSampleId :

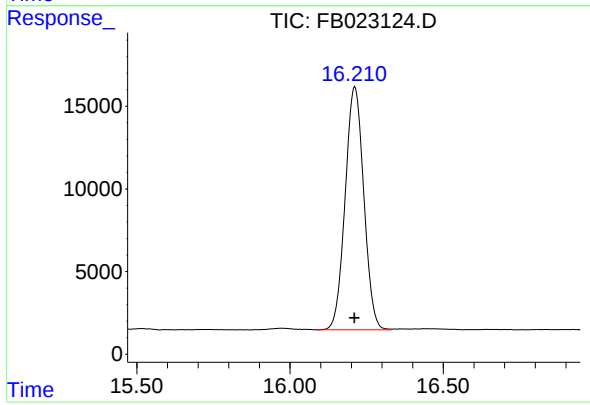

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.001 min
Response: 620996
Conc: 22.14 ng/ml