

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120219\
 Data File : FB023121.D
 Signal(s) : FID2B.CH
 Acq On : 2 Dec 2019 11:49
 Operator : DD/AJ
 Sample : BSF1202S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1202S1

Integration File: Calibration.e
 Quant Time: Dec 02 14:08:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	500547	20.377 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	947102	28.983 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1050957	30.139 ng/ml
3) t n-Heptane	7.757	344098	10.008 ng/ml
4) t Benzene	7.892	406210	9.750 ng/ml
6) t Toluene	10.630	1168354	29.003 ng/ml
7) t Ethylbenzene	13.071	362403	9.392 ng/ml
8) t m-Xylene	13.204	684428	18.808 ng/ml
9) t O-Xylene	13.932	659299	18.989 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	548171	19.547 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120219\
Data File : FB023121.D
Signal(s) : FID2B.CH
Acq On : 2 Dec 2019 11:49
Operator : DD/AJ
Sample : BSF1202S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1202S1

Integration File: Calibration.e
Quant Time: Dec 02 14:08:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

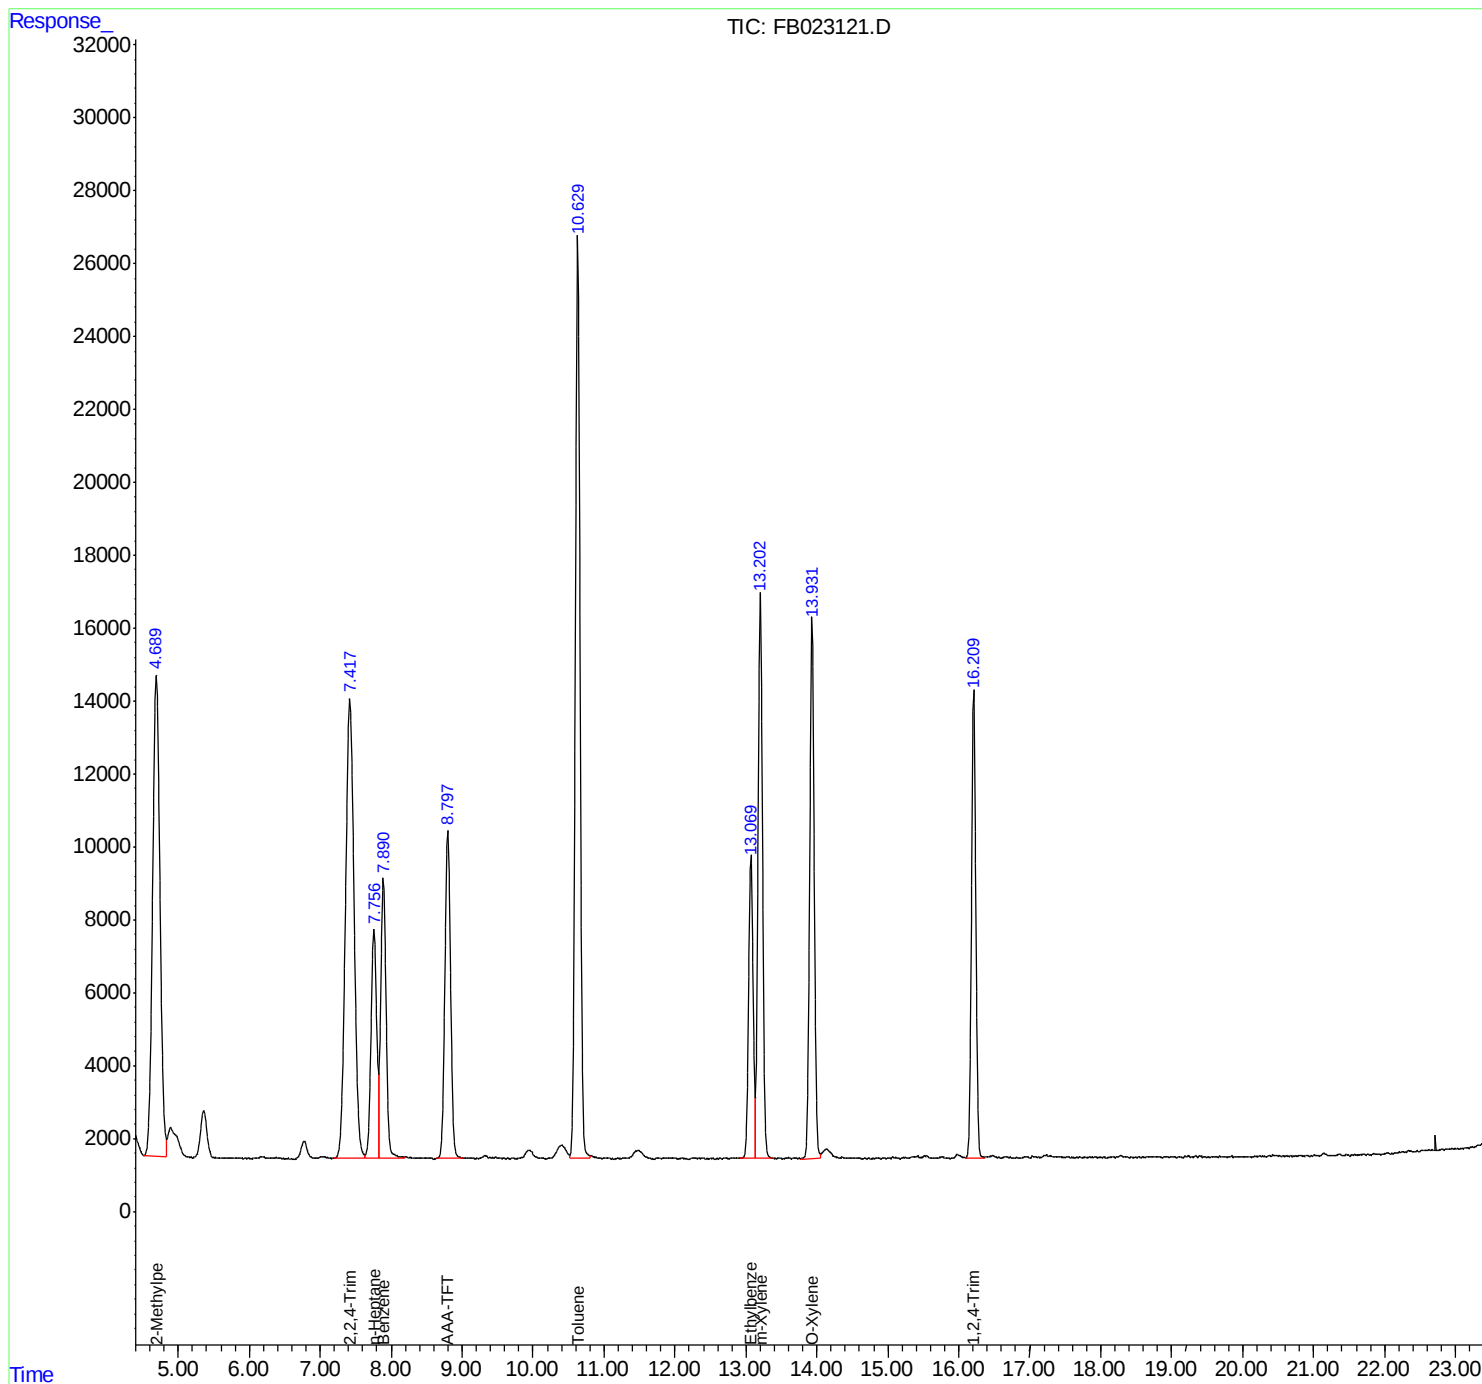


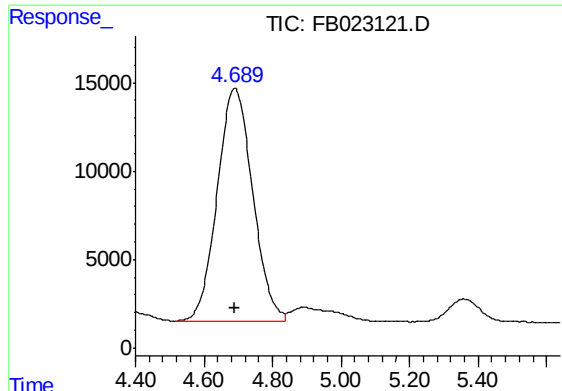

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 947102
Conc: 28.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1202S1

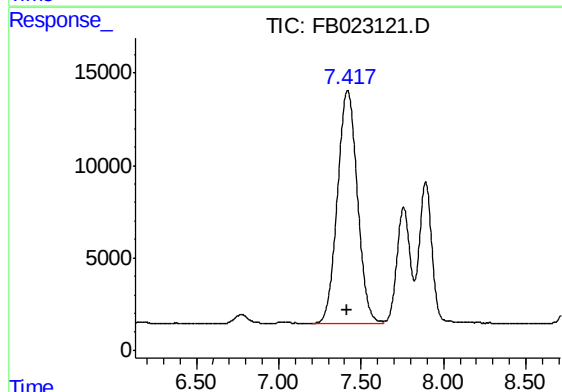


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1050957
Conc: 30.14 ng/ml

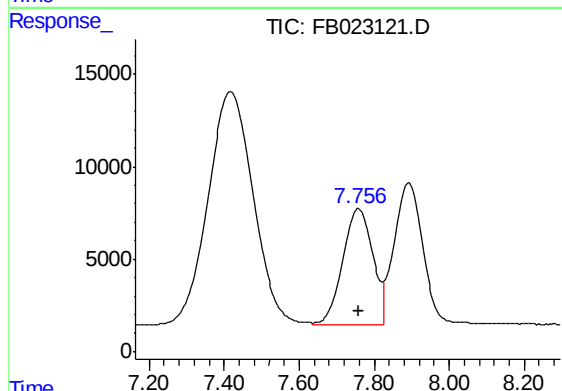


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 344098
Conc: 10.01 ng/ml

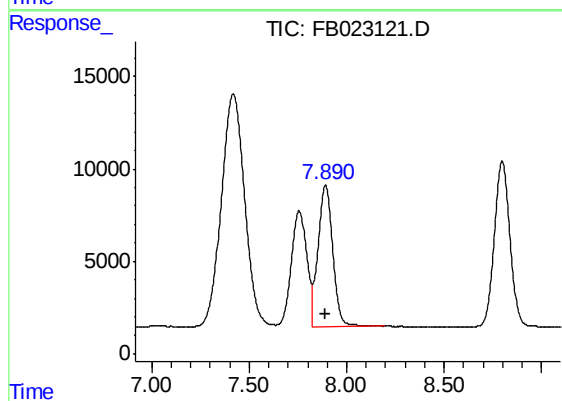

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 406210
Conc: 9.75 ng/ml

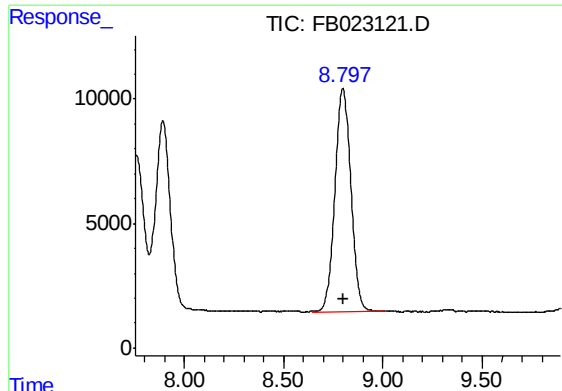

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 500547
Conc: 20.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1202S1

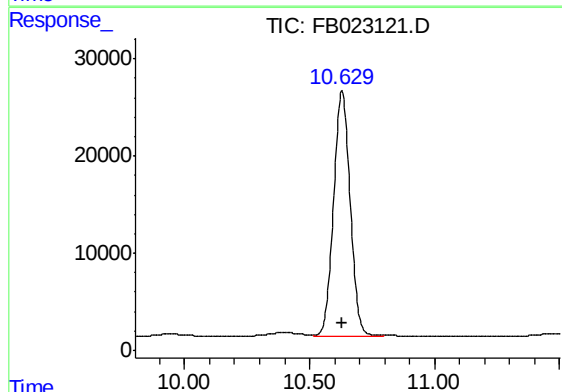


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1168354
Conc: 29.00 ng/ml

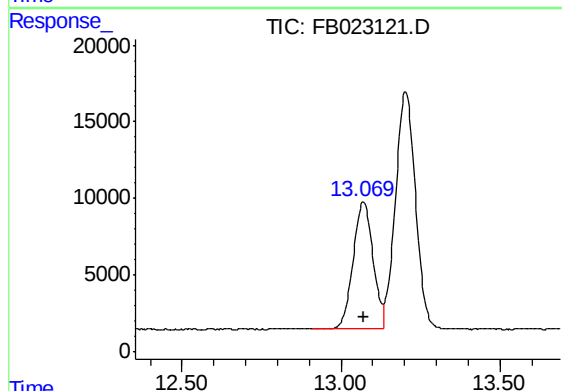


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 362403
Conc: 9.39 ng/ml

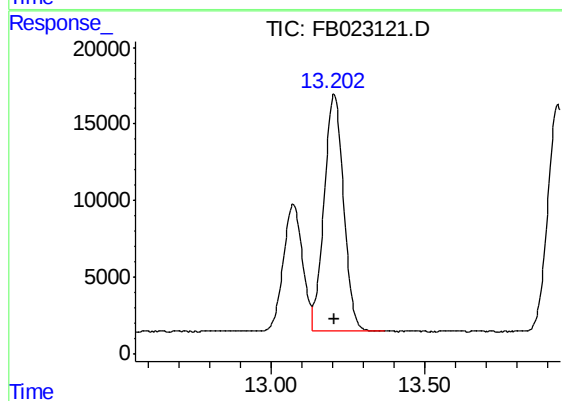

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 684428
Conc: 18.81 ng/ml

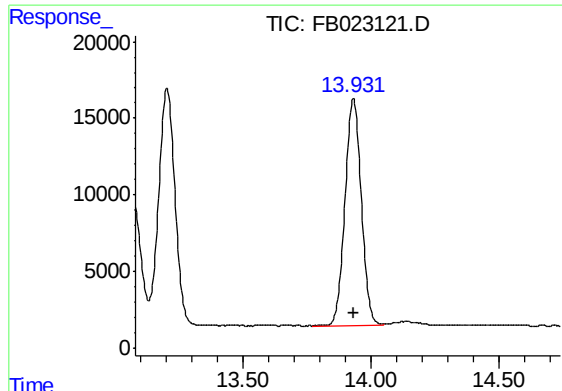

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 659299
Conc: 18.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1202S1

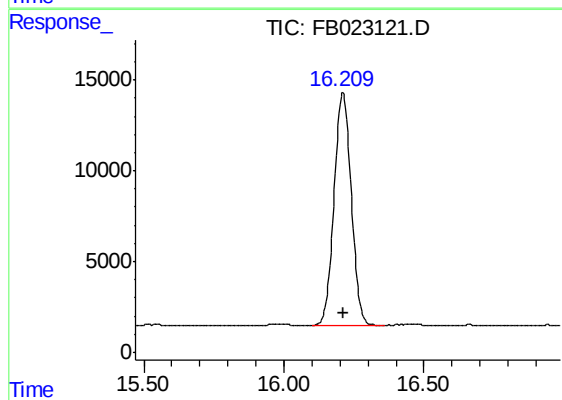

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 548171
Conc: 19.55 ng/ml