

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120220\
 Data File : FB025304.D
 Signal(s) : FID2B.CH
 Acq On : 2 Dec 2020 11:46
 Operator : DD/AJ
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 02 14:24:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 14:22:34 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	101942	4.816 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	222053	7.235 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	210836	6.826 ng/ml
3) t n-Heptane	7.757	66500	2.187 ng/ml
4) t Benzene	7.891	87572	2.312 ng/ml
6) t Toluene	10.630	257377	7.246 ng/ml
7) t Ethylbenzene	13.070	83394	2.617 ng/ml
8) t m-Xylene	13.203	165682	5.142 ng/ml
9) t O-Xylene	13.932	161192	5.088 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	133093	4.923 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120220\
Data File : FB025304.D
Signal(s) : FID2B.CH
Acq On : 2 Dec 2020 11:46
Operator : DD/AJ
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 02 14:24:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 14:22:34 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

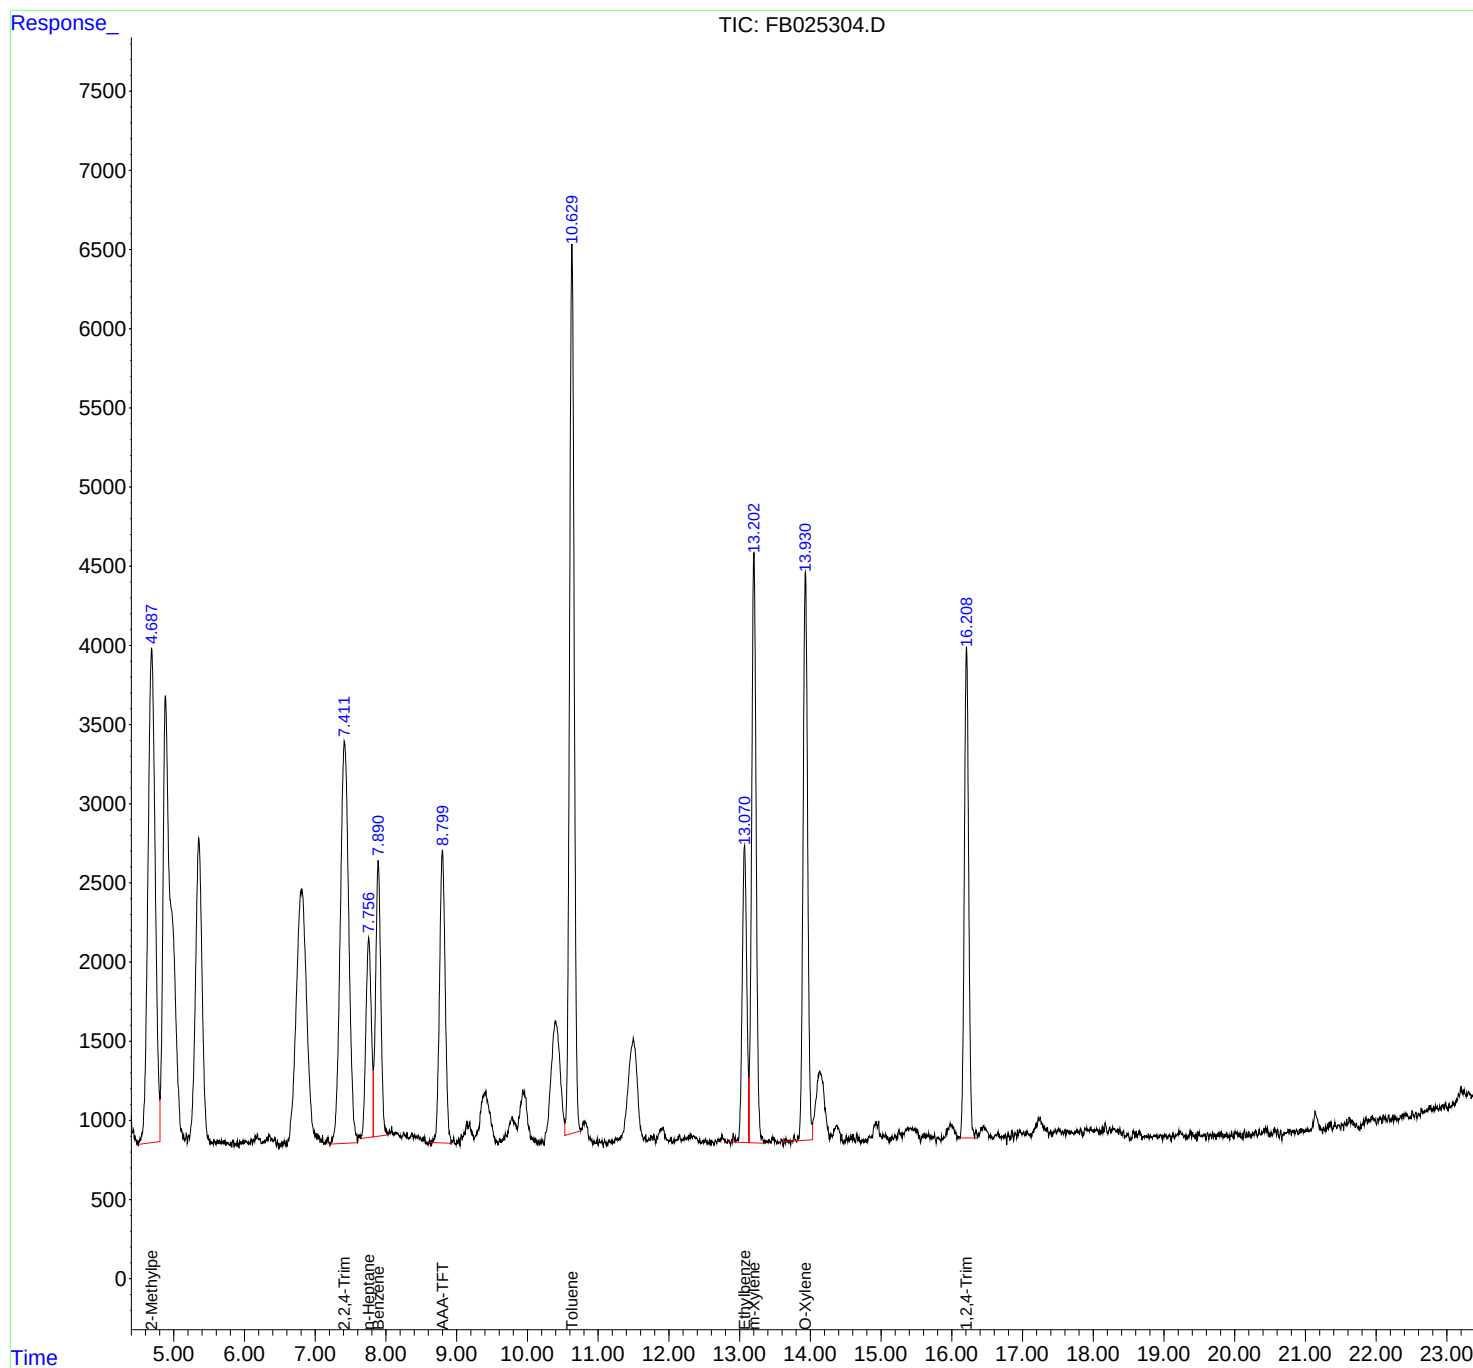


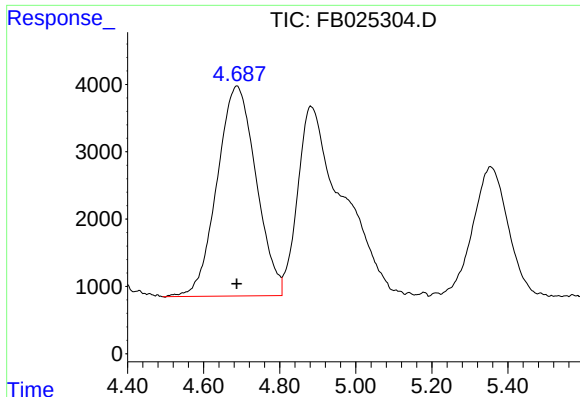

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.001 min
Response: 222053
Conc: 7.23 ng/ml

Instrument :
FID_B
ClientSampleId :

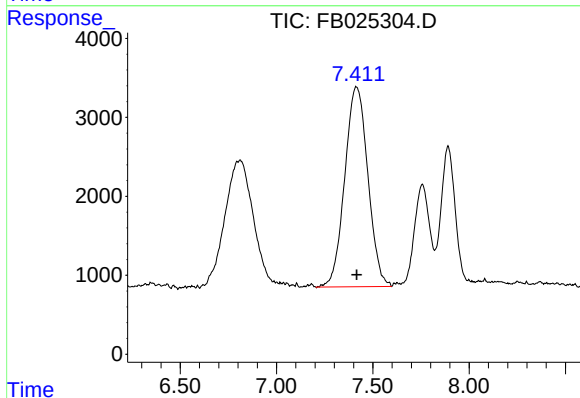


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.005 min
Response: 210836
Conc: 6.83 ng/ml

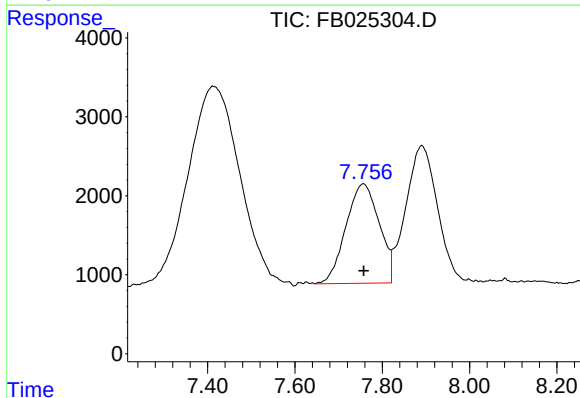


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 66500
Conc: 2.19 ng/ml

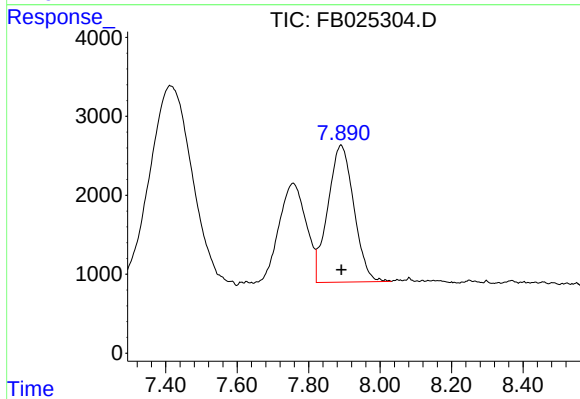

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 87572
Conc: 2.31 ng/ml

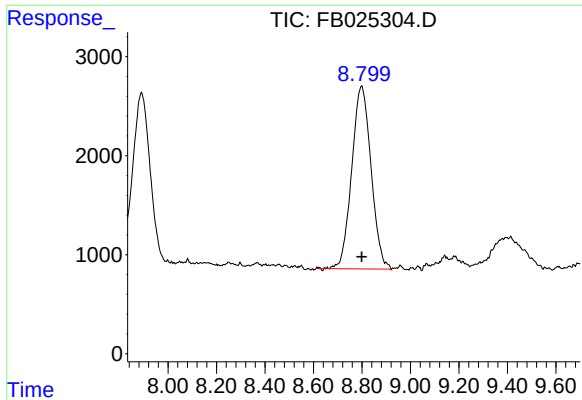

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 101942
Conc: 4.82 ng/ml

Instrument :
FID_B
ClientSampleId :

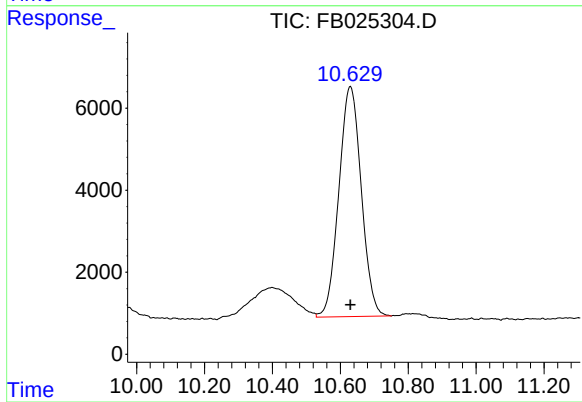


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 257377
Conc: 7.25 ng/ml

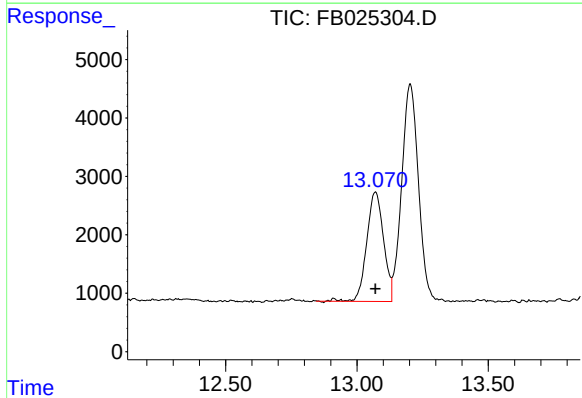


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 83394
Conc: 2.62 ng/ml

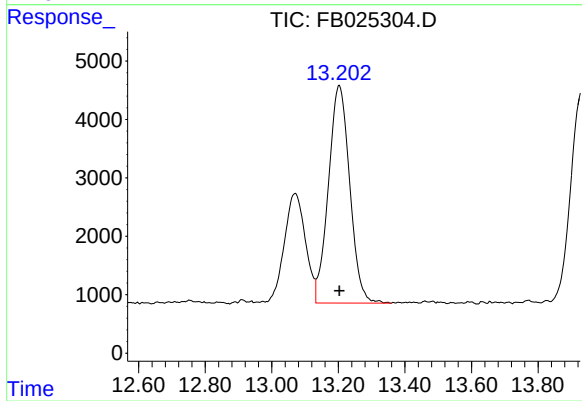

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 165682
Conc: 5.14 ng/ml

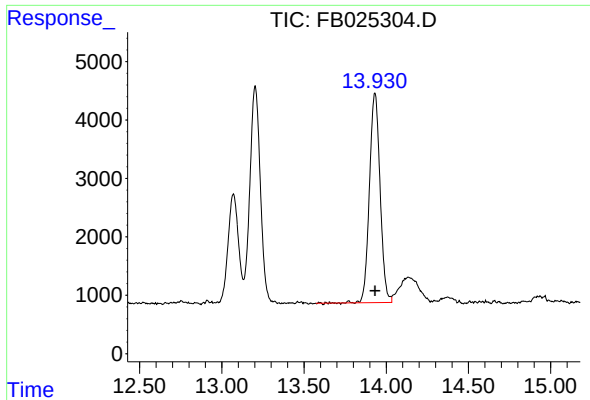

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 161192
Conc: 5.09 ng/ml

Instrument :
FID_B
ClientSampleId :

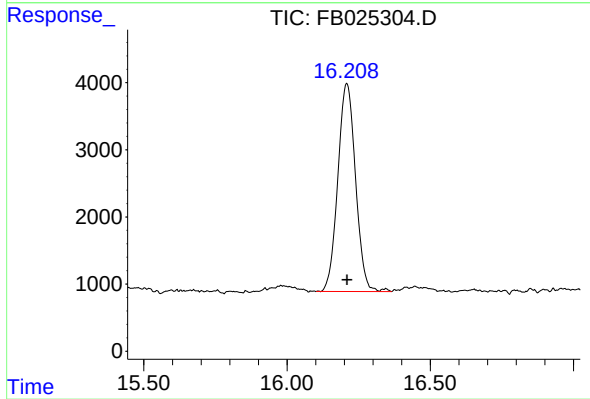

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 133093
Conc: 4.92 ng/ml