

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120220\
 Data File : FB025307.D
 Signal(s) : FID2B.CH
 Acq On : 2 Dec 2020 13:17
 Operator : DD/AJ
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 02 14:24:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 14:22:34 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	1049389	49.578 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	2289572	74.596 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	2411706	78.079 ng/ml
3) t n-Heptane	7.757	798029	26.248 ng/ml
4) t Benzene	7.892	954040	25.185 ng/ml
6) t Toluene	10.631	2711174	76.334 ng/ml
7) t Ethylbenzene	13.071	826180	25.929 ng/ml
8) t m-Xylene	13.204	1617476	50.195 ng/ml
9) t O-Xylene	13.932	1590400	50.199 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	1418195	52.455 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120220\
Data File : FB025307.D
Signal(s) : FID2B.CH
Acq On : 2 Dec 2020 13:17
Operator : DD/AJ
Sample : 50 GRO STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 02 14:24:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 14:22:34 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

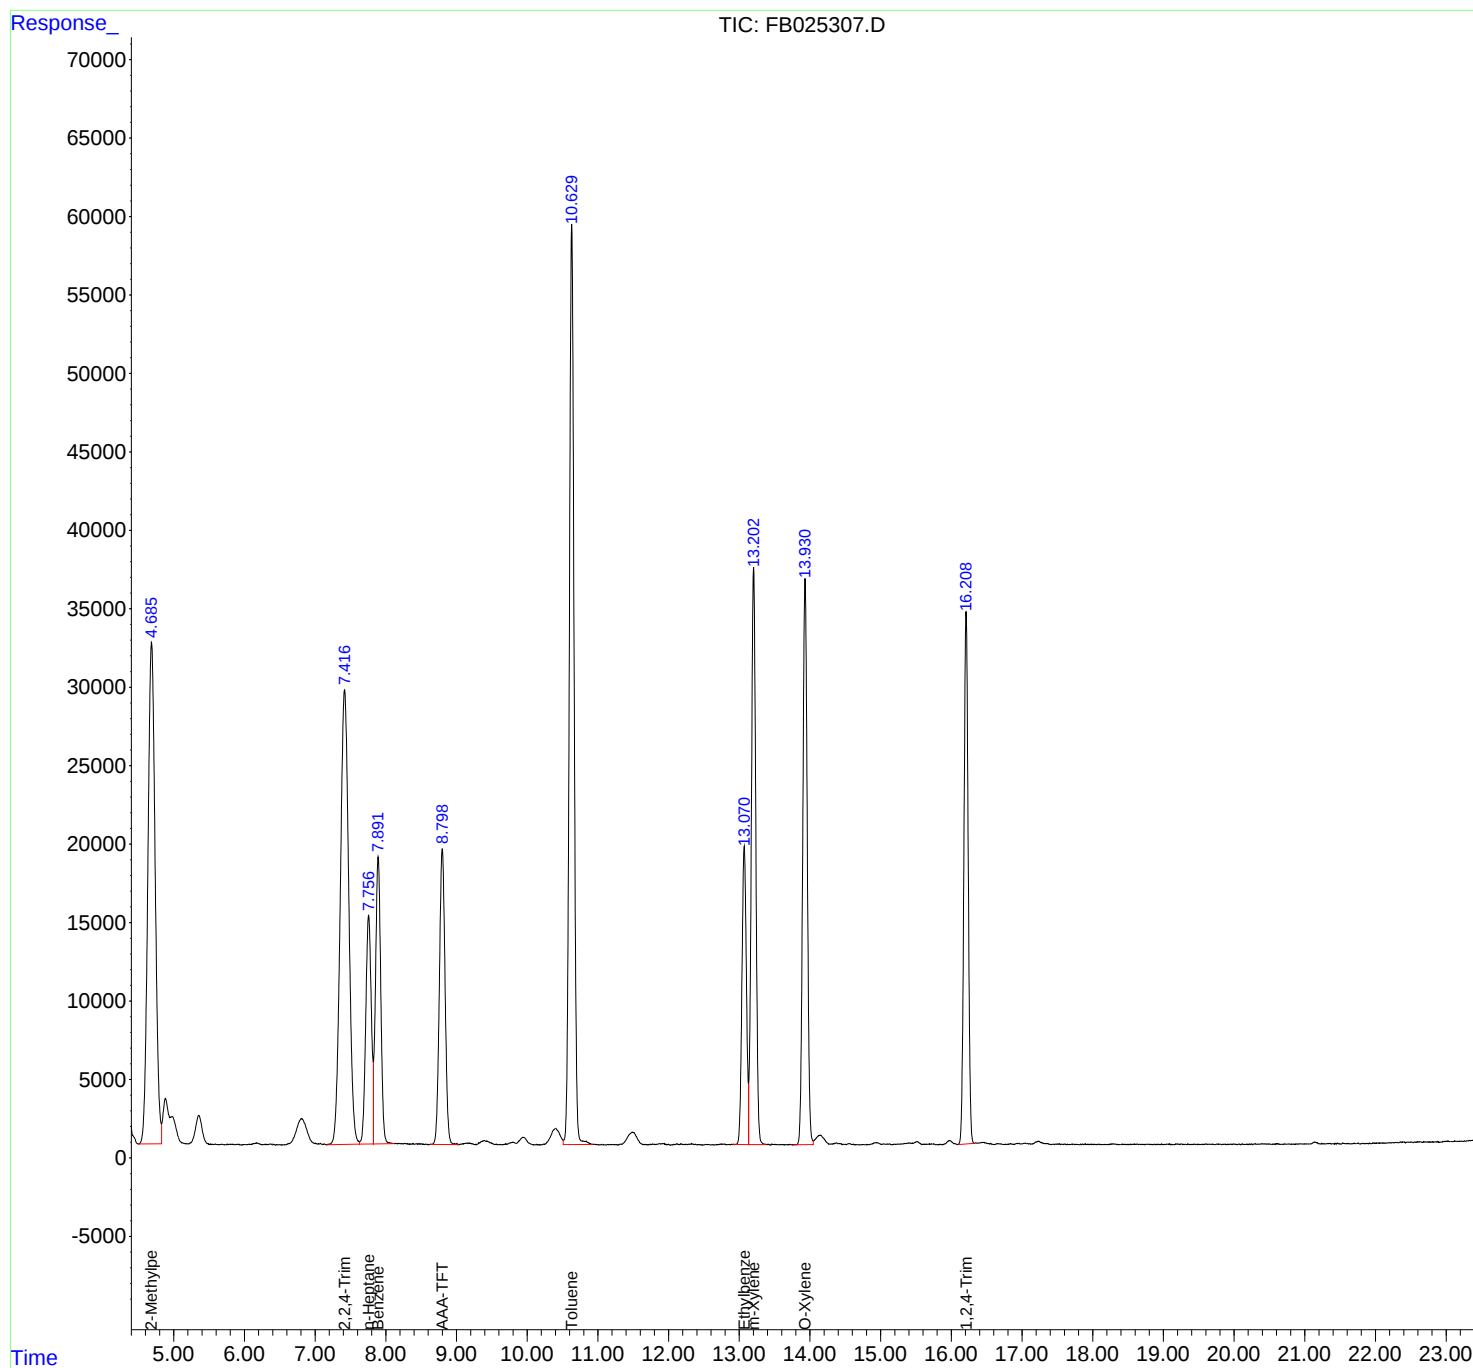


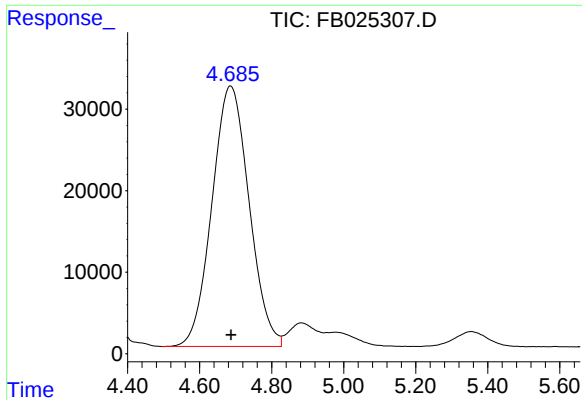

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: 0.000 min
Response: 2289572
Conc: 74.60 ng/ml

Instrument :
FID_B
ClientSampleId :

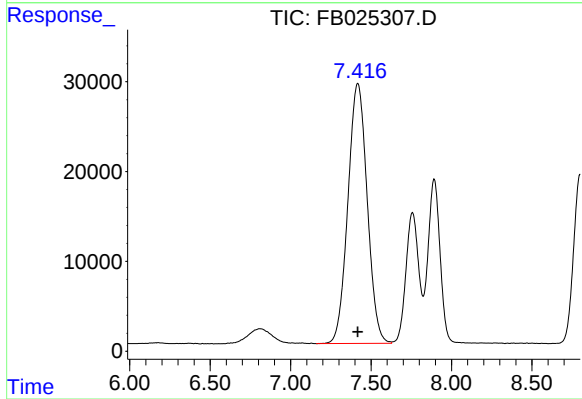


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 2411706
Conc: 78.08 ng/ml

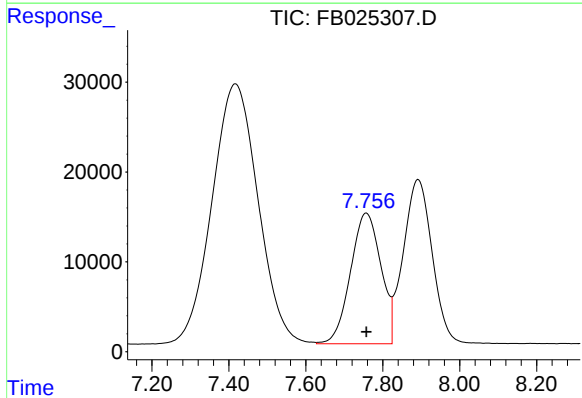


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 798029
Conc: 26.25 ng/ml

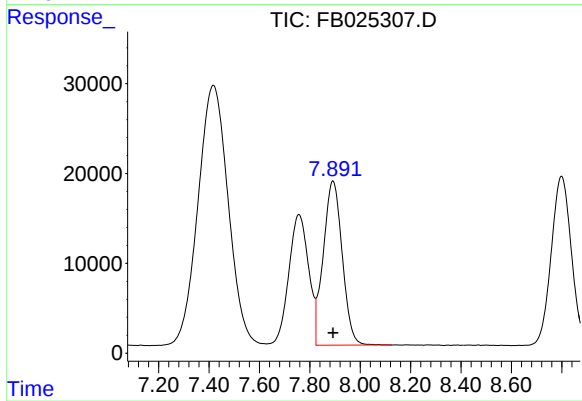

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 954040
Conc: 25.18 ng/ml

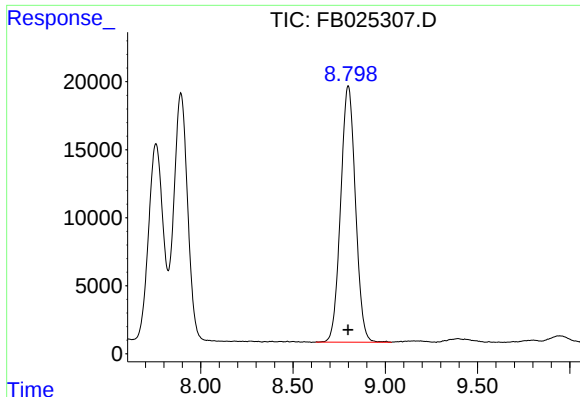

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 1049389
Conc: 49.58 ng/ml

Instrument :
FID_B
ClientSampleId :

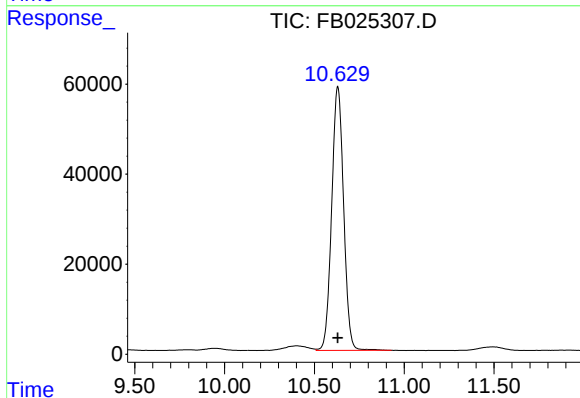


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 2711174
Conc: 76.33 ng/ml

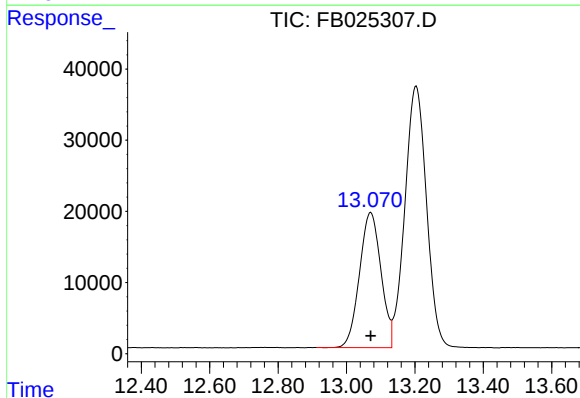


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 826180
Conc: 25.93 ng/ml

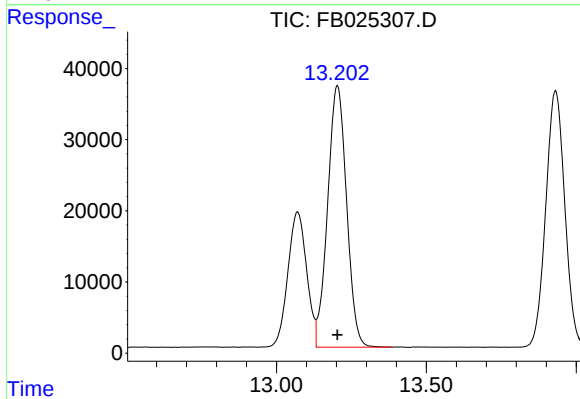

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 1617476
Conc: 50.20 ng/ml

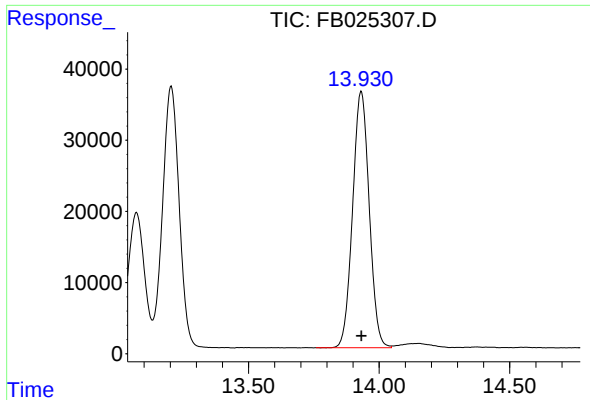

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 1590400
Conc: 50.20 ng/ml

Instrument :
FID_B
ClientSampleId :

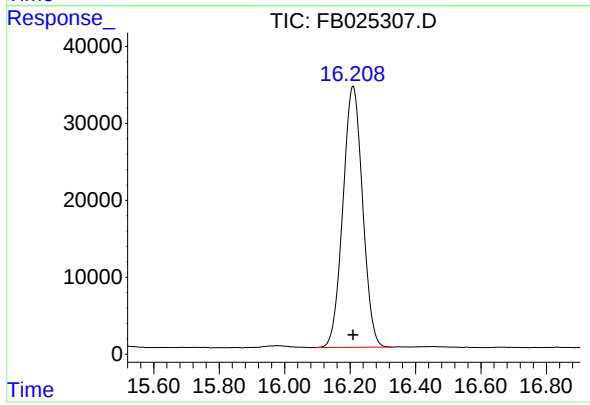

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 1418195
Conc: 52.46 ng/ml