

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD120720AL\
 Data File : FD035749.D
 Signal(s) : FID2B.CH
 Acq On : 07 Dec 2020 7:33
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 07 13:04:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 112720.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 05:38:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) T n-Docosane (C22)	13.673	153540	1.162 ug/ml
14) T n-Tetracosane (C24)	14.776	385572	2.937 ug/ml
15) T n-Hexacosane (C26)	15.793	172128	1.347 ug/ml
16) T n-Octacosane (C28)	16.739	141827	1.143 ug/ml
17) T n-Tricontane (C30)	17.622	133007	1.130 ug/ml
18) T n-Dotriacontane (C32)	18.468	391308	3.707 ug/ml
19) T n-Tetratriacontane (C34)	19.230	98945	1.033 ug/ml
20) T n-Hexatriacontane (C36)	20.013	523616	5.903 ug/ml
22) T n-Tetracontane (C40)	21.596	436630	5.186 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD120720AL\
Data File : FD035749.D
Signal(s) : FID2B.CH
Acq On : 07 Dec 2020 7:33
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_B
ClientSampled :

Integration File: autoint1.e
Quant Time: Dec 07 13:04:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 112720.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 05:38:14 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

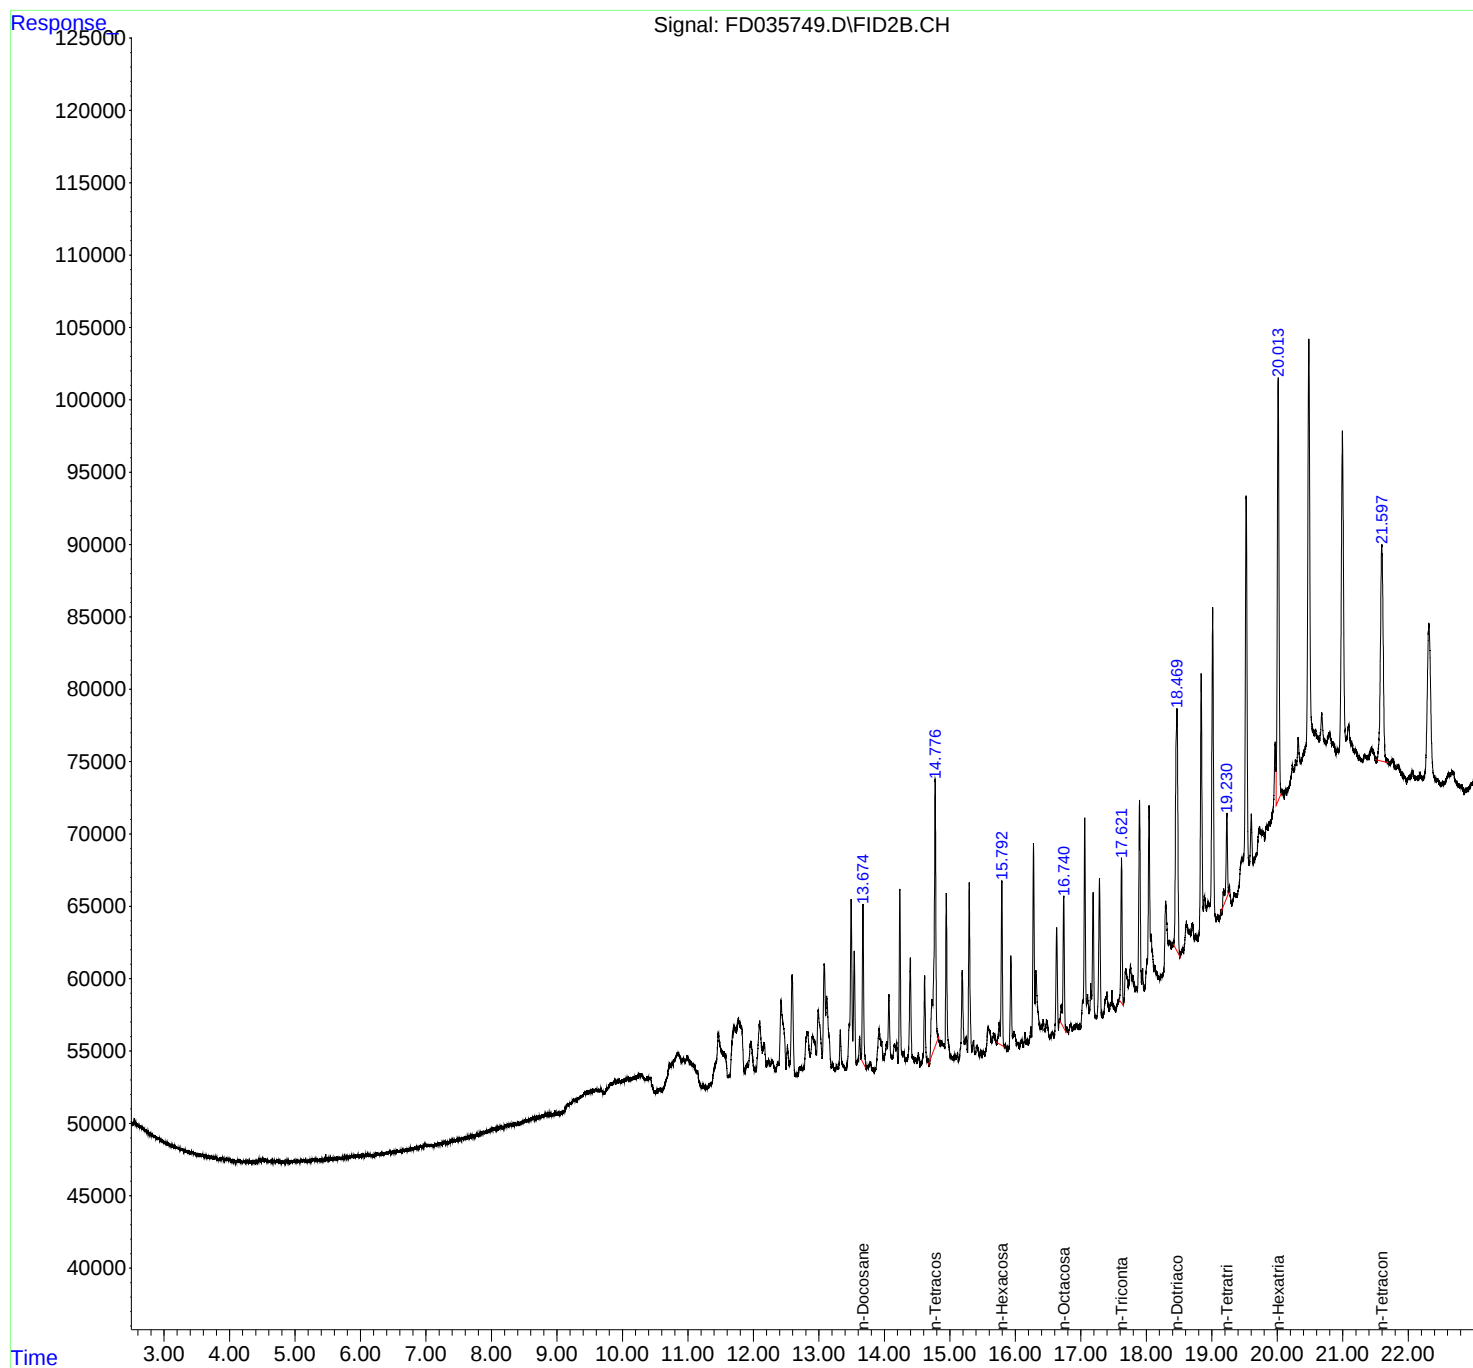


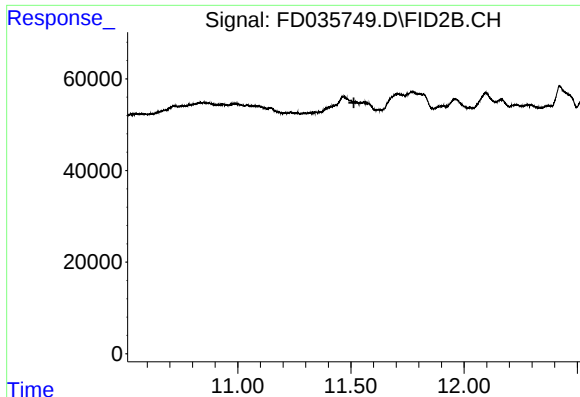

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.513 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :

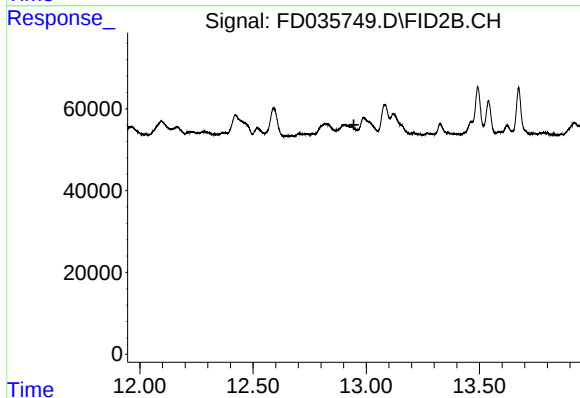


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.945 min
Response: 0
Conc: N.D.

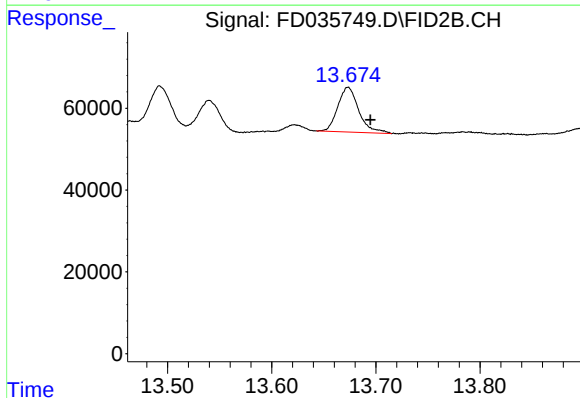


#13 n-Docosane (C22)

R.T.: 13.673 min
Delta R.T.: -0.022 min
Response: 153540
Conc: 1.16 ug/ml

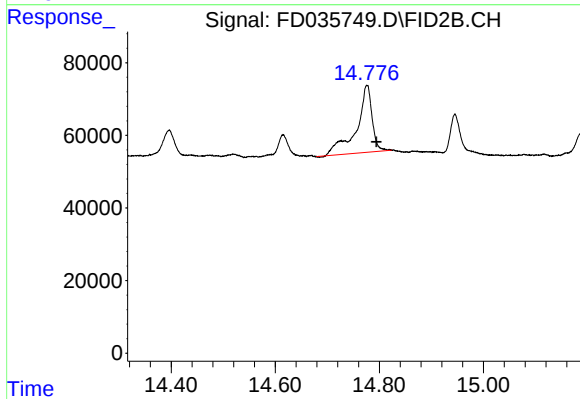

#14 n-Tetracosane (C24)


R.T.: 14.776 min
Delta R.T.: -0.018 min
Response: 385572
Conc: 2.94 ug/ml

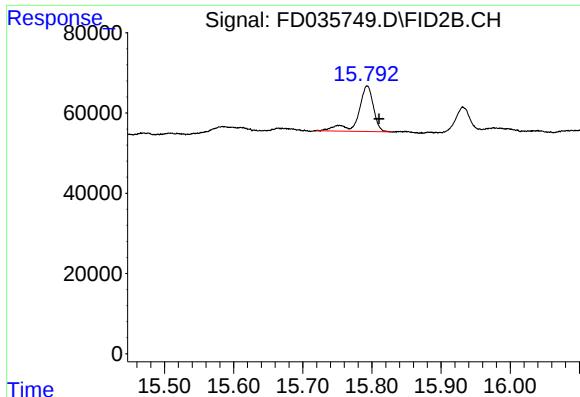

#15 n-Hexacosane (C26)


R.T.: 15.793 min
Delta R.T.: -0.017 min
Response: 172128
Conc: 1.35 ug/ml

Instrument :
FID_B
ClientSampleId :

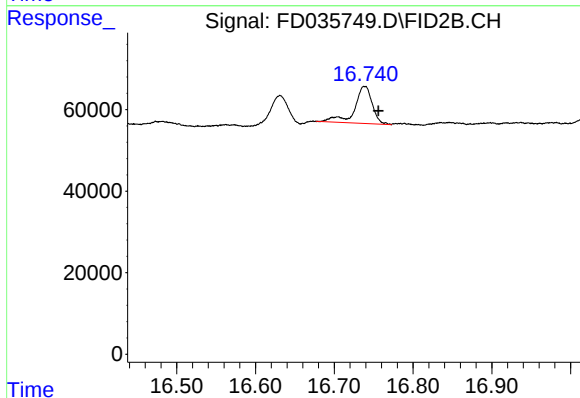


#16 n-Octacosane (C28)

R.T.: 16.739 min
Delta R.T.: -0.017 min
Response: 141827
Conc: 1.14 ug/ml

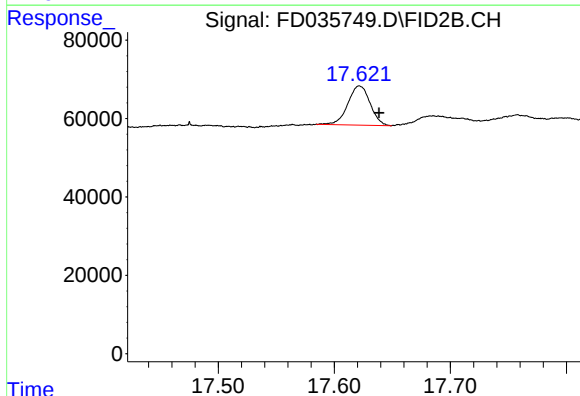


#17 n-Tricontane (C30)

R.T.: 17.622 min
Delta R.T.: -0.017 min
Response: 133007
Conc: 1.13 ug/ml

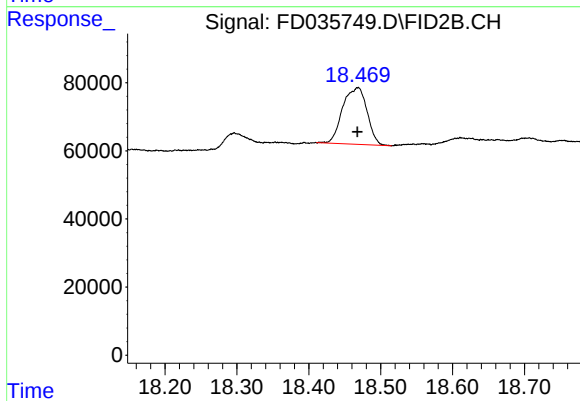

#18 n-Dotriacontane (C32)


R.T.: 18.468 min
Delta R.T.: 0.001 min
Response: 391308
Conc: 3.71 ug/ml

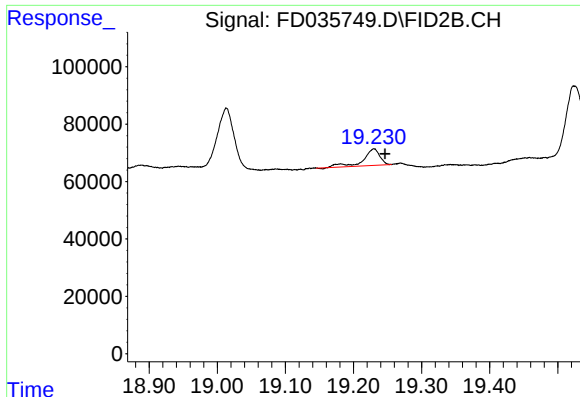

#19 n-Tetratriacontane (C34)


R.T.: 19.230 min
Delta R.T.: -0.016 min
Response: 98945
Conc: 1.03 ug/ml

Instrument :
FID_B
ClientSampleId :

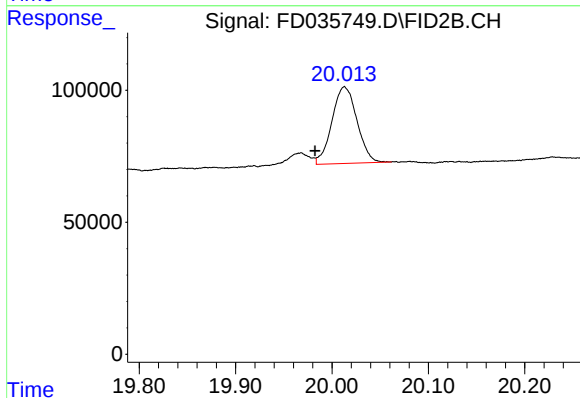

#20 n-Hexatriacontane (C36)

R.T.: 20.013 min
Delta R.T.: 0.030 min
Response: 523616
Conc: 5.90 ug/ml

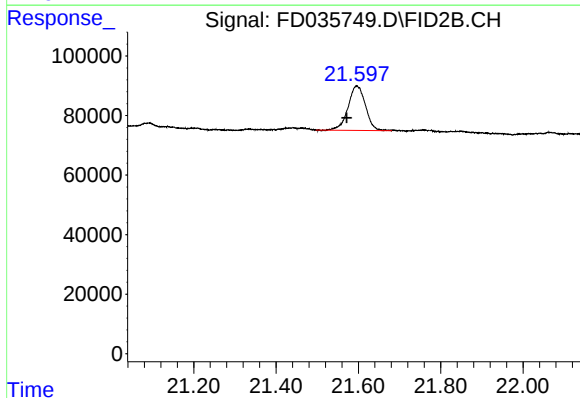

#22 n-Tetracontane (C40)

R.T.: 21.596 min
Delta R.T.: 0.024 min
Response: 436630
Conc: 5.19 ug/ml