

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120220\
 Data File : FB025309.D
 Signal(s) : FID2B.CH
 Acq On : 2 Dec 2020 15:27
 Operator : DD/AJ
 Sample : FB120220GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB120220GROICV

Integration File: Calibration.e
 Quant Time: Dec 02 15:59:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	412527	19.623 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	933603	31.054 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	933176	31.014 ng/ml
3) t n-Heptane	7.757	307189	10.374 ng/ml
4) t Benzene	7.892	392135	10.602 ng/ml
6) t Toluene	10.631	1098639	31.264 ng/ml
7) t Ethylbenzene	13.071	338203	10.354 ng/ml
8) t m-Xylene	13.204	675703	20.877 ng/ml
9) t O-Xylene	13.932	663815	20.998 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	566340	20.856 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120220\
Data File : FB025309.D
Signal(s) : FID2B.CH
Acq On : 2 Dec 2020 15:27
Operator : DD/AJ
Sample : FB120220GROICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB120220GROICV

Integration File: Calibration.e
Quant Time: Dec 02 15:59:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

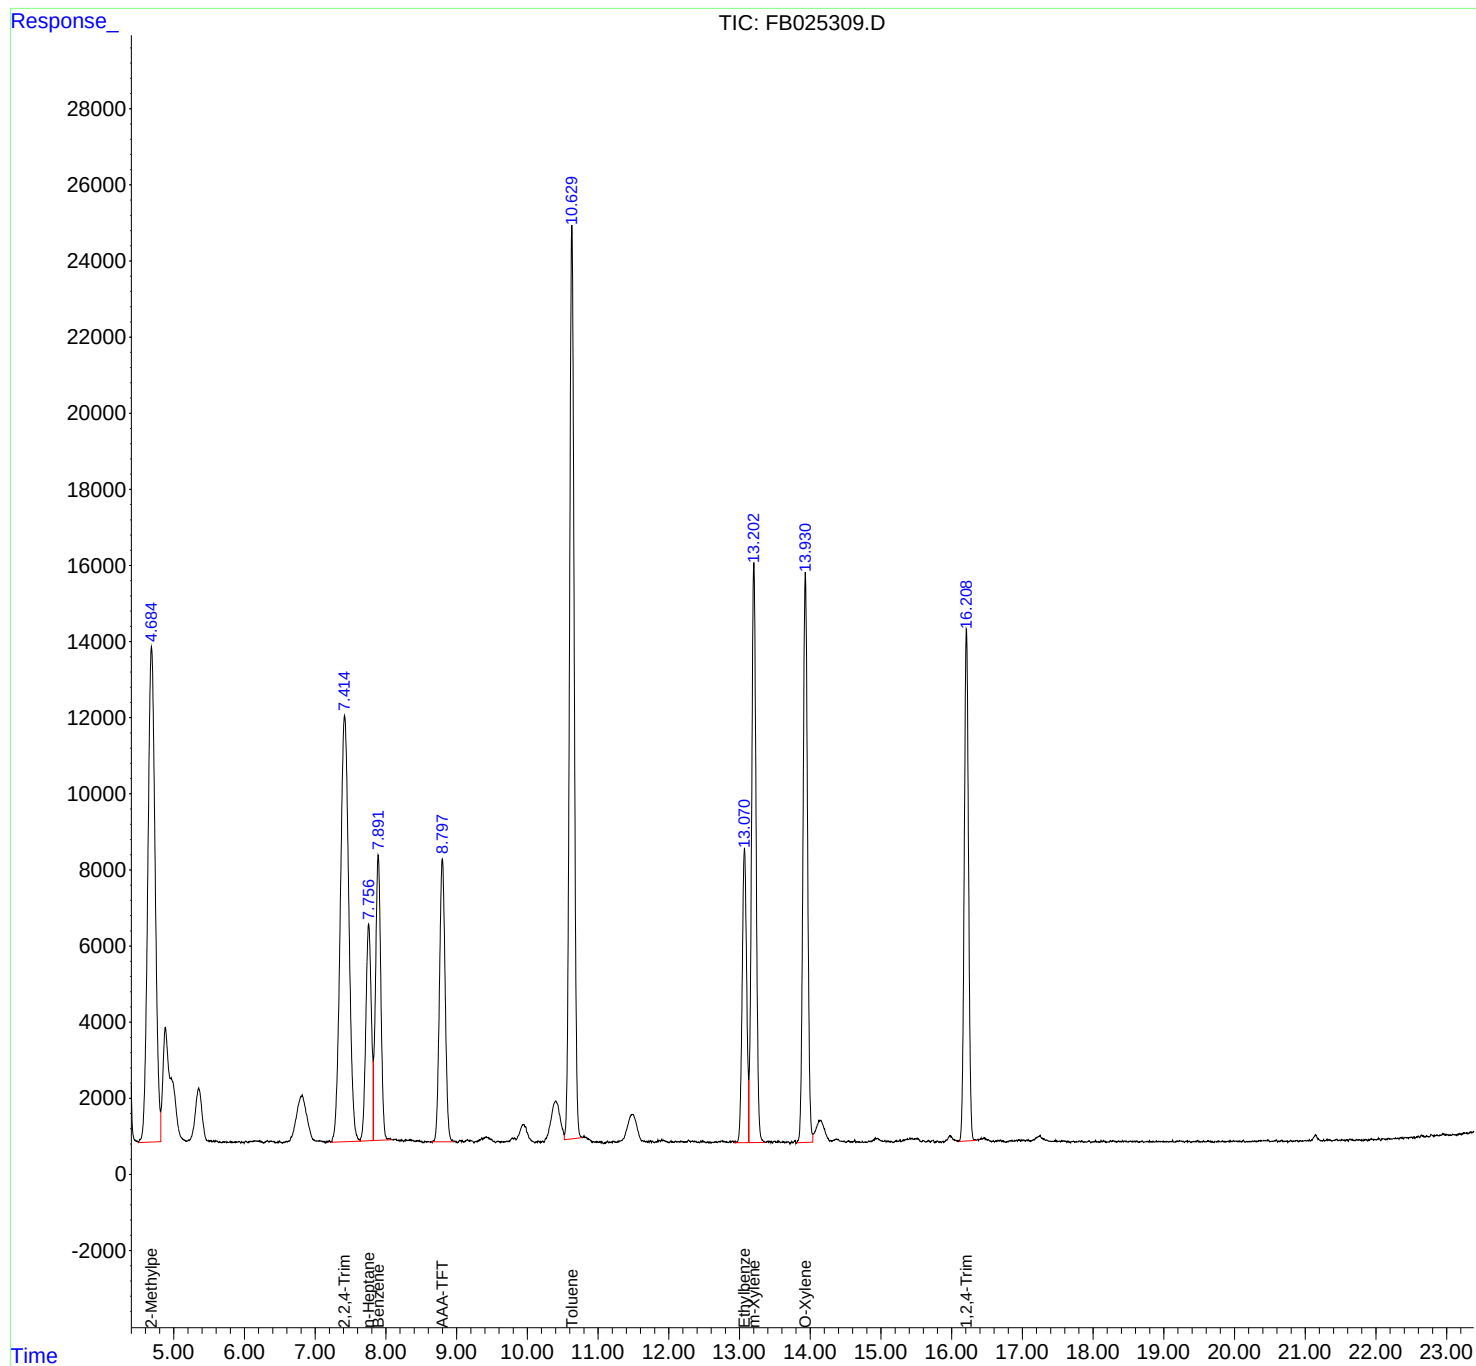


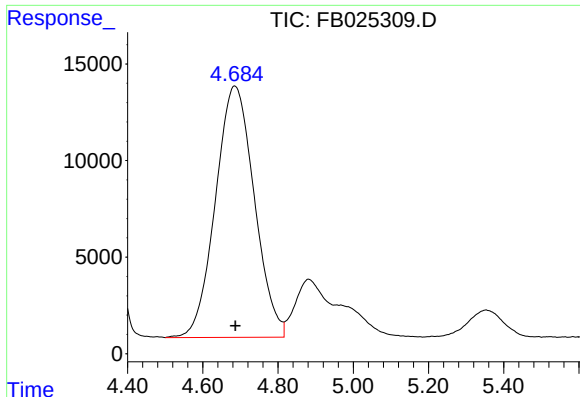

#1 2-Methylpentane


R.T.: 4.685 min
Delta R.T.: -0.002 min
Response: 933603
Conc: 31.05 ng/ml

Instrument :
FID_B
ClientSampleId :
FB120220GROICV

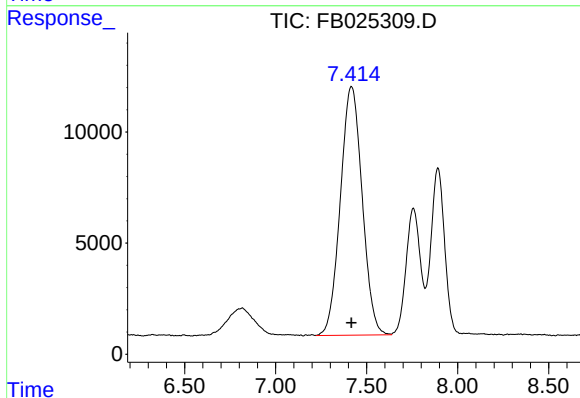


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 933176
Conc: 31.01 ng/ml

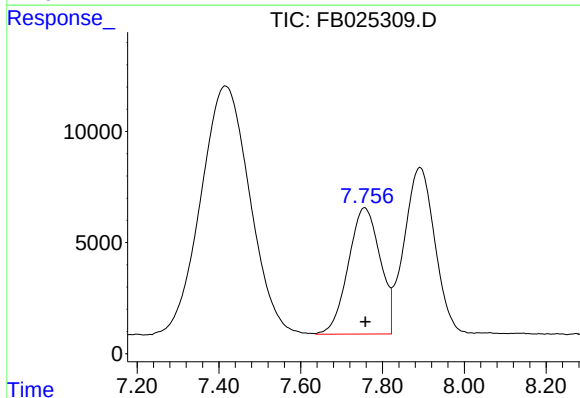


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 307189
Conc: 10.37 ng/ml

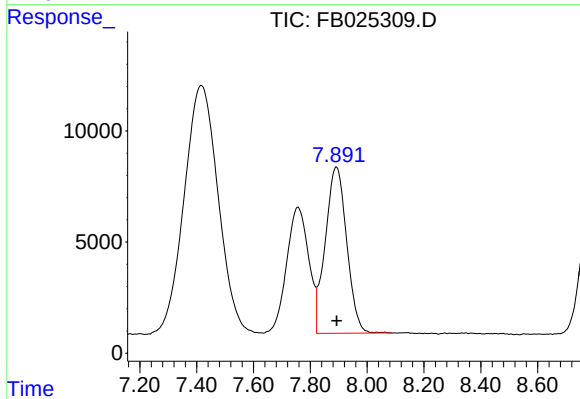

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 392135
Conc: 10.60 ng/ml

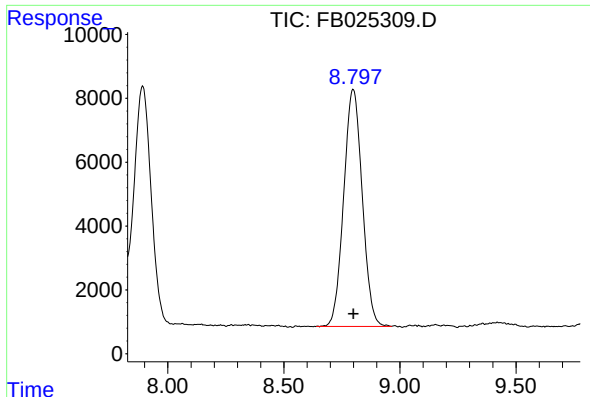

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 412527
Conc: 19.62 ng/ml

Instrument :
FID_B
ClientSampleId :
FB120220GROICV

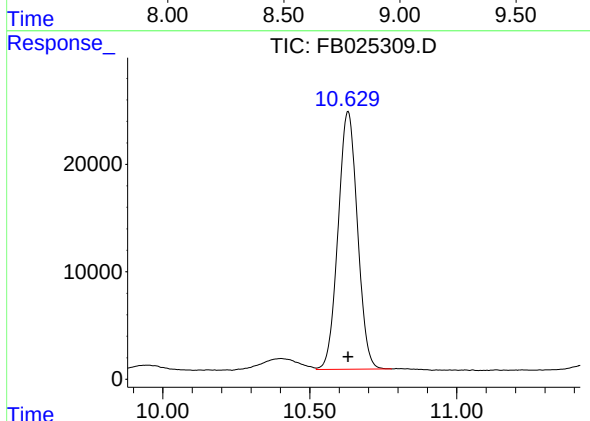


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1098639
Conc: 31.26 ng/ml

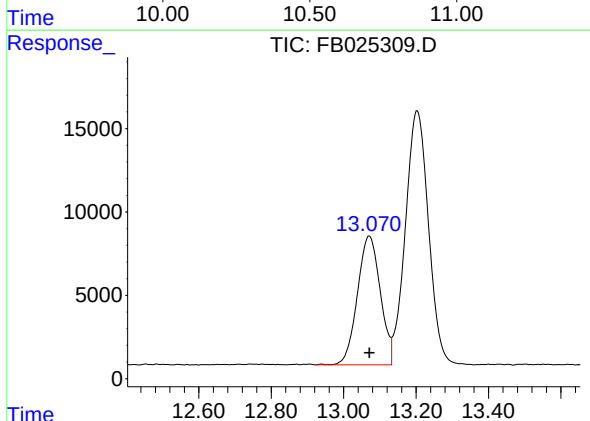


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 338203
Conc: 10.35 ng/ml

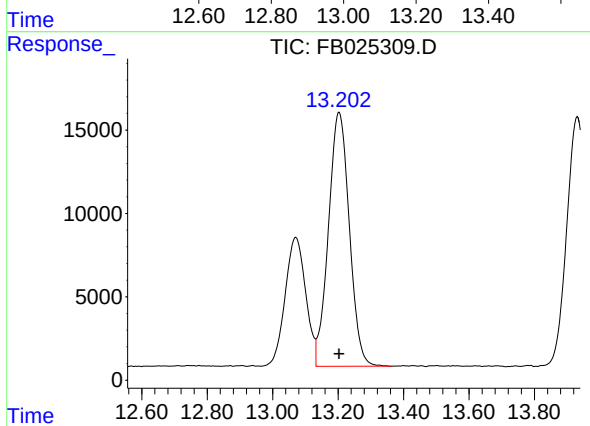

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 675703
Conc: 20.88 ng/ml

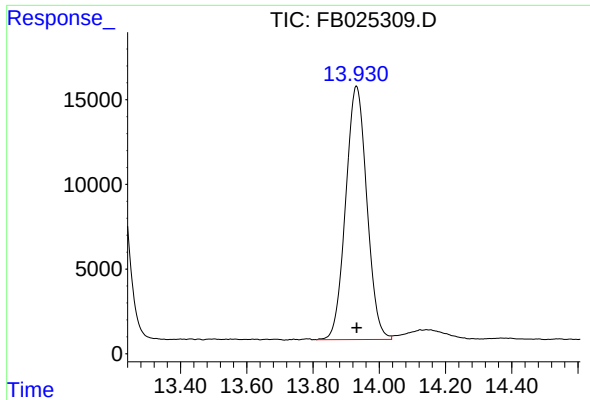

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 663815
Conc: 21.00 ng/ml

Instrument :
FID_B
ClientSampleId :
FB120220GROICV

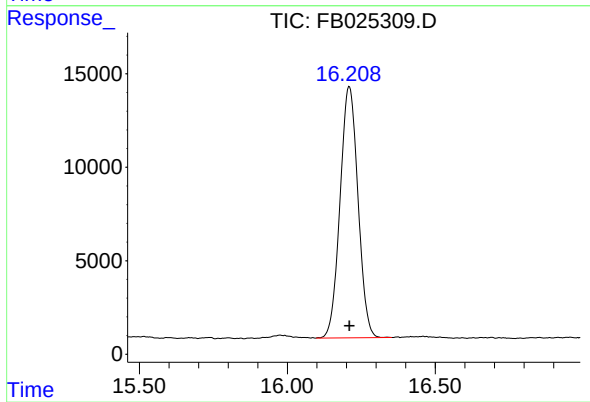

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 566340
Conc: 20.86 ng/ml