

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
Data File : FB023130.D
Signal(s) : FID2B.CH
Acq On : 4 Dec 2019 12:31
Operator : DD/AJ
Sample : K6119-03
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 05 00:38:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	501648	20.422 ng/ml
Target Compounds			
6) t Toluene	10.626	1384	0.034 ng/ml
8) t m-Xylene	13.195	1228	0.034 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	336	0.012 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
Data File : FB023130.D
Signal(s) : FID2B.CH
Acq On : 4 Dec 2019 12:31
Operator : DD/AJ
Sample : K6119-03
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 05 00:38:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

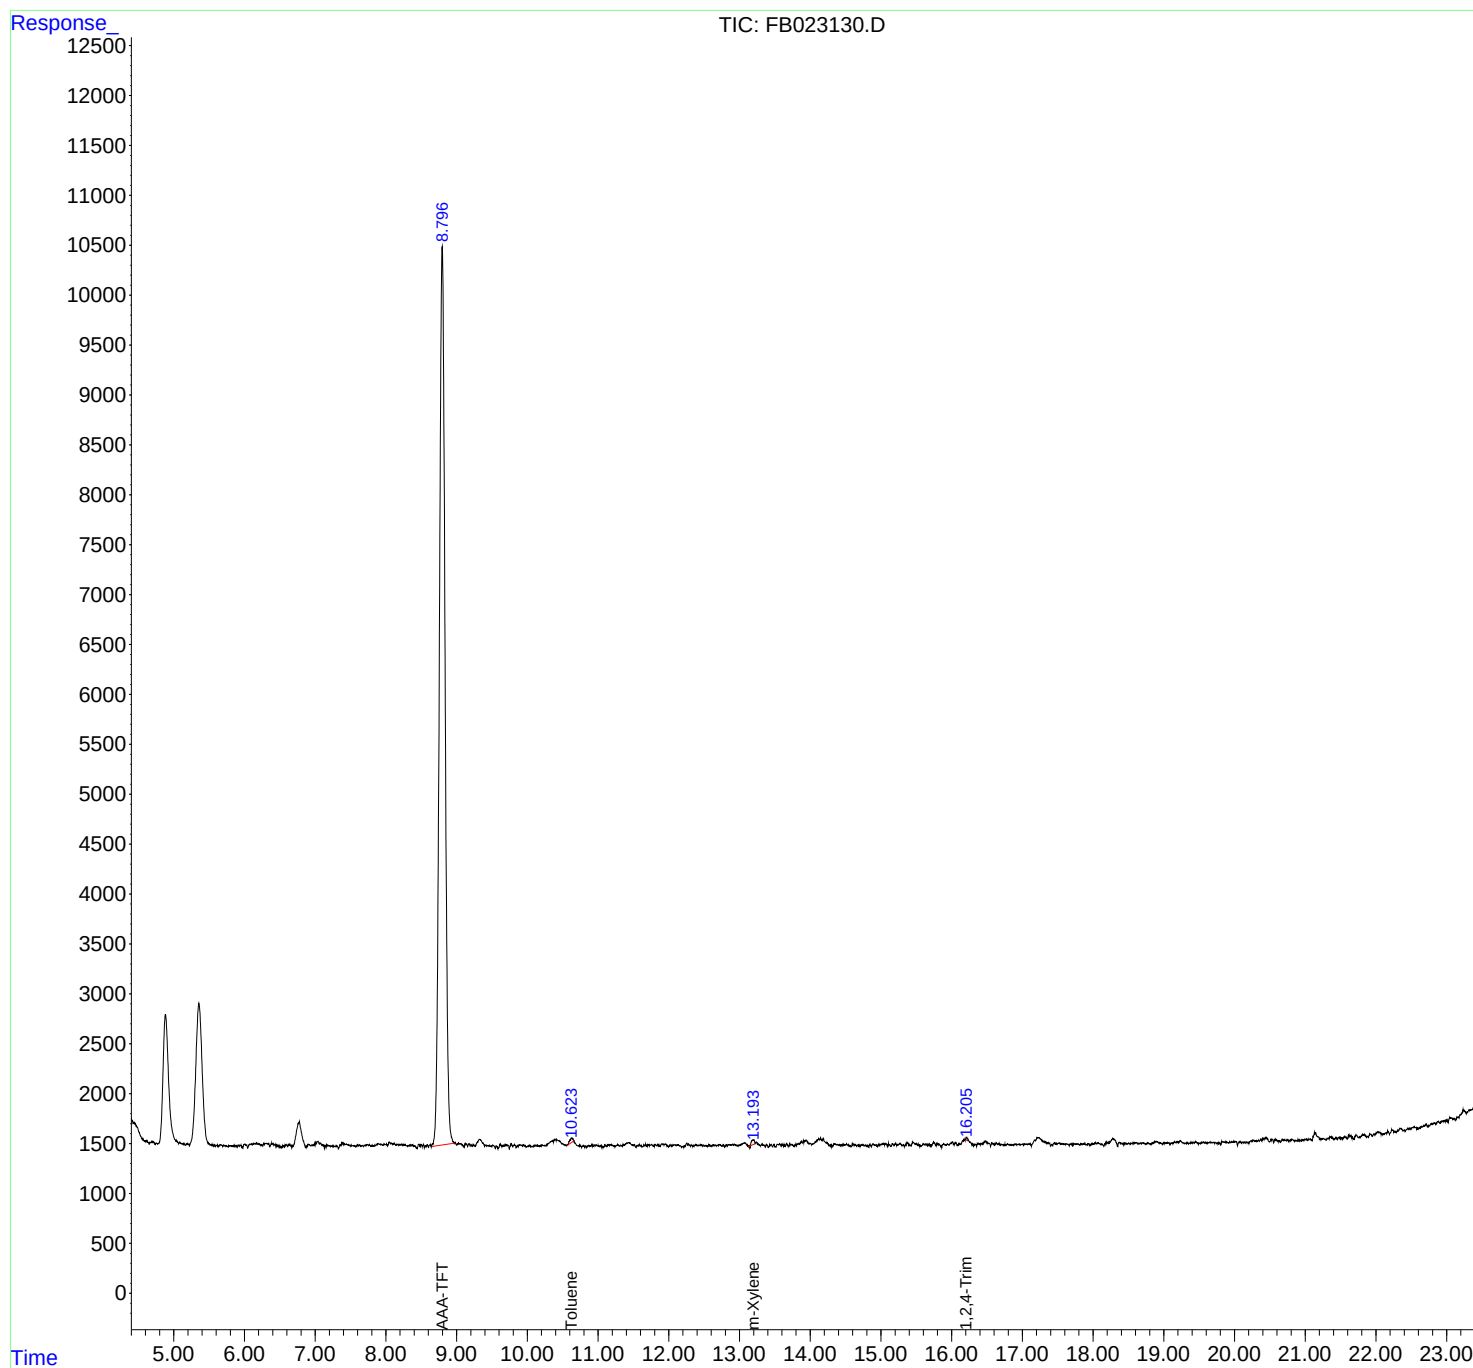


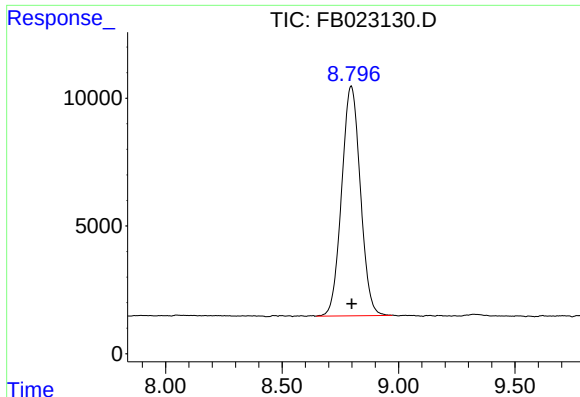

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 501648
Conc: 20.42 ng/ml

Instrument :
FID_B
ClientSampleId :

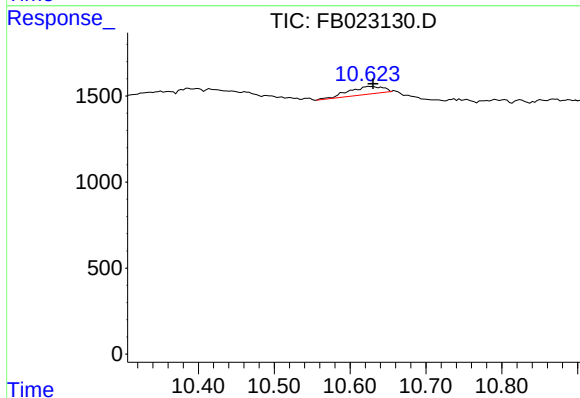


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.004 min
Response: 1384
Conc: 0.03 ng/ml

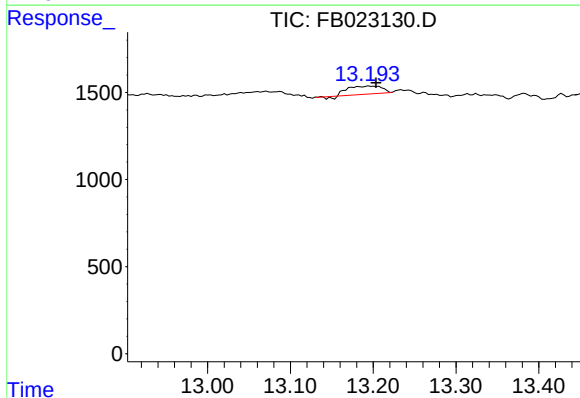

#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: -0.008 min
Response: 1228
Conc: 0.03 ng/ml

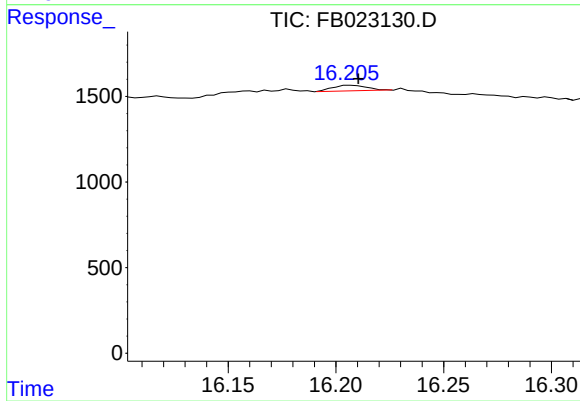

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 336
Conc: 0.01 ng/ml