

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
 Data File : FB023133.D
 Signal(s) : FID2B.CH
 Acq On : 4 Dec 2019 14:15
 Operator : DD/AJ
 Sample : K6119-01
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 05 00:38:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.799	400381	16.300 ng/ml
Target Compounds				
3) t	n-Heptane	7.718	330	0.010 ng/ml
6) t	Toluene	10.629	9560	0.237 ng/ml
7) t	Ethylbenzene	13.061	20040	0.519 ng/ml
8) t	m-Xylene	13.204	61155	1.681 ng/ml
9) t	O-Xylene	13.933	31918	0.919 ng/ml
10) t	1,2,4-Trimethylbenzene	16.211	3493	0.125 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
Data File : FB023133.D
Signal(s) : FID2B.CH
Acq On : 4 Dec 2019 14:15
Operator : DD/AJ
Sample : K6119-01
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 05 00:38:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

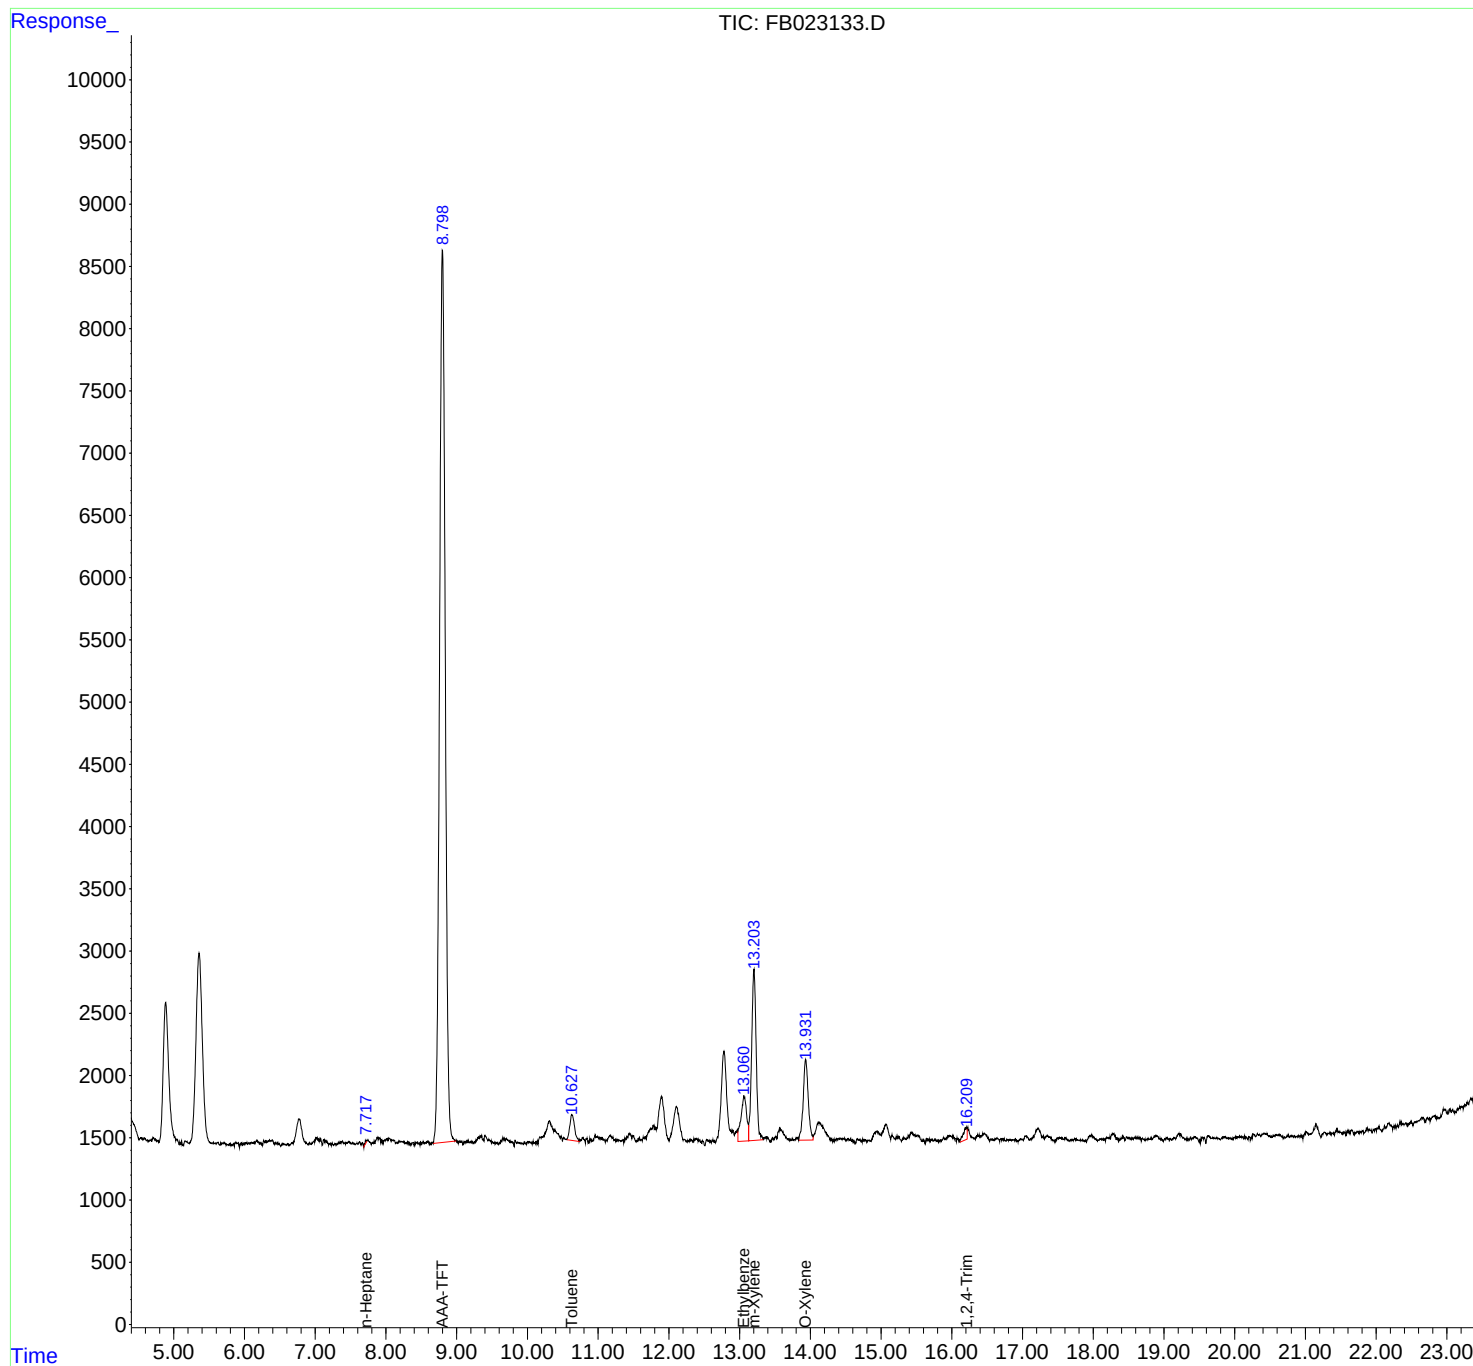


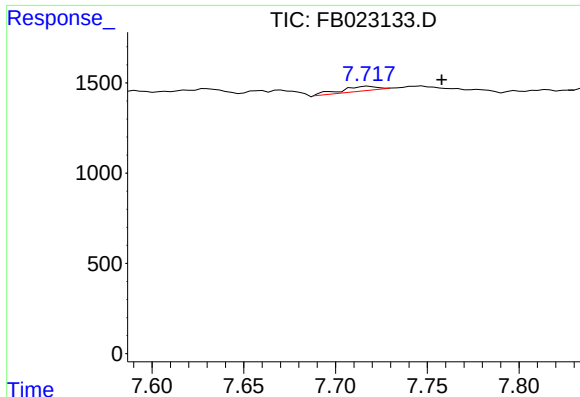

#3 n-Heptane


R.T.: 7.718 min
Delta R.T.: -0.040 min
Response: 330
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :

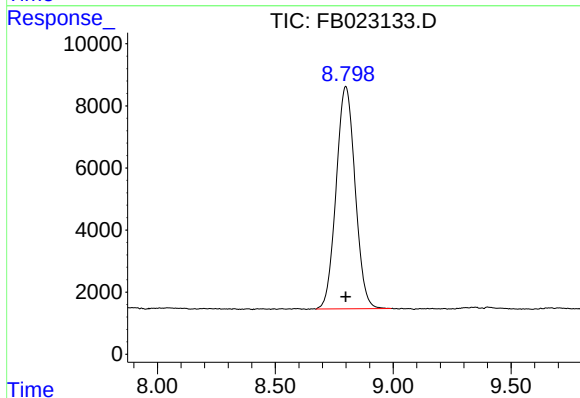


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 400381
Conc: 16.30 ng/ml

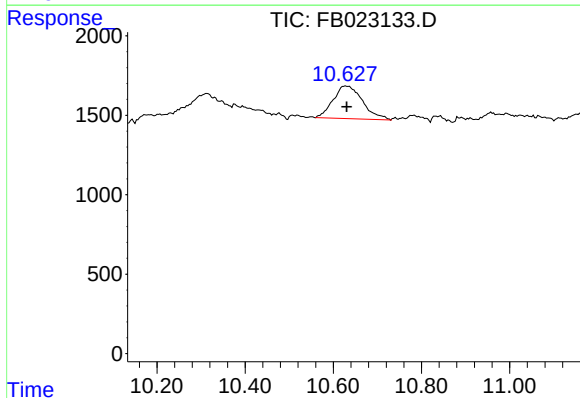


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.002 min
Response: 9560
Conc: 0.24 ng/ml

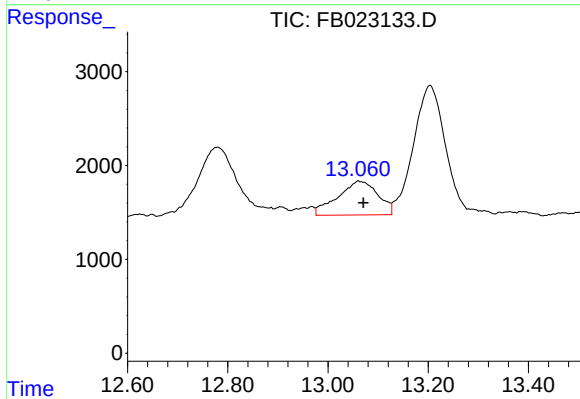

#7 Ethylbenzene


R.T.: 13.061 min
Delta R.T.: -0.009 min
Response: 20040
Conc: 0.52 ng/ml

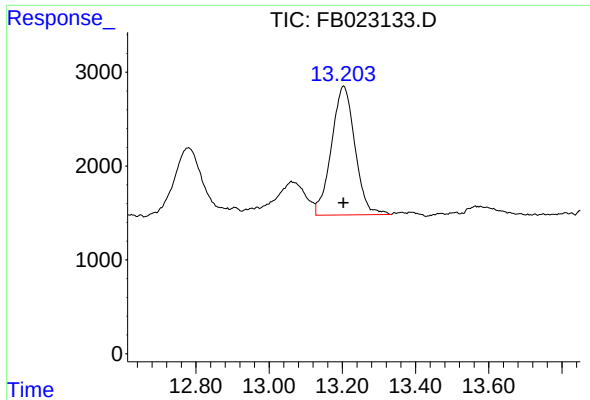

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 61155
Conc: 1.68 ng/ml

Instrument :
FID_B
ClientSampleId :

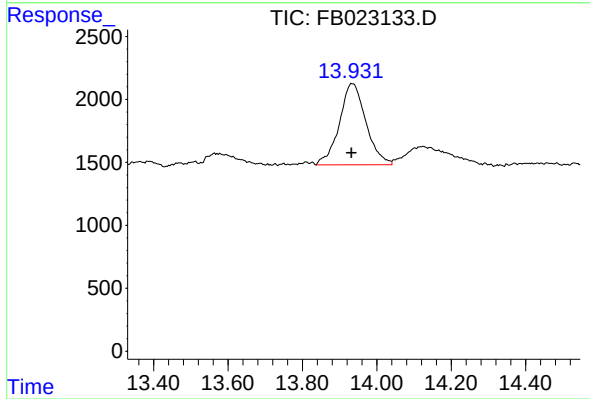

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.002 min
Response: 31918
Conc: 0.92 ng/ml

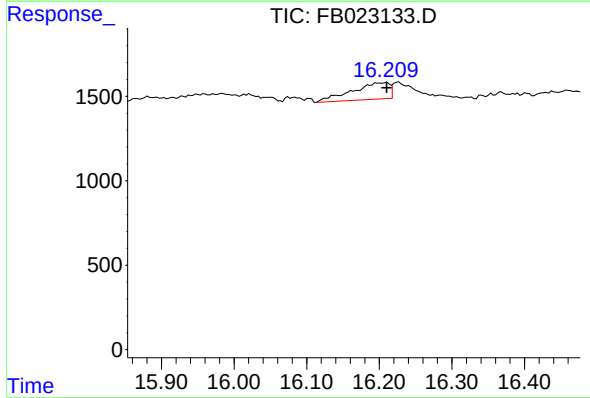

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 3493
Conc: 0.12 ng/ml