

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
 Data File : FB023135.D
 Signal(s) : FID2B.CH
 Acq On : 4 Dec 2019 17:47
 Operator : DD/AJ
 Sample : K6119-05
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 05 00:39:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	488357	19.881 ng/ml
Target Compounds			
6) t Toluene	10.627	415	0.010 ng/ml
8) t m-Xylene	13.213	2342	0.064 ng/ml
9) t O-Xylene	13.928	637	0.018 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	1613	0.058 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
Data File : FB023135.D
Signal(s) : FID2B.CH
Acq On : 4 Dec 2019 17:47
Operator : DD/AJ
Sample : K6119-05
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 05 00:39:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

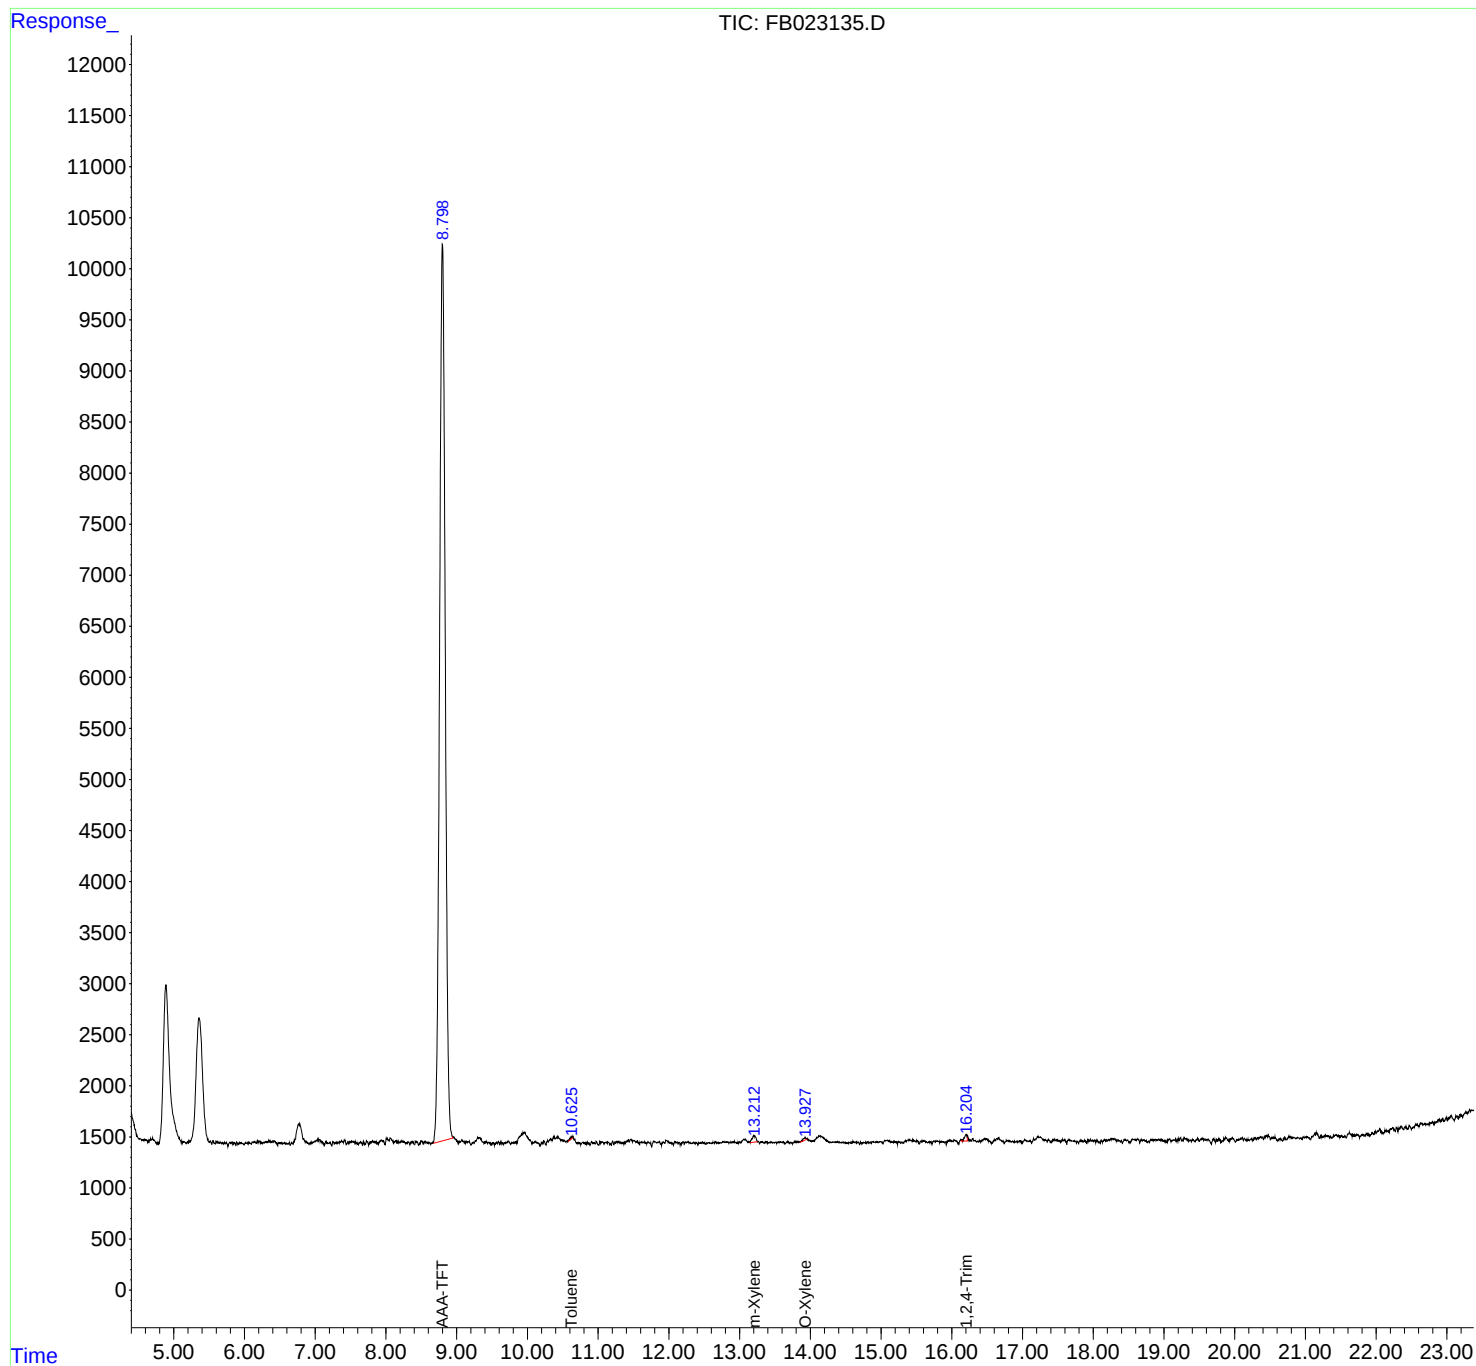

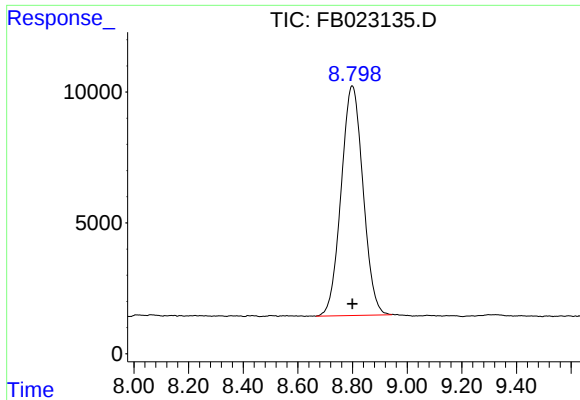


#5 AAA-TFT
 R.T.: 8.799 min
 Delta R.T.: 0.000 min
 Response: 488357
 Conc: 19.88 ng/ml


Instrument :
 FID_B
 ClientSampleId :

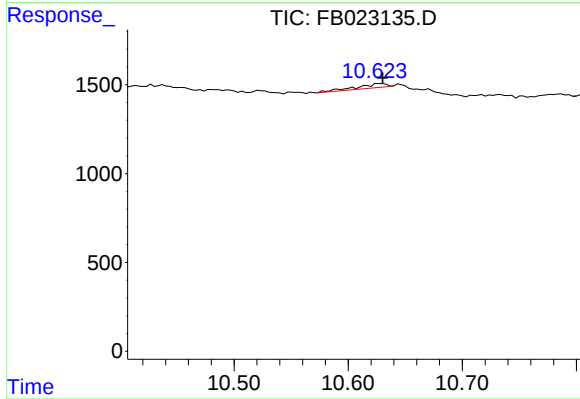


#6 Toluene
 R.T.: 10.627 min
 Delta R.T.: -0.003 min
 Response: 415
 Conc: 0.01 ng/ml

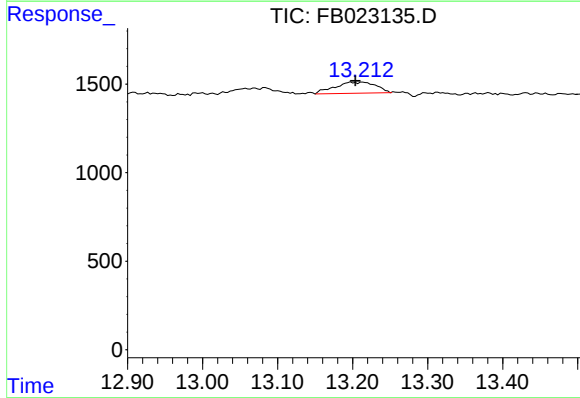

#8 m-Xylene
 R.T.: 13.213 min
 Delta R.T.: 0.010 min
 Response: 2342
 Conc: 0.06 ng/ml

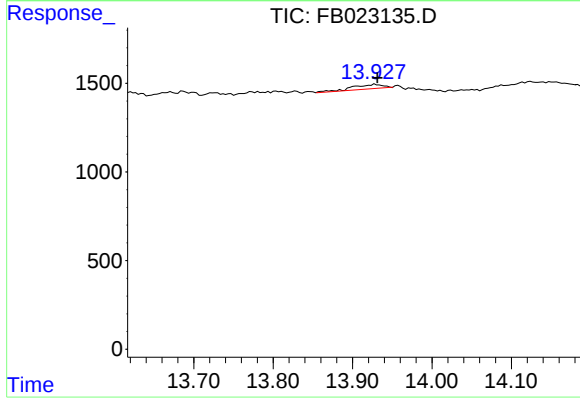

#9 O-Xylene
 R.T.: 13.928 min
 Delta R.T.: -0.003 min
 Response: 637
 Conc: 0.02 ng/ml

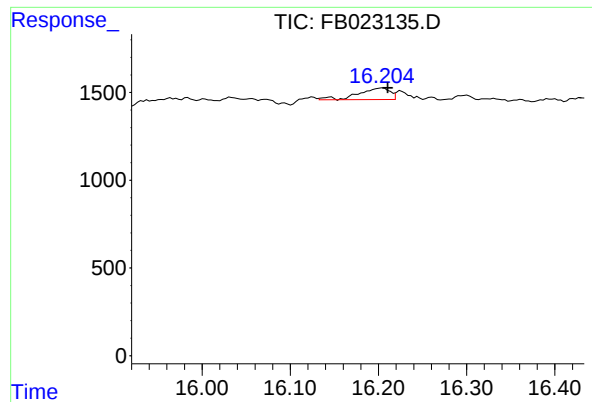

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.005 min
Response: 1613
Conc: 0.06 ng/ml

Instrument :
FID_B
ClientSampleId :