

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
Data File : FB023136.D
Signal(s) : FID2B.CH
Acq On : 4 Dec 2019 18:17
Operator : DD/AJ
Sample : K6119-09
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 05 00:39:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	478191	19.467 ng/ml
Target Compounds			
8) t m-Xylene	13.205	2406	0.066 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
Data File : FB023136.D
Signal(s) : FID2B.CH
Acq On : 4 Dec 2019 18:17
Operator : DD/AJ
Sample : K6119-09
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 05 00:39:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

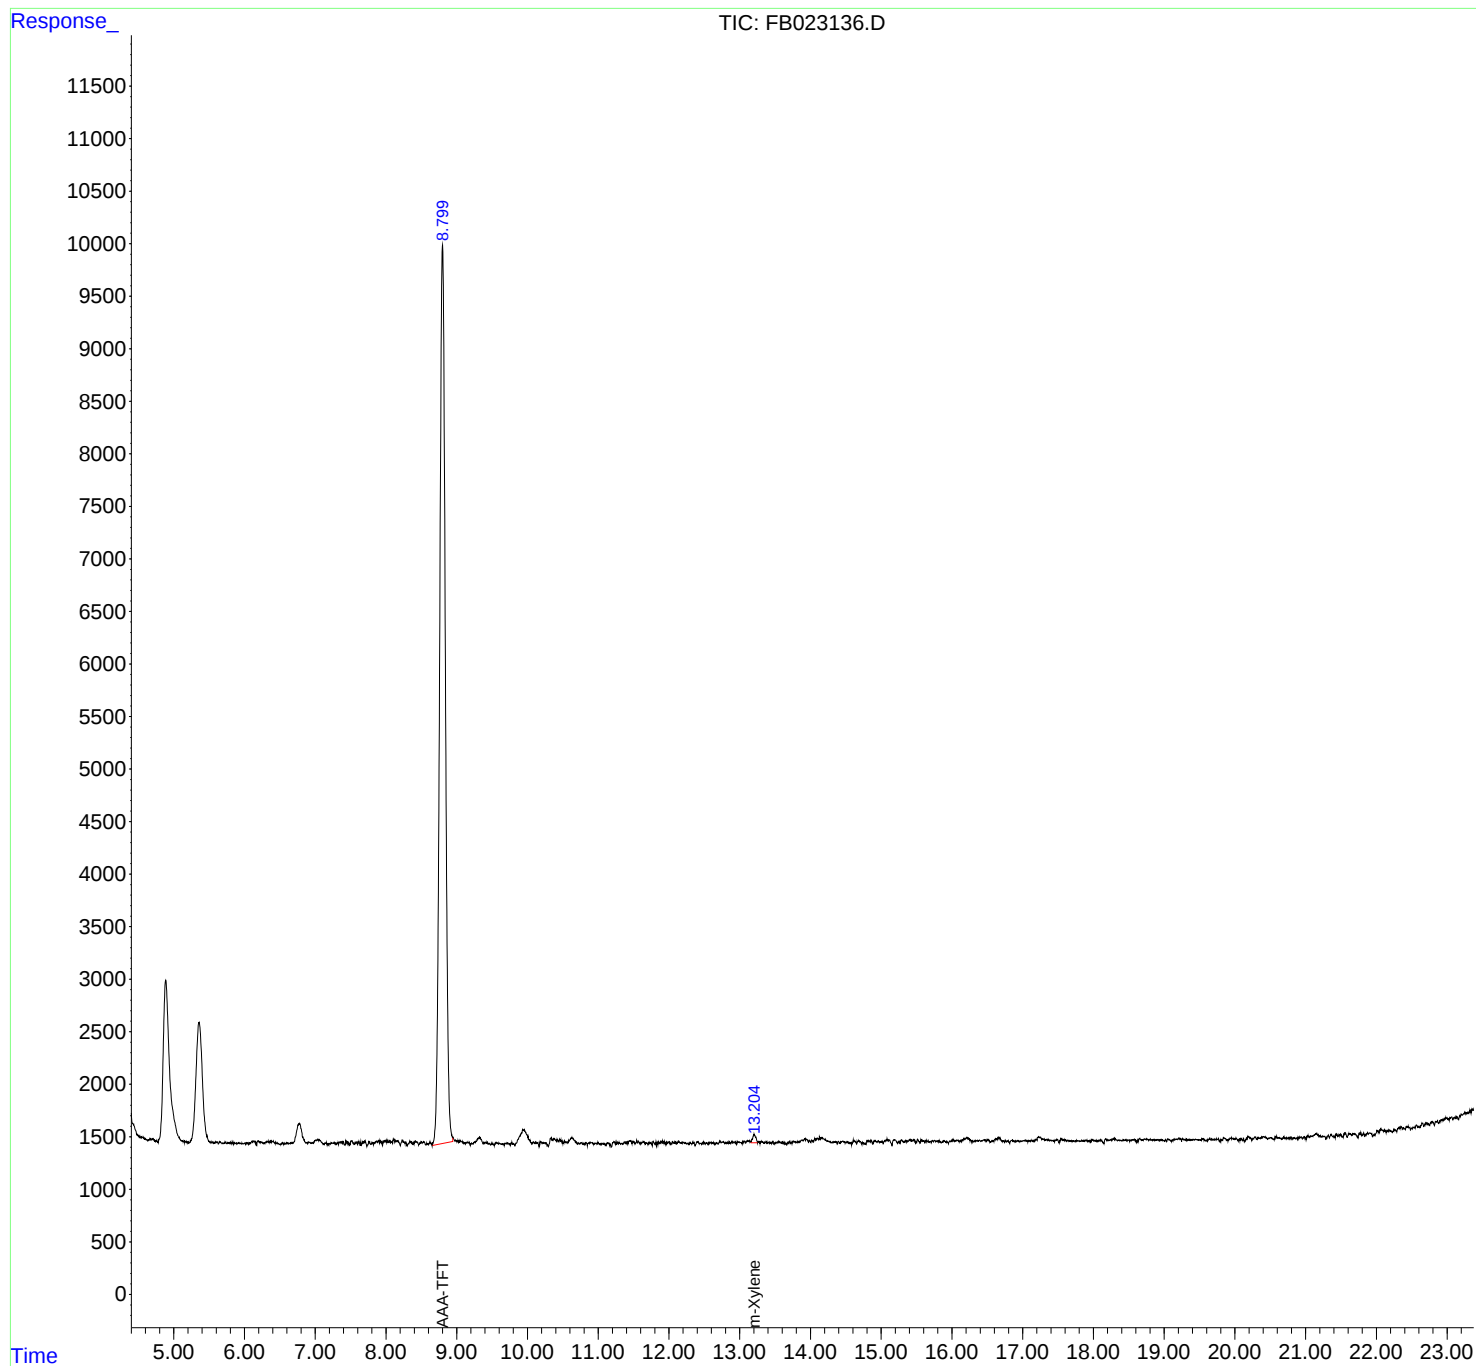


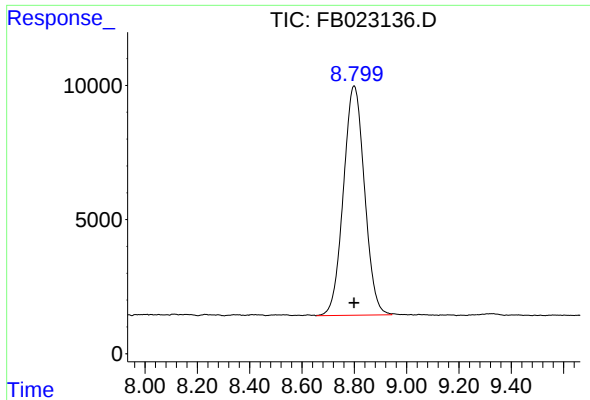

#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 478191
Conc: 19.47 ng/ml

Instrument :
FID_B
ClientSampleId :

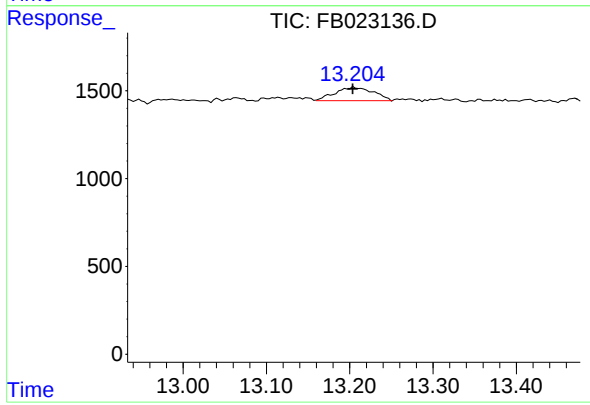

#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.002 min
Response: 2406
Conc: 0.07 ng/ml