

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
 Data File : FB023131.D
 Signal(s) : FID2B.CH
 Acq On : 4 Dec 2019 13:01
 Operator : DD/AJ
 Sample : K6119-03MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-6-(1-3)MS

Integration File: Calibration.e
 Quant Time: Dec 05 00:38:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	503912	20.514 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	1000468	30.616 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1106793	31.740 ng/ml
3) t n-Heptane	7.758	361034	10.500 ng/ml
4) t Benzene	7.893	447735	10.746 ng/ml
6) t Toluene	10.631	1263446	31.364 ng/ml
7) t Ethylbenzene	13.072	399740	10.359 ng/ml
8) t m-Xylene	13.205	753848	20.716 ng/ml
9) t O-Xylene	13.933	722224	20.801 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	597337	21.300 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
Data File : FB023131.D
Signal(s) : FID2B.CH
Acq On : 4 Dec 2019 13:01
Operator : DD/AJ
Sample : K6119-03MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-6-(1-3)MS

Integration File: Calibration.e
Quant Time: Dec 05 00:38:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

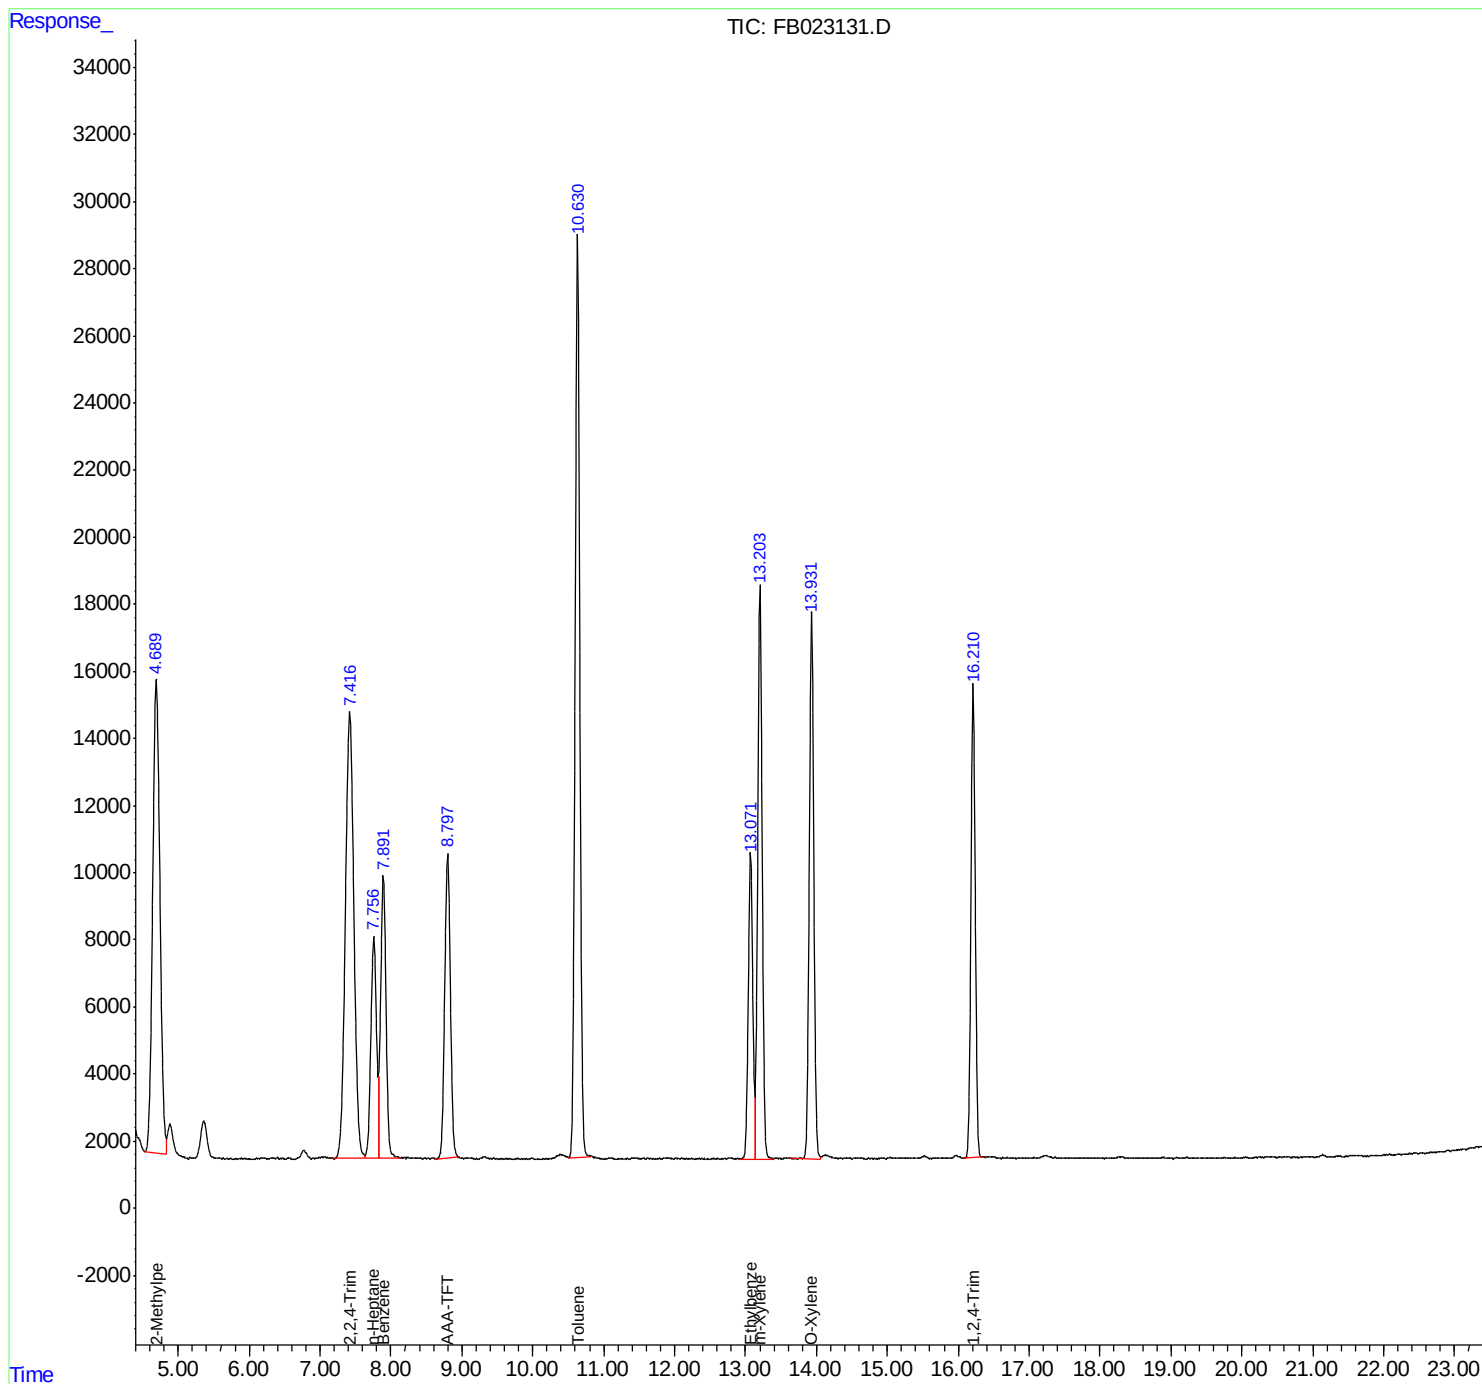


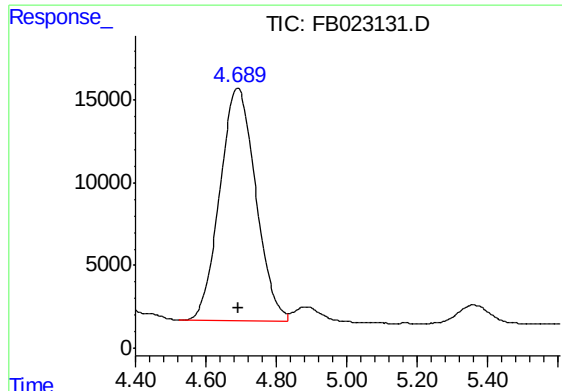

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 1000468
Conc: 30.62 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-6-(1-3)MS

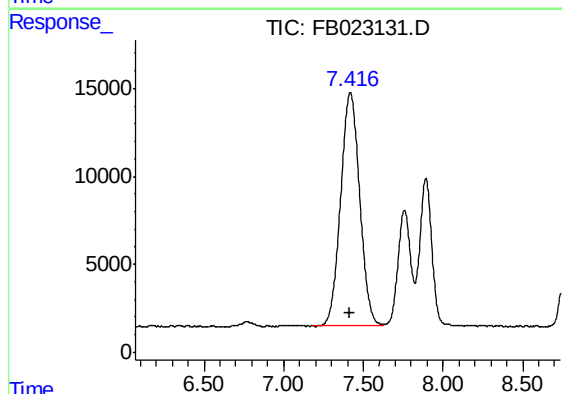


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1106793
Conc: 31.74 ng/ml

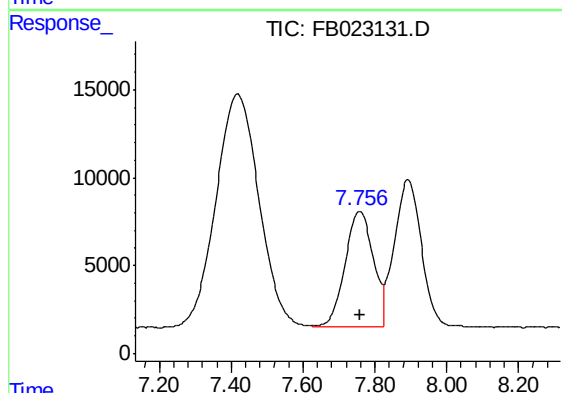


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 361034
Conc: 10.50 ng/ml

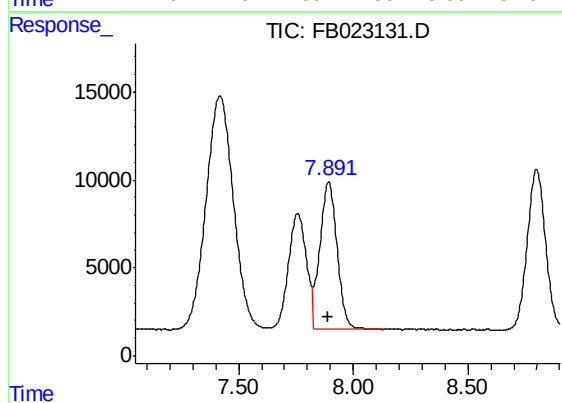

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 447735
Conc: 10.75 ng/ml

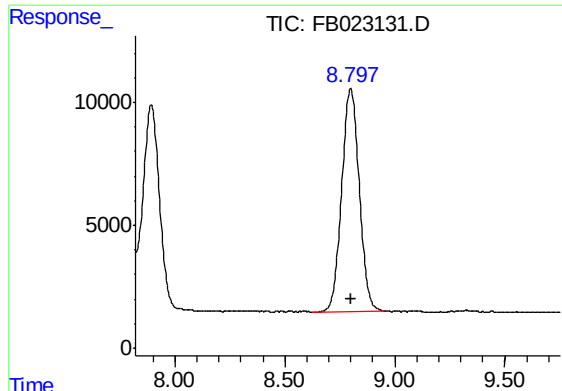

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 503912
Conc: 20.51 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-6-(1-3)MS

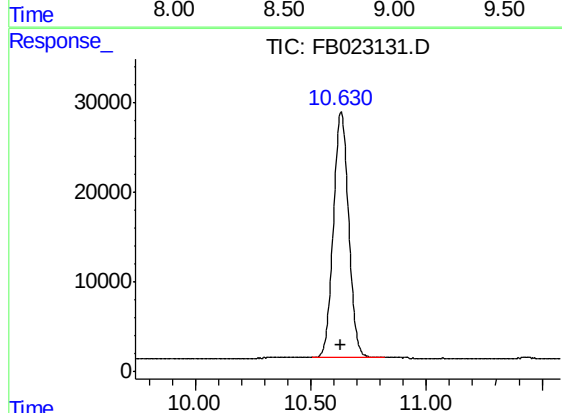


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1263446
Conc: 31.36 ng/ml

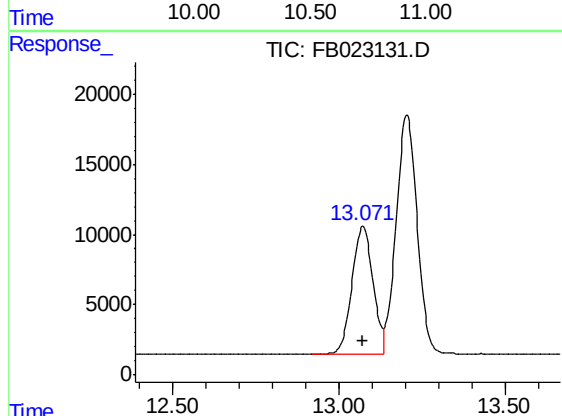


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.002 min
Response: 399740
Conc: 10.36 ng/ml

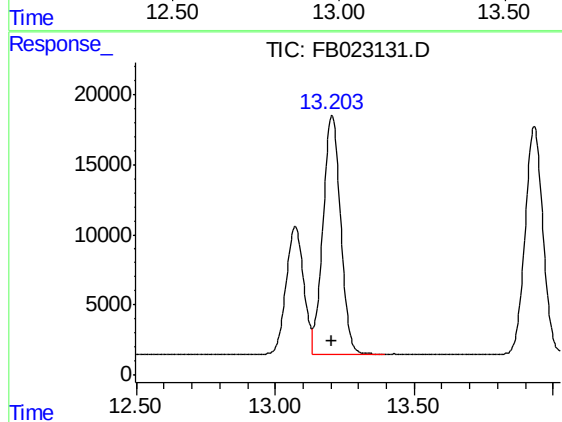

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.001 min
Response: 753848
Conc: 20.72 ng/ml

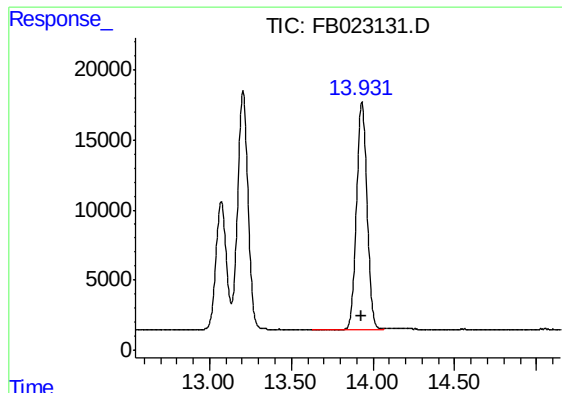

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.001 min
Response: 722224
Conc: 20.80 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-6-(1-3)MS

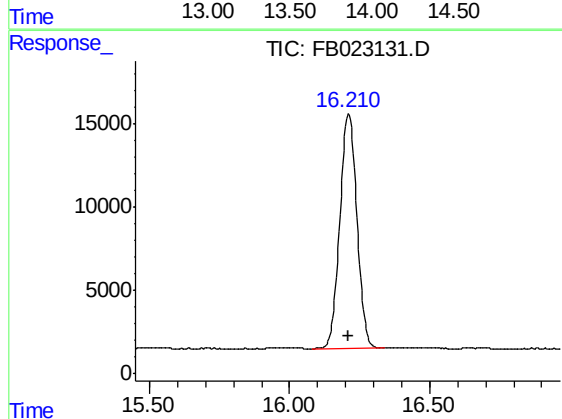

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 597337
Conc: 21.30 ng/ml