

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
 Data File : FB023132.D
 Signal(s) : FID2B.CH
 Acq On : 4 Dec 2019 13:31
 Operator : DD/AJ
 Sample : K6119-03MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-6-(1-3)MSD

Integration File: Calibration.e
 Quant Time: Dec 05 11:11:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	481055	19.584 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	862653	26.398 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	955563	27.403 ng/ml
3) t n-Heptane	7.759	312586	9.091 ng/ml
4) t Benzene	7.893	403320	9.680 ng/ml
6) t Toluene	10.631	1160381	28.805 ng/ml
7) t Ethylbenzene	13.072	368793	9.557 ng/ml
8) t m-Xylene	13.205	702546	19.306 ng/ml
9) t O-Xylene	13.933	677144	19.503 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	567045	20.220 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120419\
Data File : FB023132.D
Signal(s) : FID2B.CH
Acq On : 4 Dec 2019 13:31
Operator : DD/AJ
Sample : K6119-03MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-6-(1-3)MSD

Integration File: Calibration.e
Quant Time: Dec 05 11:11:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

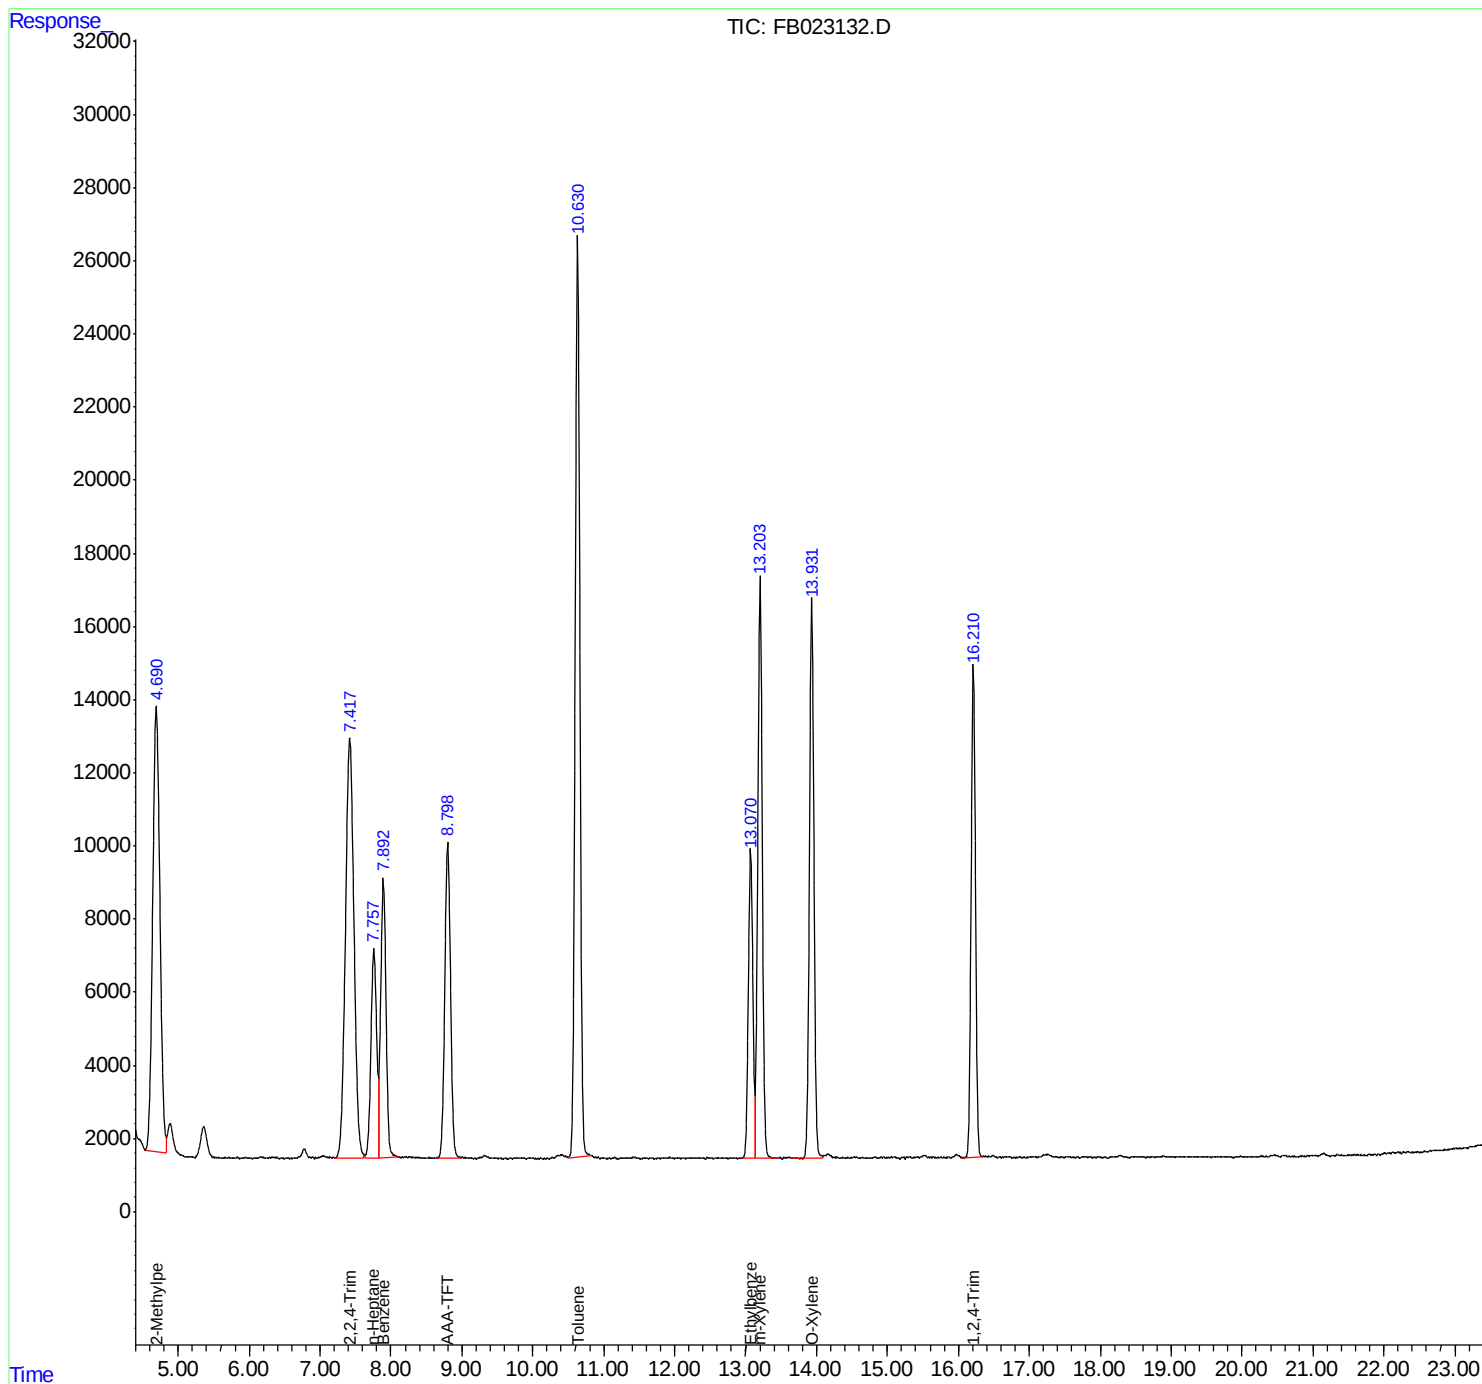


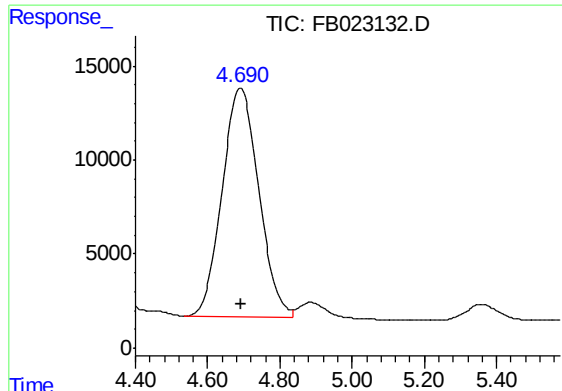

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 862653
Conc: 26.40 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-6-(1-3)MSD

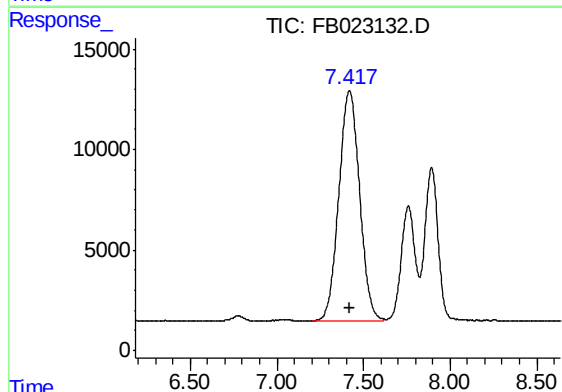


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 955563
Conc: 27.40 ng/ml

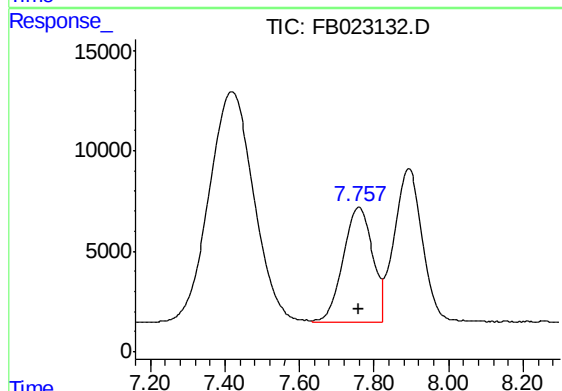


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 312586
Conc: 9.09 ng/ml

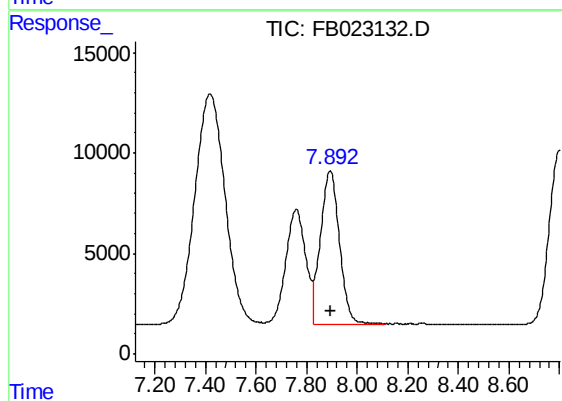

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 403320
Conc: 9.68 ng/ml

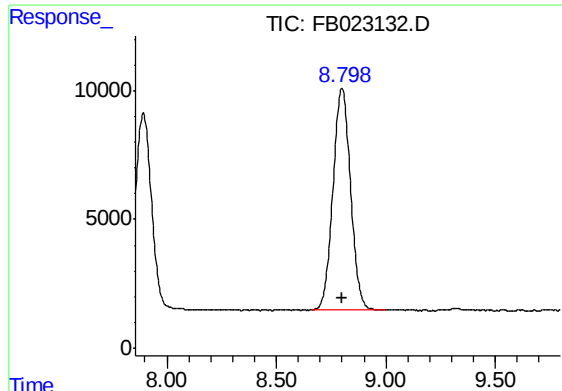

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 481055
Conc: 19.58 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-6-(1-3)MSD

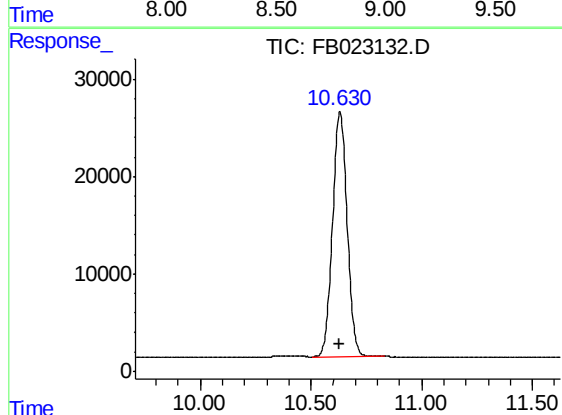


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1160381
Conc: 28.81 ng/ml

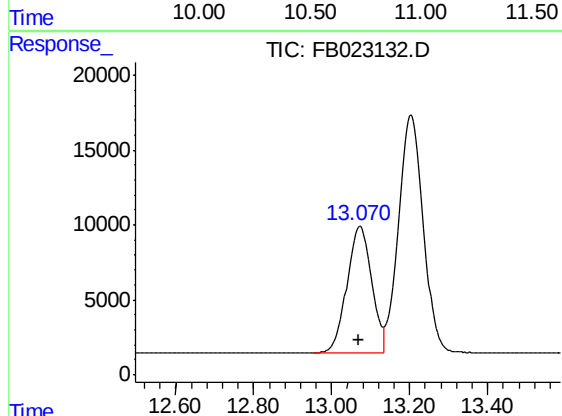


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.001 min
Response: 368793
Conc: 9.56 ng/ml

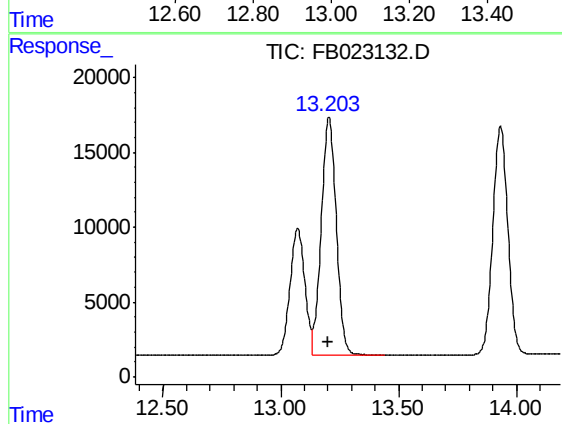

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.001 min
Response: 702546
Conc: 19.31 ng/ml

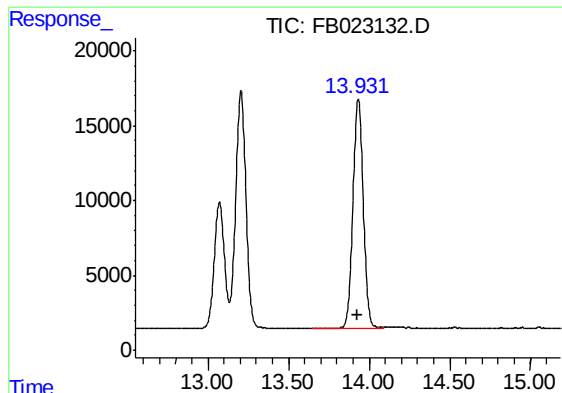

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.001 min
Response: 677144
Conc: 19.50 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-6-(1-3)MSD

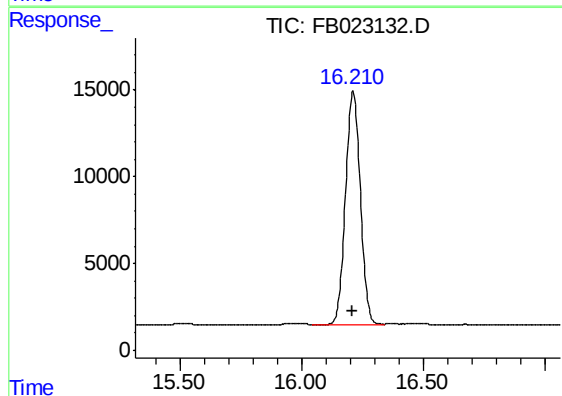

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.001 min
Response: 567045
Conc: 20.22 ng/ml