

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
 Data File : FB023141.D
 Signal(s) : FID2B.CH
 Acq On : 5 Dec 2019 13:47
 Operator : DD/AJ
 Sample : K6112-02
 Misc : 4.98g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 06 00:18:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	475627	19.363 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.424	3360	0.096 ng/ml
4) t Benzene	7.889	9231	0.222 ng/ml
6) t Toluene	10.627	30175	0.749 ng/ml
7) t Ethylbenzene	13.060	9982	0.259 ng/ml
8) t m-Xylene	13.199	20693	0.569 ng/ml
9) t O-Xylene	13.929	31306	0.902 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	27051	0.965 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
Data File : FB023141.D
Signal(s) : FID2B.CH
Acq On : 5 Dec 2019 13:47
Operator : DD/AJ
Sample : K6112-02
Misc : 4.98g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 06 00:18:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

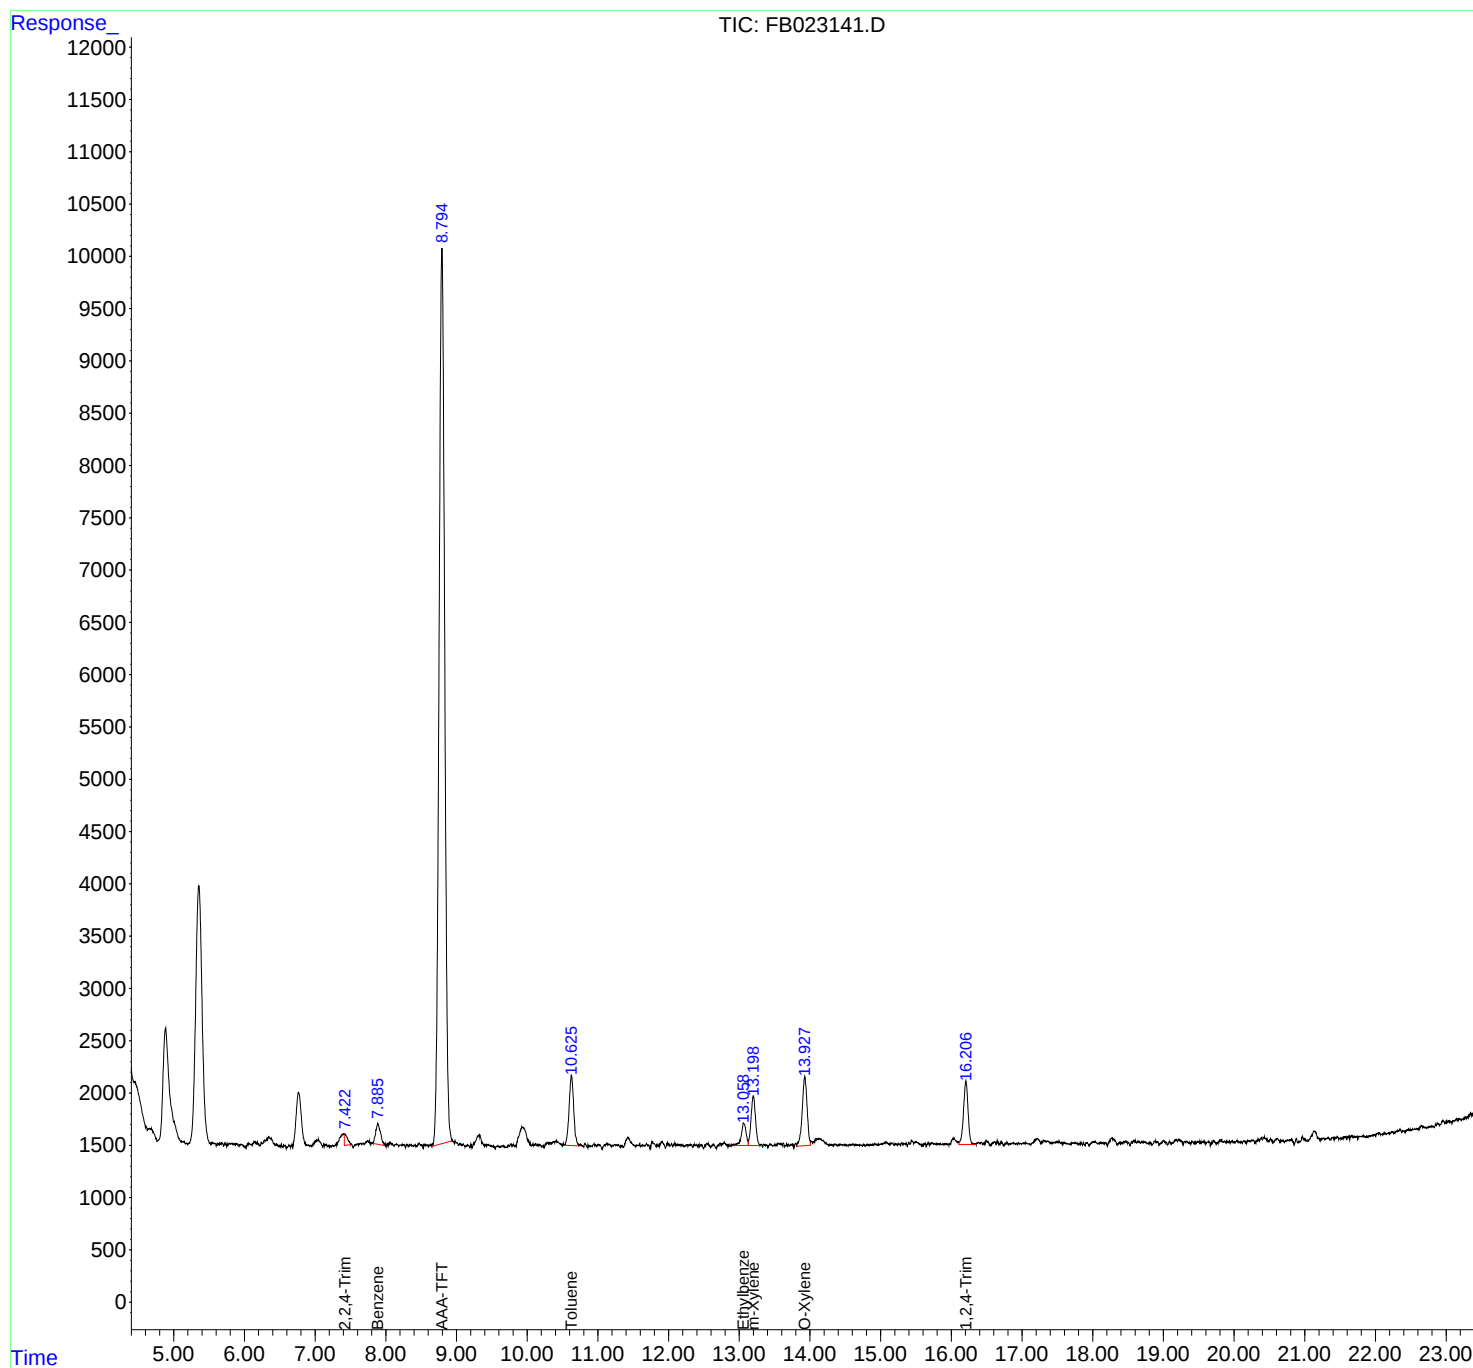


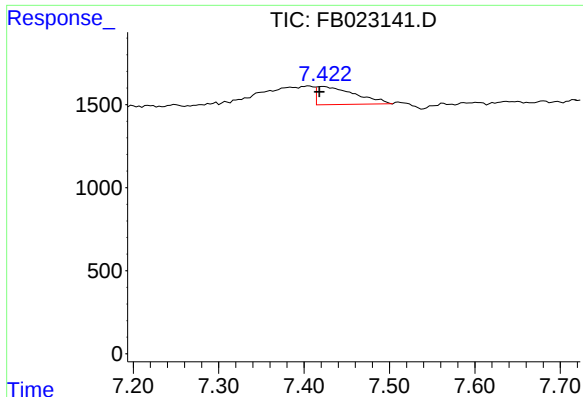

#2 2,2,4-Trimethylpentane


R.T.: 7.424 min
Delta R.T.: 0.006 min
Response: 3360
Conc: 0.10 ng/ml

Instrument :
FID_B
ClientSampleId :

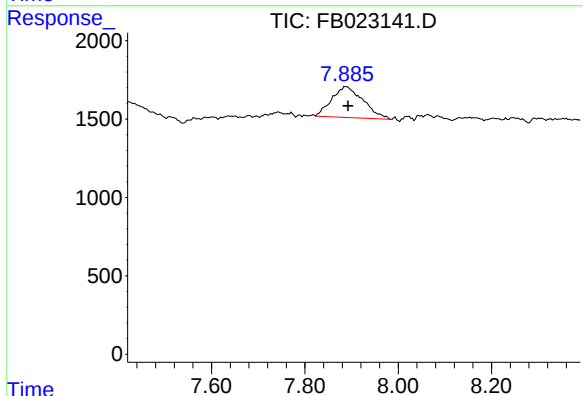


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 9231
Conc: 0.22 ng/ml

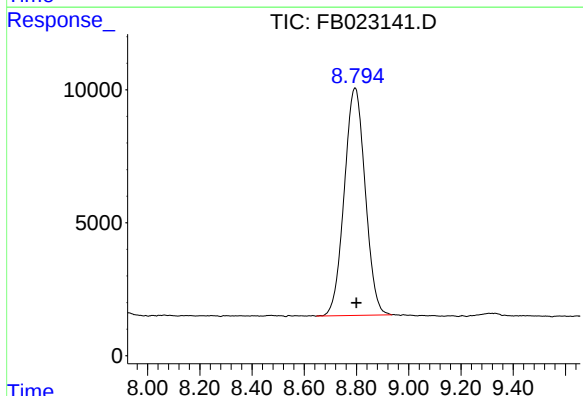


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 475627
Conc: 19.36 ng/ml

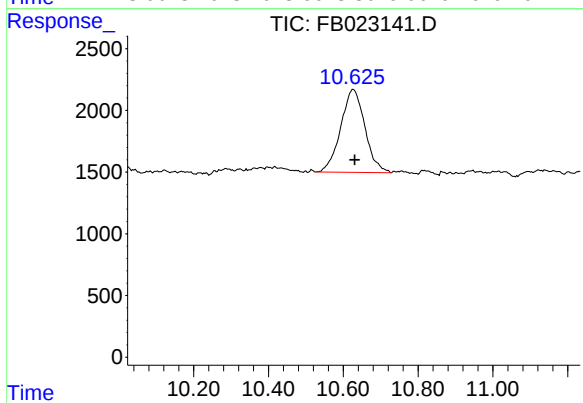

#6 Toluene


R.T.: 10.627 min
Delta R.T.: -0.004 min
Response: 30175
Conc: 0.75 ng/ml

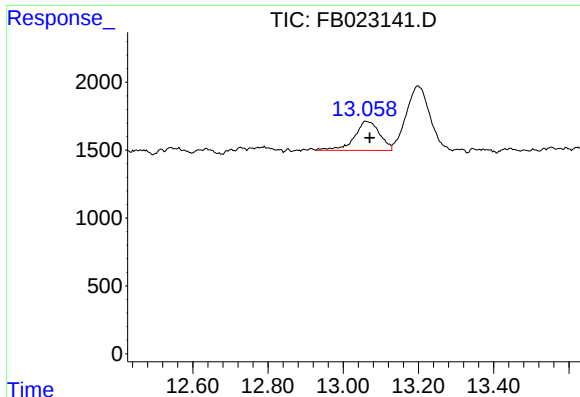

#7 Ethylbenzene


R.T.: 13.060 min
Delta R.T.: -0.010 min
Response: 9982
Conc: 0.26 ng/ml

Instrument :
FID_B
ClientSampleId :

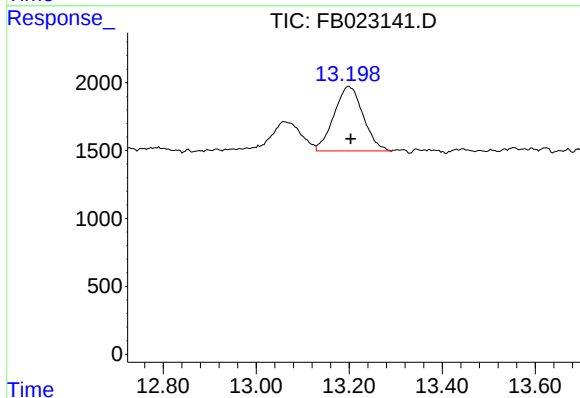


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.004 min
Response: 20693
Conc: 0.57 ng/ml

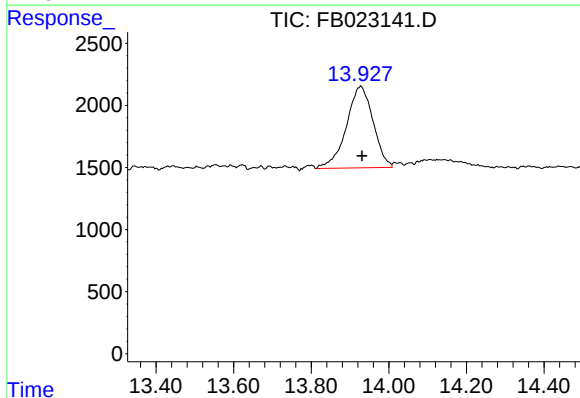

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.003 min
Response: 31306
Conc: 0.90 ng/ml

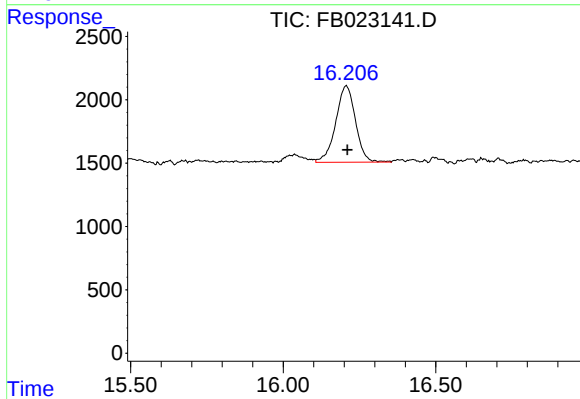

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.003 min
Response: 27051
Conc: 0.96 ng/ml