

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
 Data File : FB023144.D
 Signal(s) : FID2B.CH
 Acq On : 5 Dec 2019 15:33
 Operator : DD/AJ
 Sample : K6119-05MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 06 00:18:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	503911	20.514 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	865922	26.498 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	980559	28.120 ng/ml
3) t n-Heptane	7.755	319748	9.300 ng/ml
4) t Benzene	7.889	399826	9.596 ng/ml
6) t Toluene	10.628	1165574	28.934 ng/ml
7) t Ethylbenzene	13.069	366507	9.498 ng/ml
8) t m-Xylene	13.202	689831	18.957 ng/ml
9) t O-Xylene	13.930	661913	19.064 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	543087	19.366 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
Data File : FB023144.D
Signal(s) : FID2B.CH
Acq On : 5 Dec 2019 15:33
Operator : DD/AJ
Sample : K6119-05MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 06 00:18:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

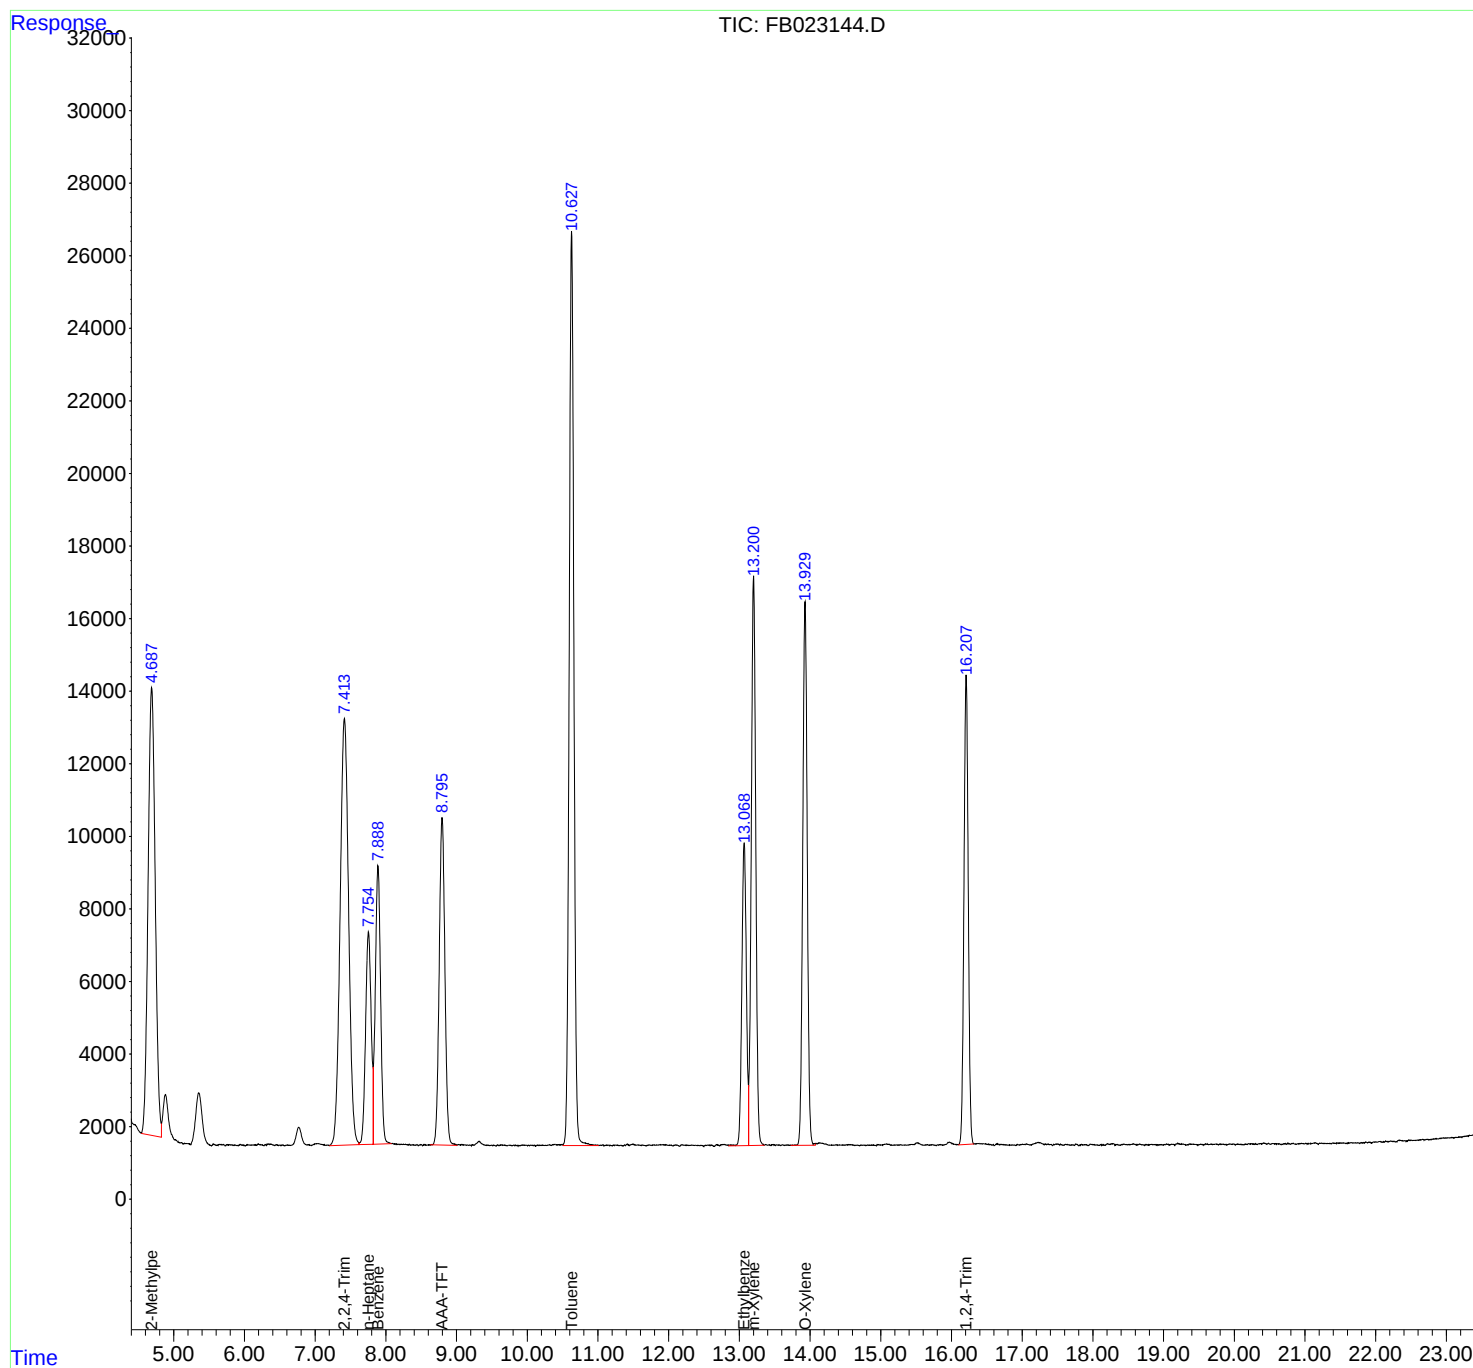


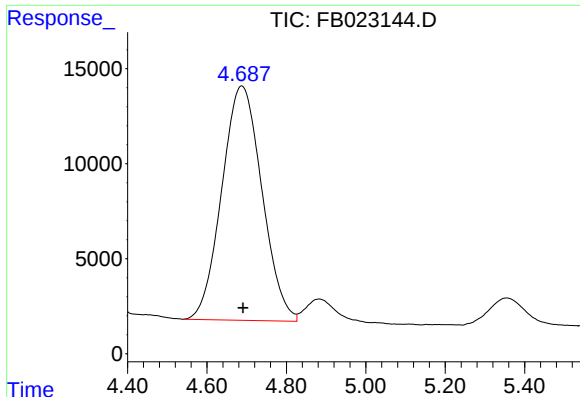

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 865922
Conc: 26.50 ng/ml

Instrument :
FID_B
ClientSampleId :

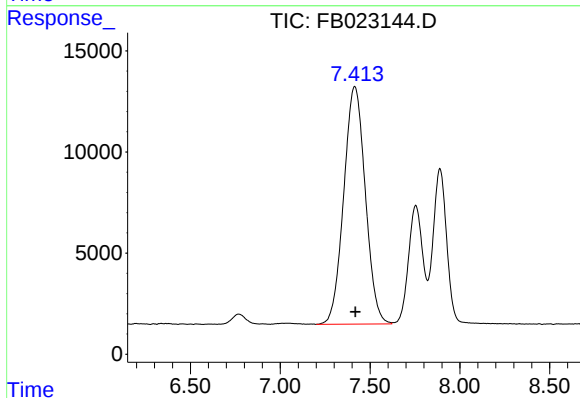


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.004 min
Response: 980559
Conc: 28.12 ng/ml

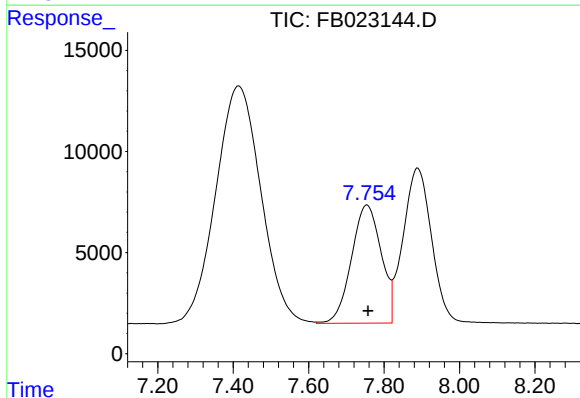


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 319748
Conc: 9.30 ng/ml

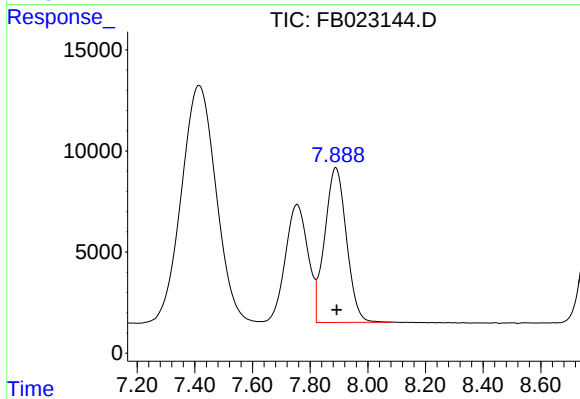

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 399826
Conc: 9.60 ng/ml

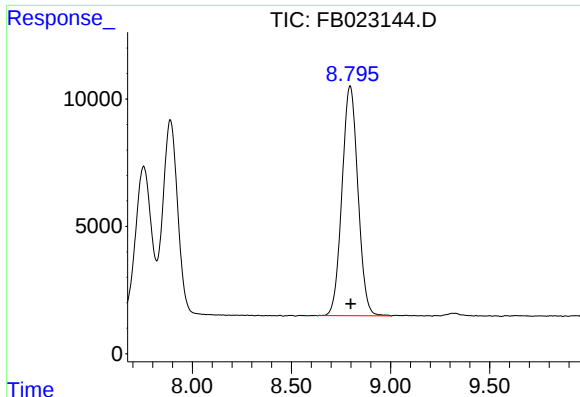

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 503911
Conc: 20.51 ng/ml

Instrument :
FID_B
ClientSampleId :

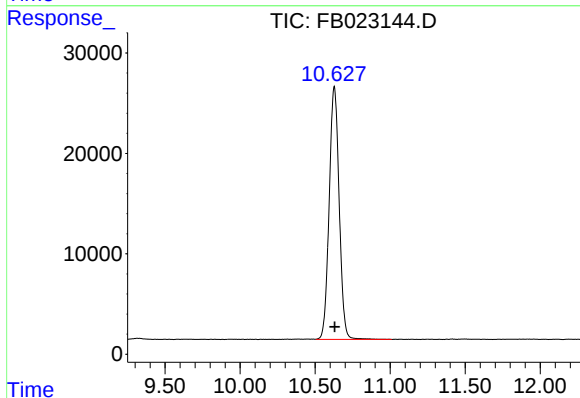


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 1165574
Conc: 28.93 ng/ml

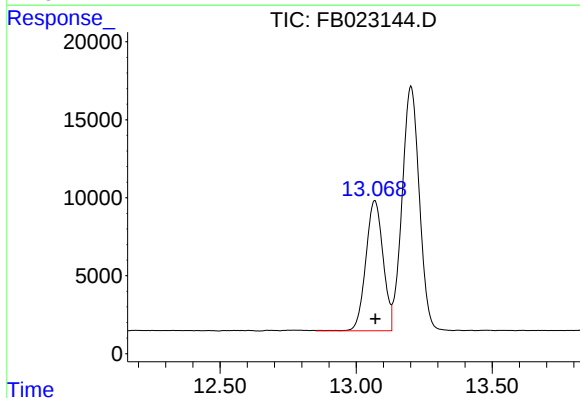


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 366507
Conc: 9.50 ng/ml

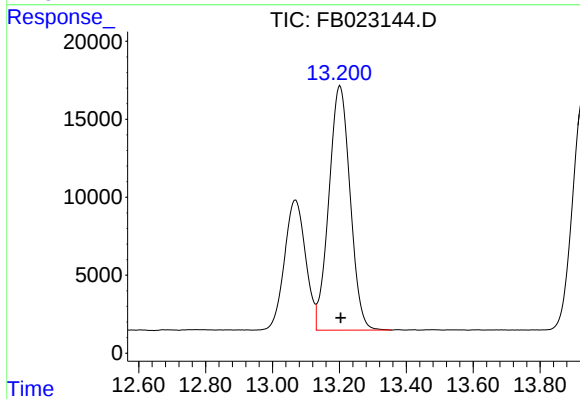

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.002 min
Response: 689831
Conc: 18.96 ng/ml

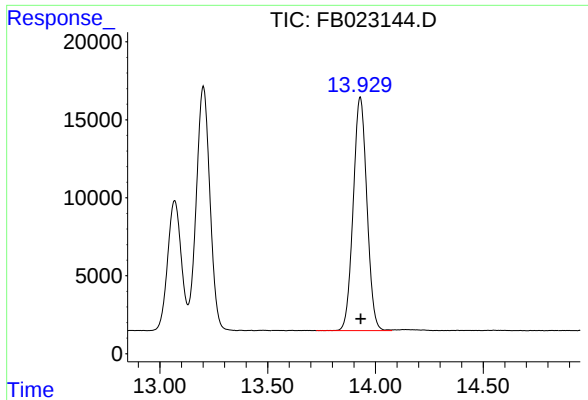

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.002 min
Response: 661913
Conc: 19.06 ng/ml

Instrument :
FID_B
ClientSampleId :

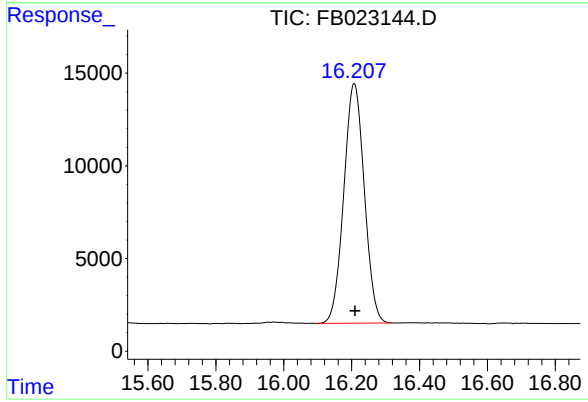

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 543087
Conc: 19.37 ng/ml