

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
 Data File : FB023147.D
 Signal(s) : FID2B.CH
 Acq On : 5 Dec 2019 17:34
 Operator : DD/AJ
 Sample : K6174-02
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 06 00:18:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.858	513740	20.914 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	521866	15.970 ng/ml
2) t 2,2,4-Trimethylpentane	7.372	281223	8.065 ng/ml
3) t n-Heptane	7.758	663743	19.304 ng/ml
6) t Toluene	10.658	23650	0.587 ng/ml
7) t Ethylbenzene	13.065	53708	1.392 ng/ml
8) t m-Xylene	13.200	76123	2.092 ng/ml
9) t O-Xylene	13.930	2885	0.083 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	67508	2.407 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
Data File : FB023147.D
Signal(s) : FID2B.CH
Acq On : 5 Dec 2019 17:34
Operator : DD/AJ
Sample : K6174-02
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 06 00:18:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

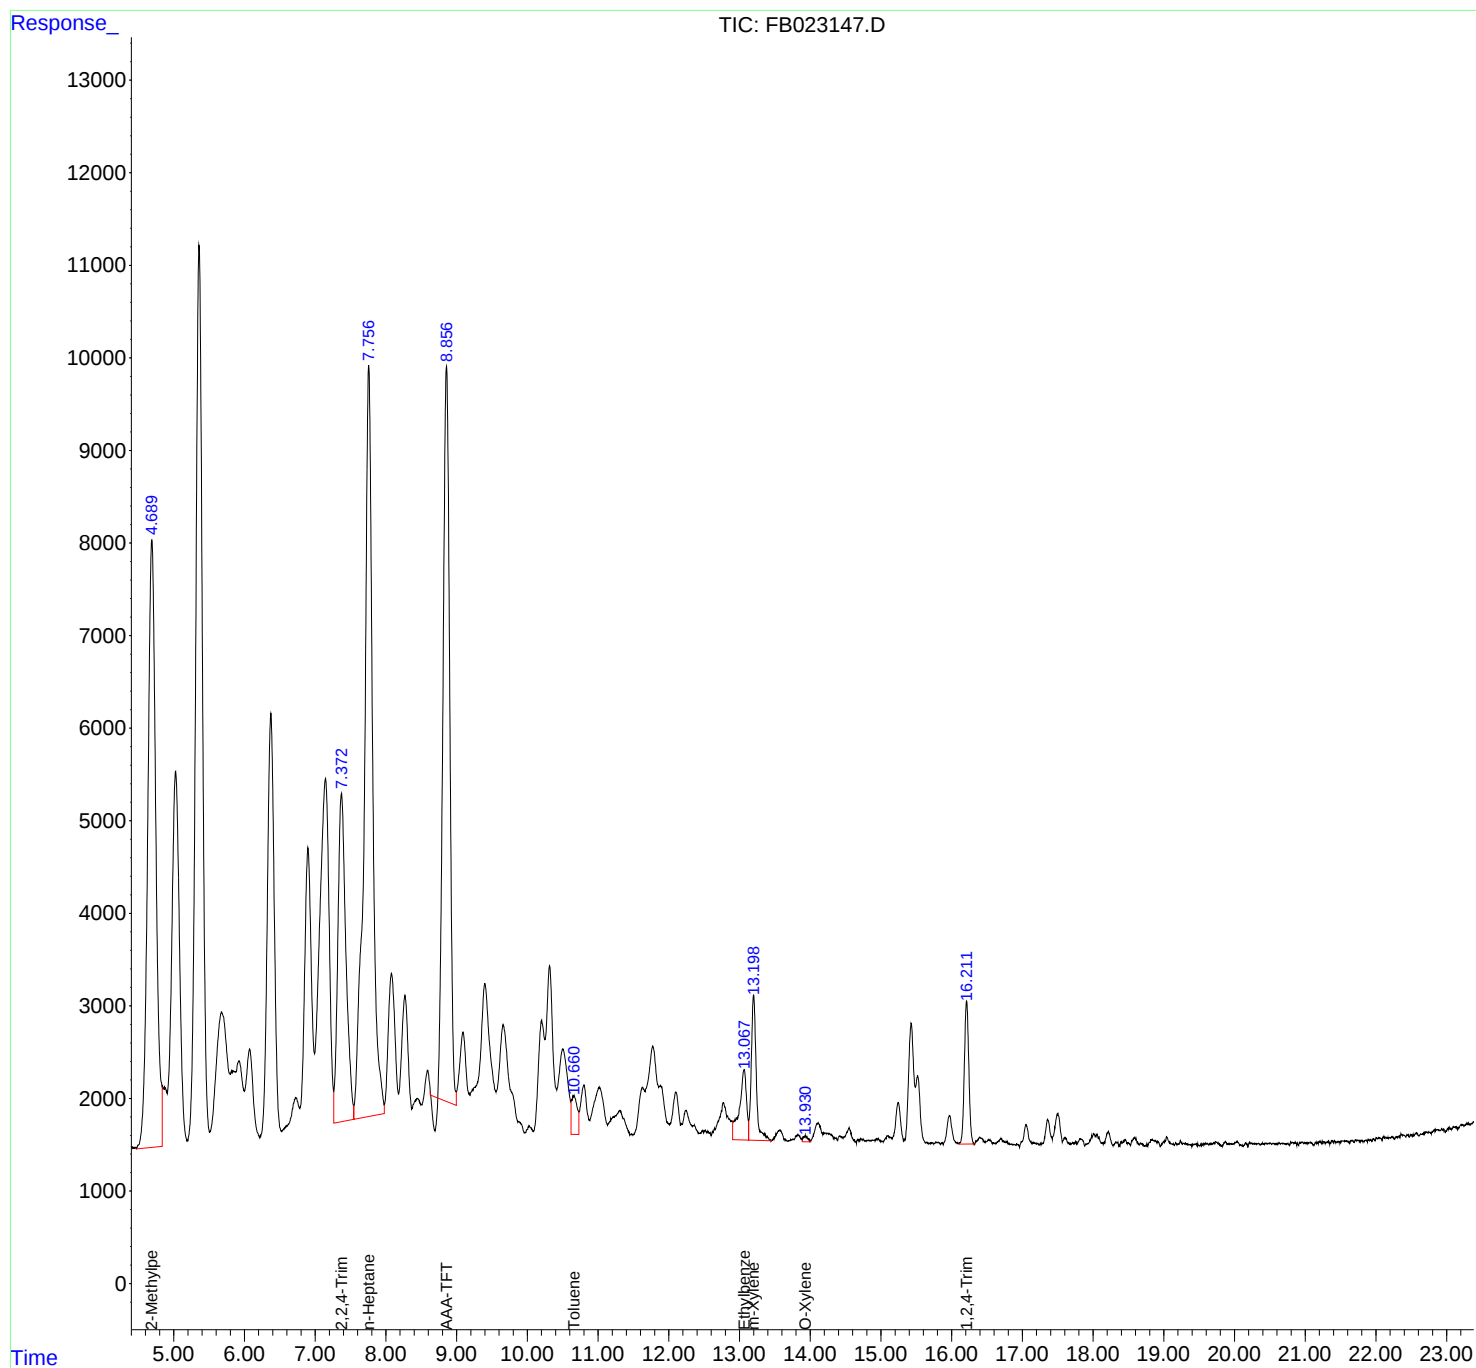


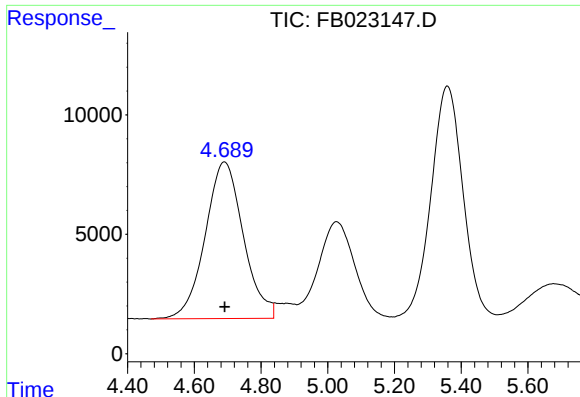

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 521866
Conc: 15.97 ng/ml

Instrument :
FID_B
ClientSampleId :

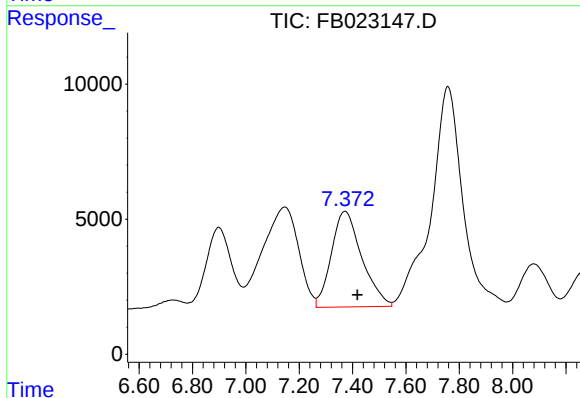


#2 2,2,4-Trimethylpentane

R.T.: 7.372 min
Delta R.T.: -0.046 min
Response: 281223
Conc: 8.06 ng/ml

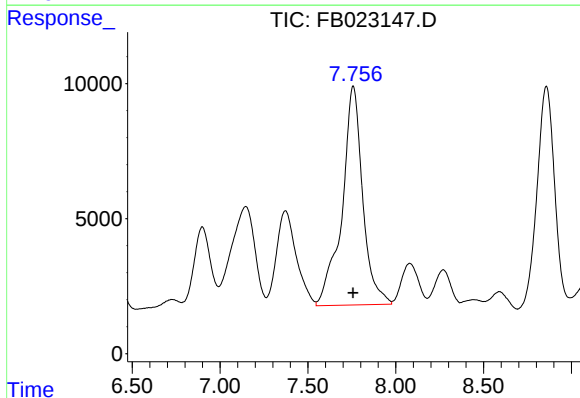


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 663743
Conc: 19.30 ng/ml

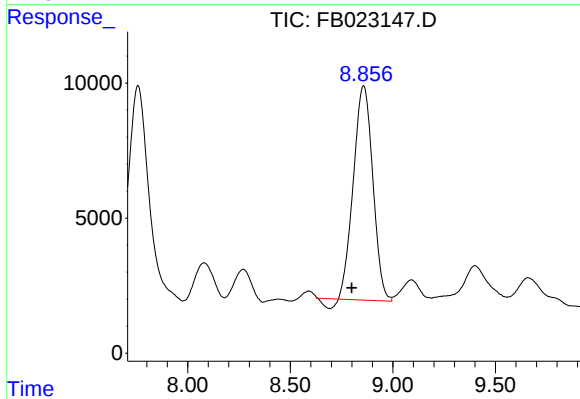

#5 AAA-TFT


R.T.: 8.858 min
Delta R.T.: 0.058 min
Response: 513740
Conc: 20.91 ng/ml

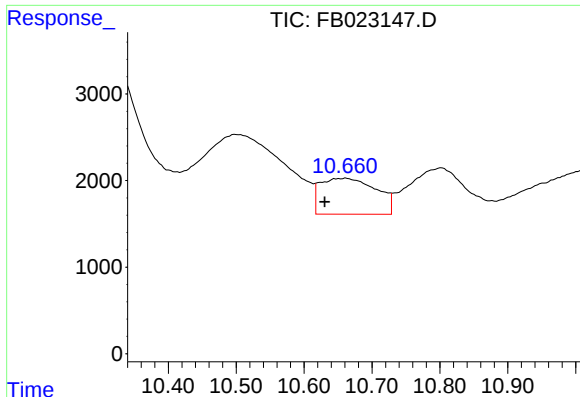

#6 Toluene


R.T.: 10.658 min
Delta R.T.: 0.028 min
Response: 23650
Conc: 0.59 ng/ml

Instrument :
FID_B
ClientSampleId :

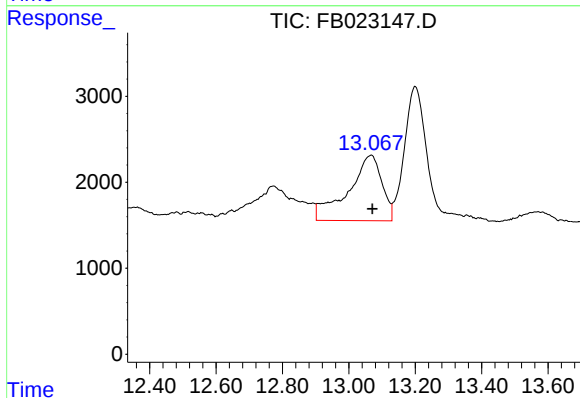


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.005 min
Response: 53708
Conc: 1.39 ng/ml

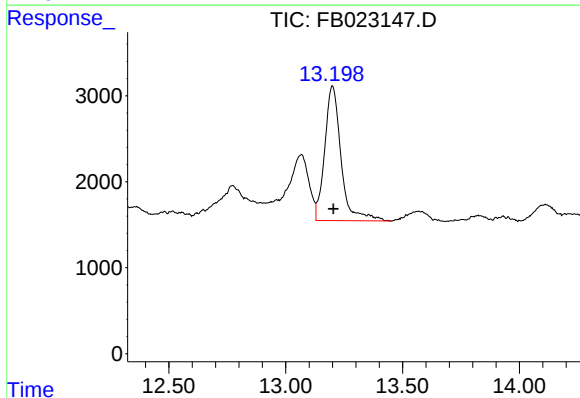


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 76123
Conc: 2.09 ng/ml

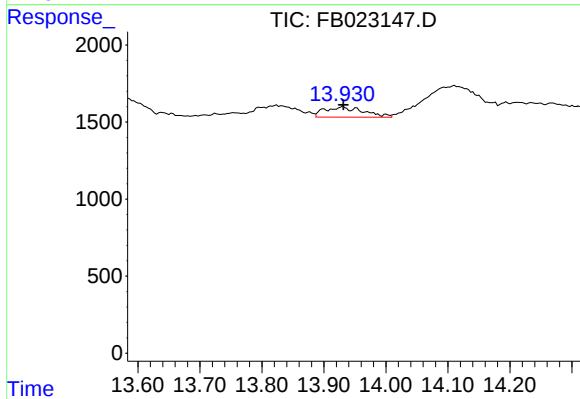

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 2885
Conc: 0.08 ng/ml

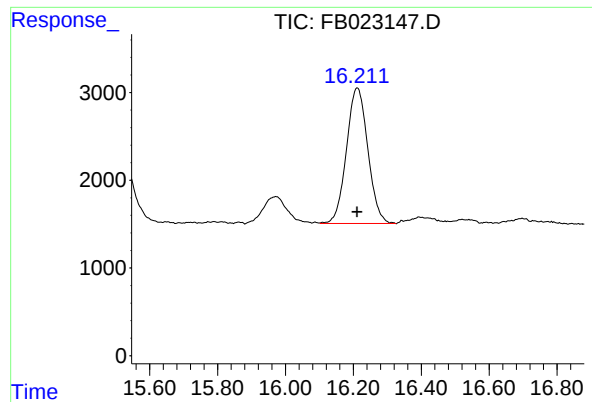

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.002 min
Response: 67508
Conc: 2.41 ng/ml

Instrument :
FID_B
ClientSampleId :