

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
 Data File : FB023140.D
 Signal(s) : FID2B.CH
 Acq On : 5 Dec 2019 11:19
 Operator : DD/AJ
 Sample : BSF1205S1
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1205S1

Integration File: Calibration.e
 Quant Time: Dec 06 00:17:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	533651	21.725 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	1001933	30.661 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	1123741	32.226 ng/ml
3) t n-Heptane	7.756	365210	10.622 ng/ml
4) t Benzene	7.891	436729	10.482 ng/ml
6) t Toluene	10.629	1274845	31.647 ng/ml
7) t Ethylbenzene	13.069	392961	10.183 ng/ml
8) t m-Xylene	13.202	746486	20.514 ng/ml
9) t O-Xylene	13.930	718702	20.699 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	596151	21.258 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
Data File : FB023140.D
Signal(s) : FID2B.CH
Acq On : 5 Dec 2019 11:19
Operator : DD/AJ
Sample : BSF1205S1
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1205S1

Integration File: Calibration.e
Quant Time: Dec 06 00:17:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

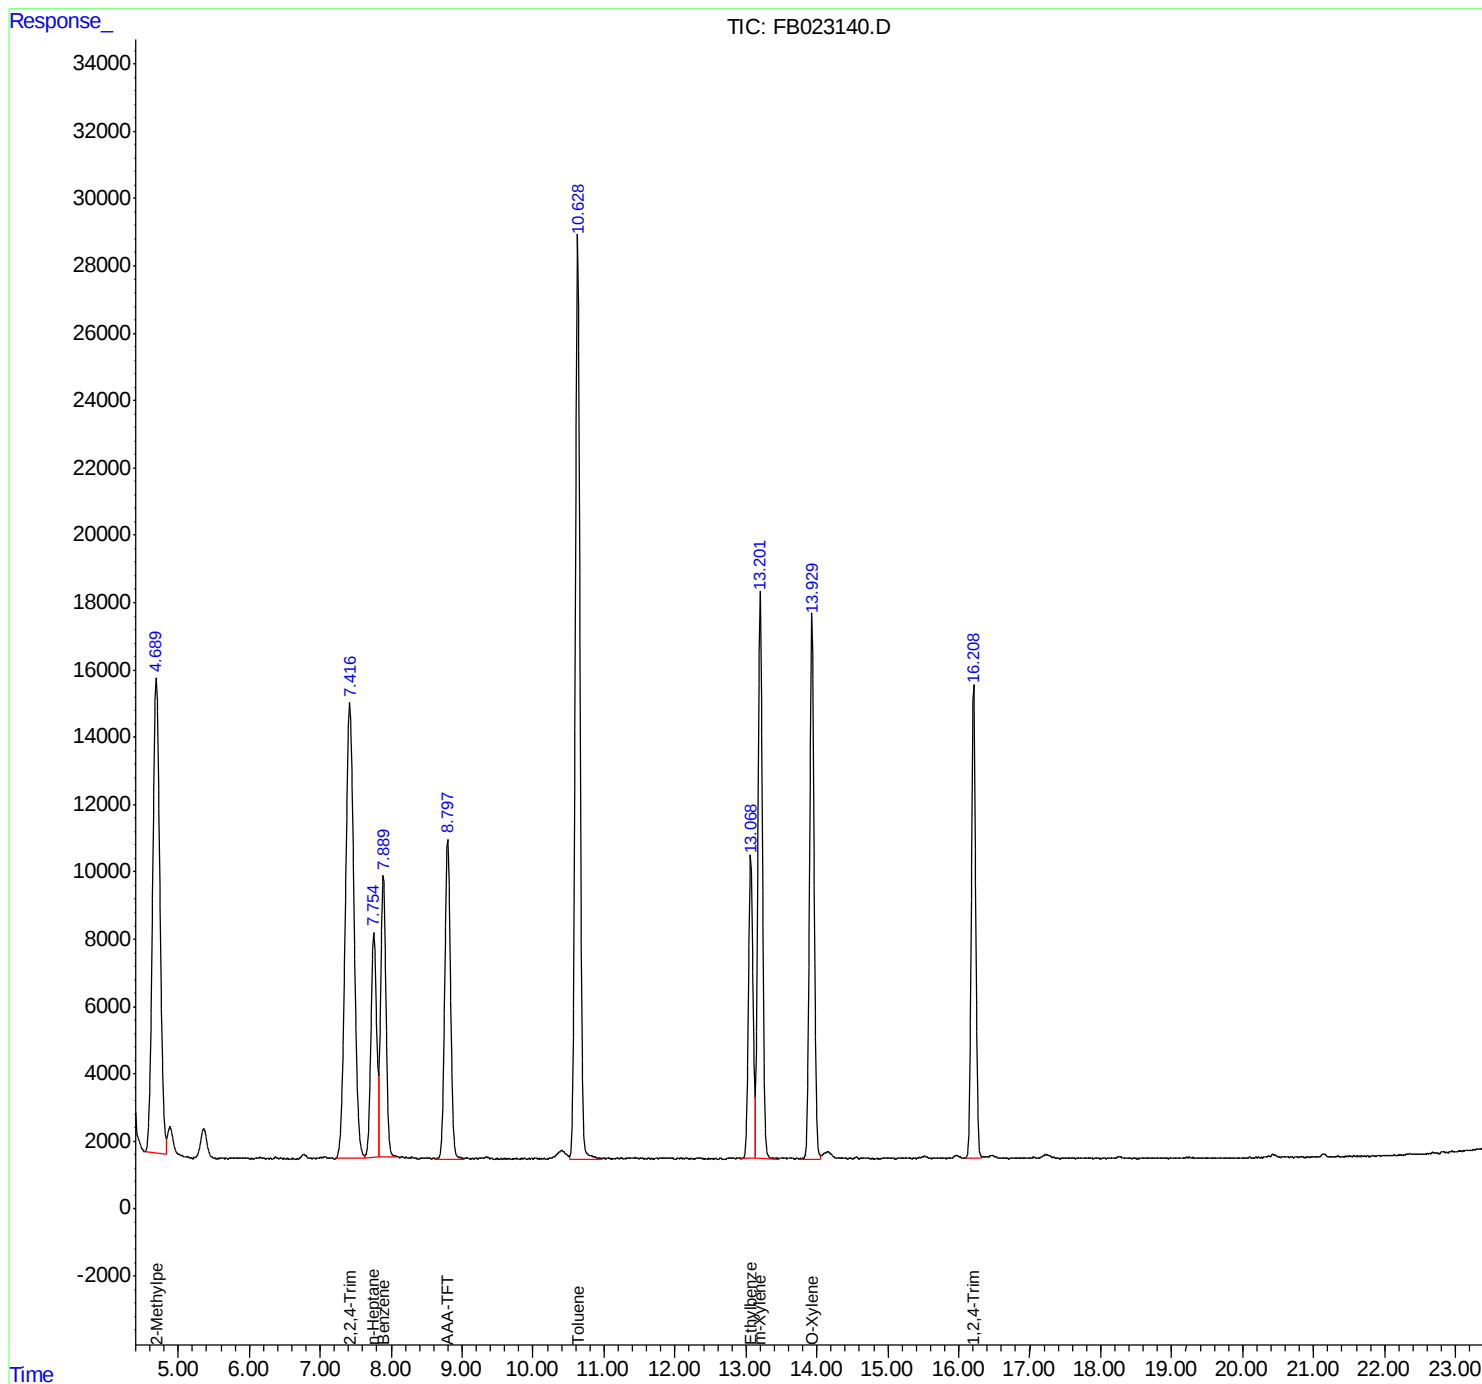


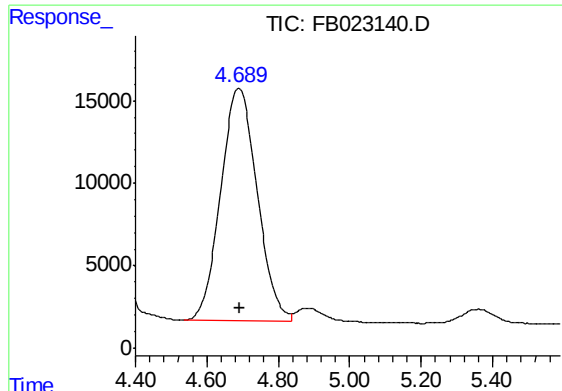

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 1001933
Conc: 30.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1205S1

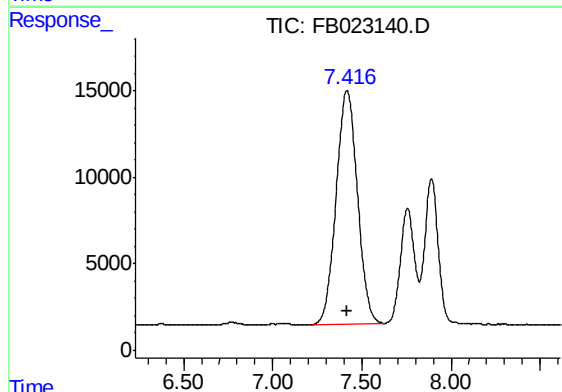


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.001 min
Response: 1123741
Conc: 32.23 ng/ml

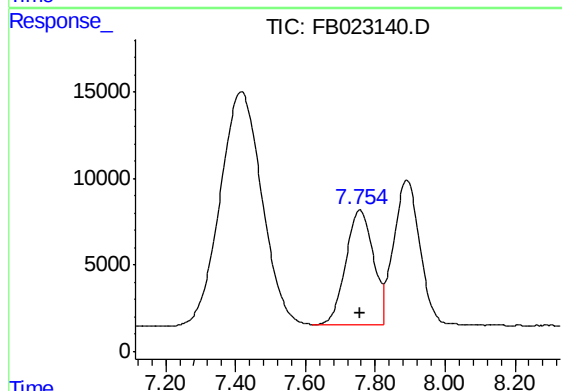


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 365210
Conc: 10.62 ng/ml

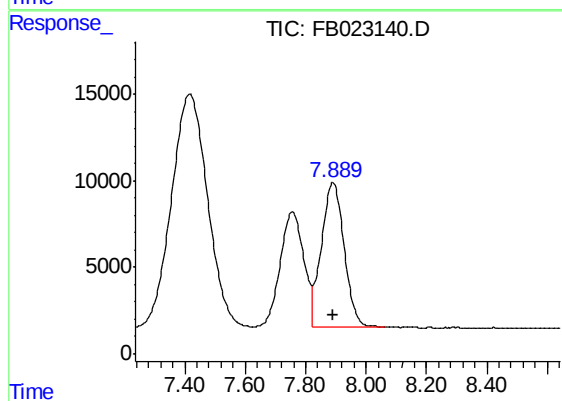

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 436729
Conc: 10.48 ng/ml

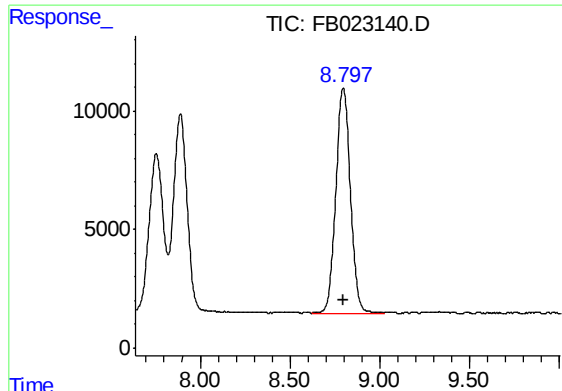

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 533651
Conc: 21.72 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1205S1

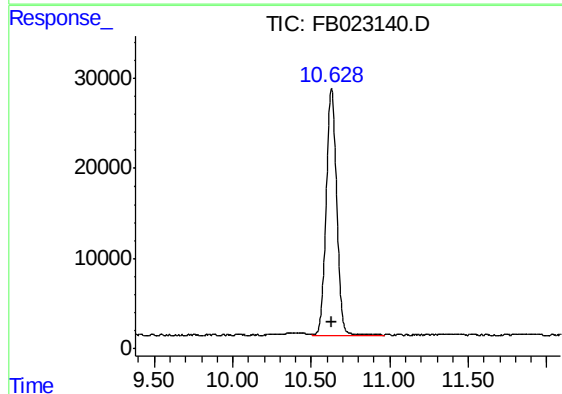


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.002 min
Response: 1274845
Conc: 31.65 ng/ml

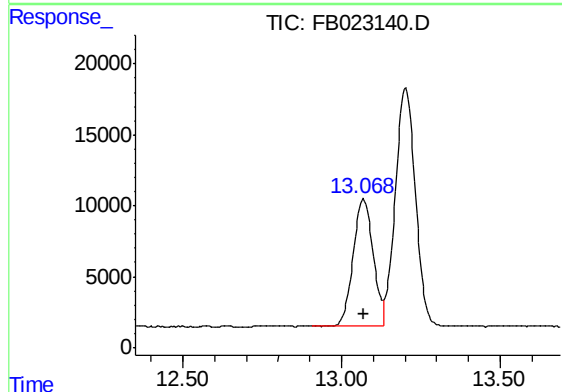


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 392961
Conc: 10.18 ng/ml

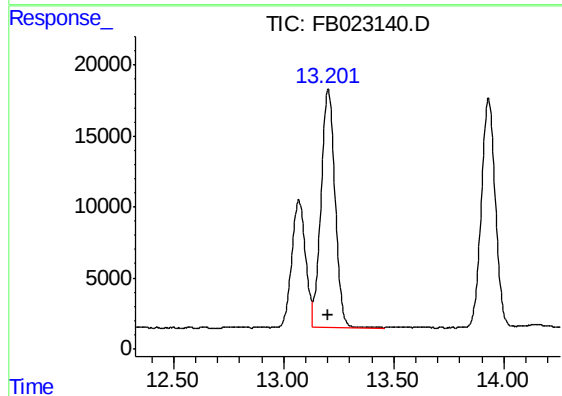

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 746486
Conc: 20.51 ng/ml

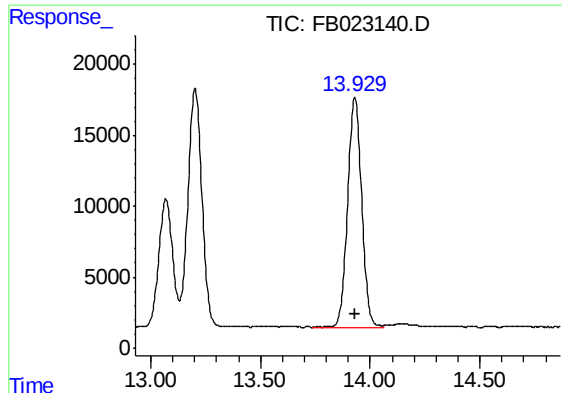

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 718702
Conc: 20.70 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1205S1

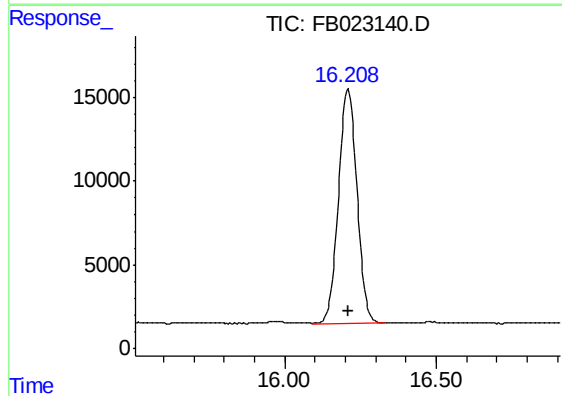

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.001 min
Response: 596151
Conc: 21.26 ng/ml