

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
 Data File : FB023143.D
 Signal(s) : FID2B.CH
 Acq On : 5 Dec 2019 14:46
 Operator : DD/AJ
 Sample : K6119-05MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-4-(0-2)MS

Integration File: Calibration.e
 Quant Time: Dec 06 00:18:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	422292	17.192 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	757179	23.171 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	839525	24.075 ng/ml
3) t n-Heptane	7.756	272389	7.922 ng/ml
4) t Benzene	7.890	345433	8.291 ng/ml
6) t Toluene	10.628	1000254	24.830 ng/ml
7) t Ethylbenzene	13.068	322191	8.349 ng/ml
8) t m-Xylene	13.201	617627	16.973 ng/ml
9) t O-Xylene	13.929	590556	17.009 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	466579	16.638 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
Data File : FB023143.D
Signal(s) : FID2B.CH
Acq On : 5 Dec 2019 14:46
Operator : DD/AJ
Sample : K6119-05MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-4-(0-2)MS

Integration File: Calibration.e
Quant Time: Dec 06 00:18:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

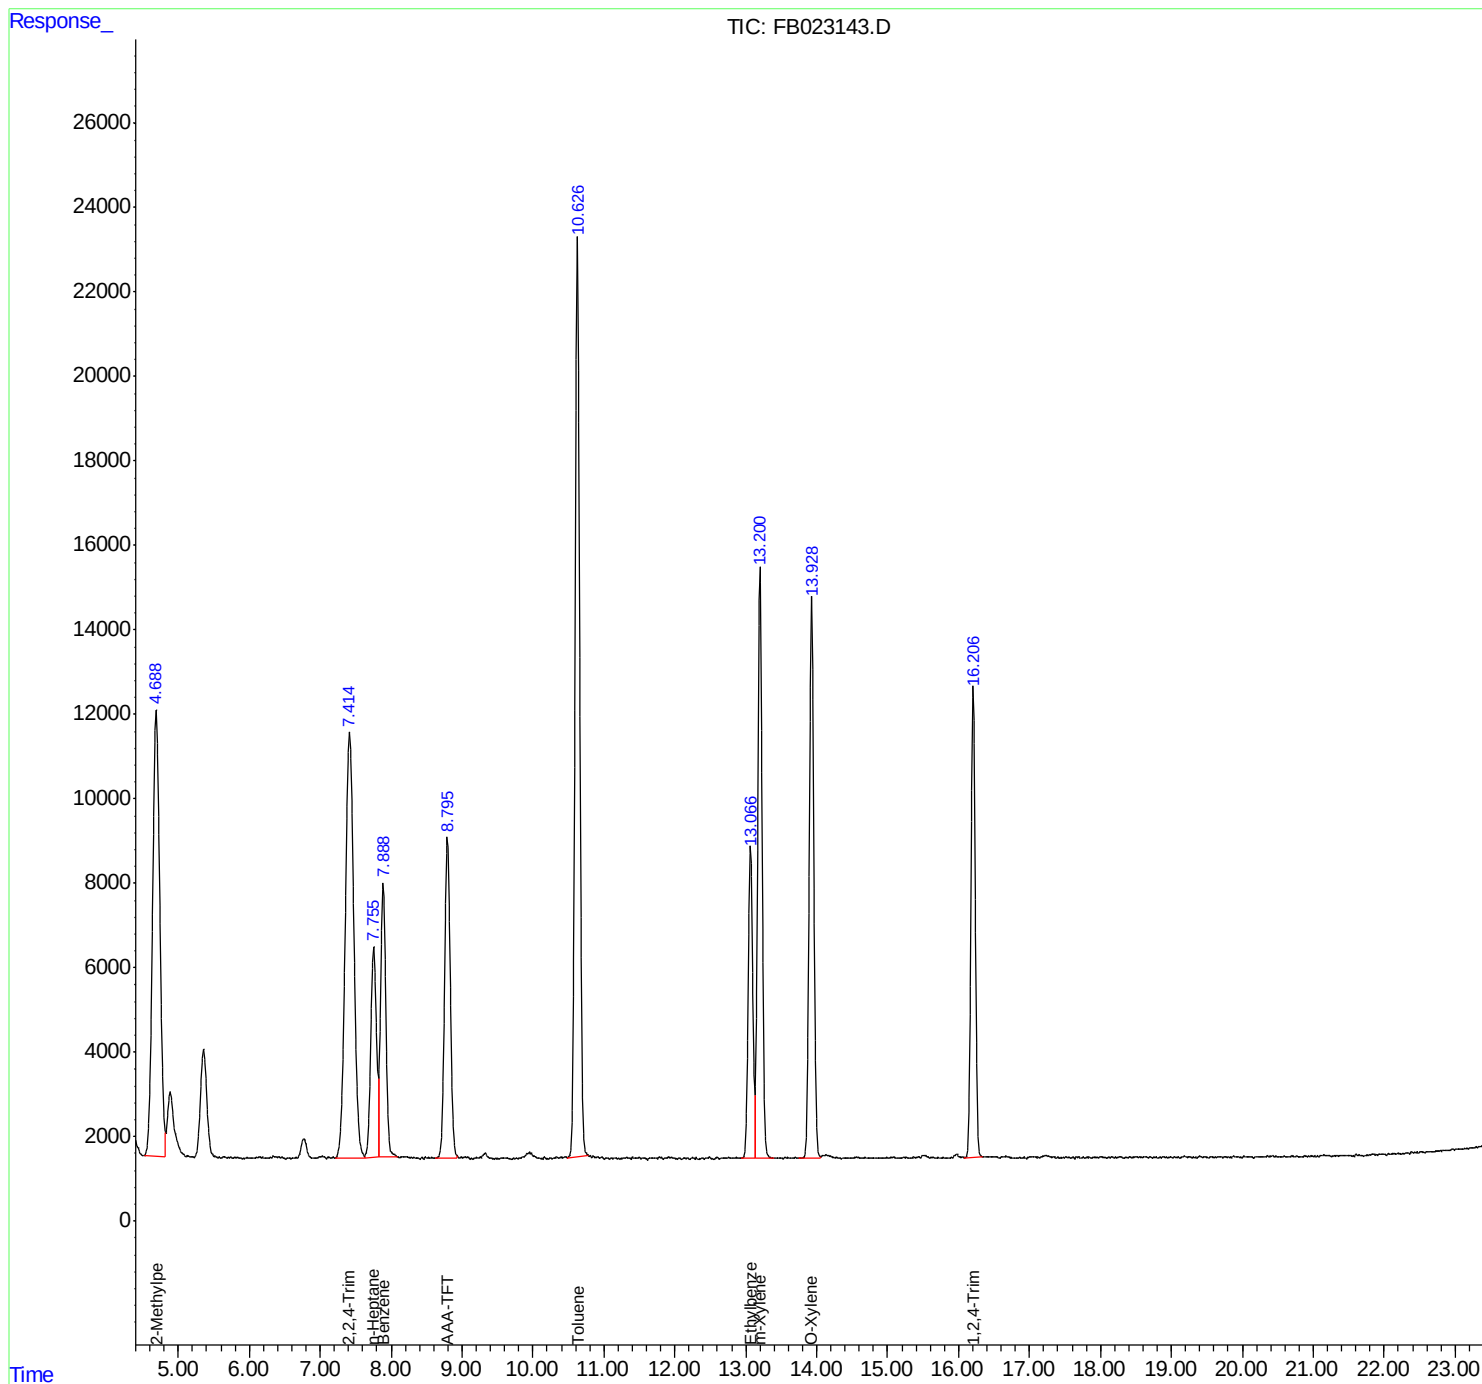


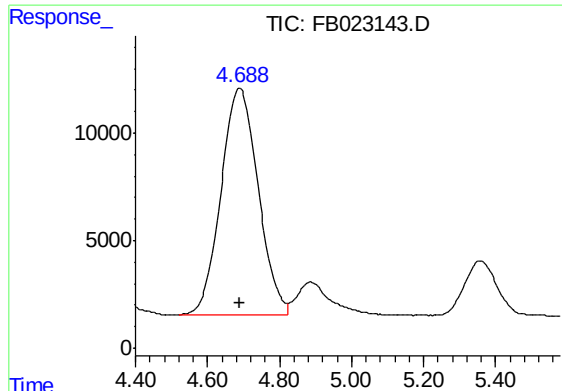

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: -0.001 min
Response: 757179
Conc: 23.17 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-4-(0-2)MS

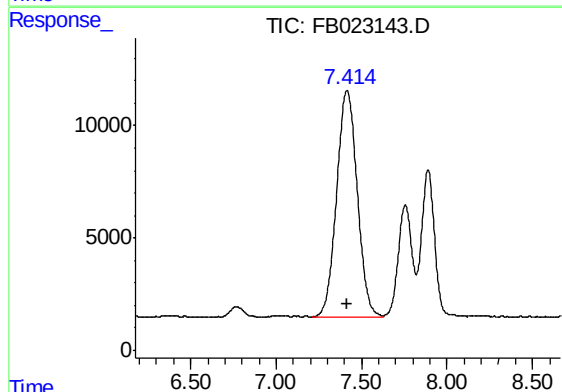


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 839525
Conc: 24.08 ng/ml

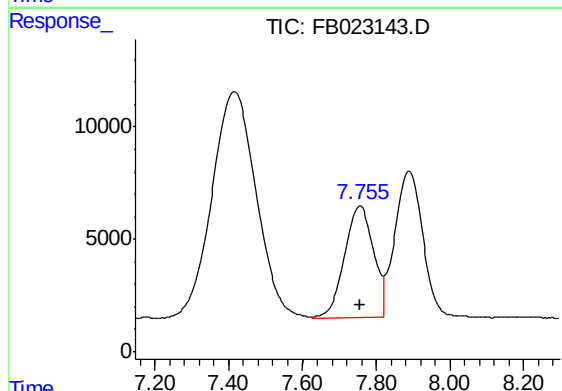


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 272389
Conc: 7.92 ng/ml

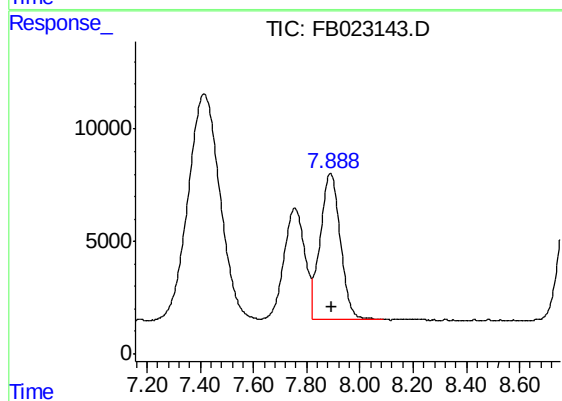

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 345433
Conc: 8.29 ng/ml

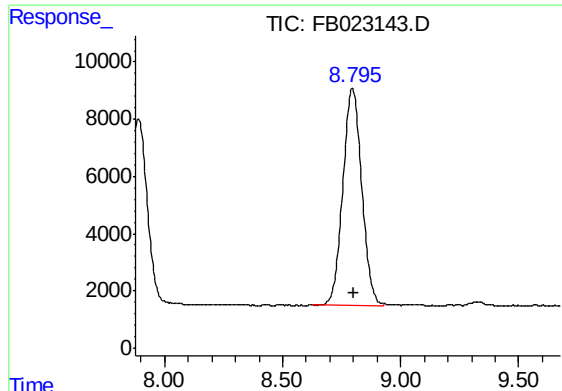

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 422292
Conc: 17.19 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-4-(0-2)MS

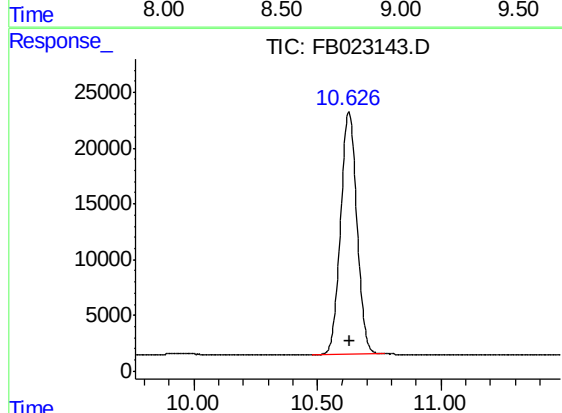


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 1000254
Conc: 24.83 ng/ml

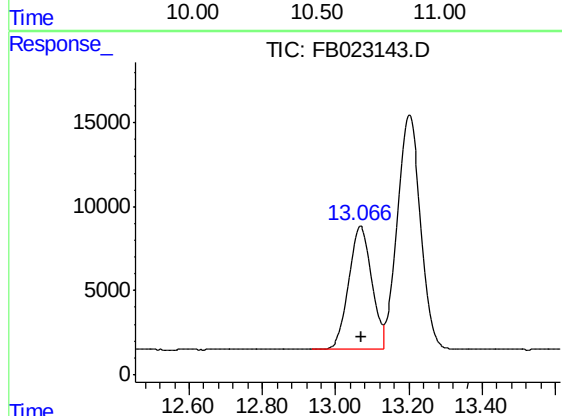


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 322191
Conc: 8.35 ng/ml

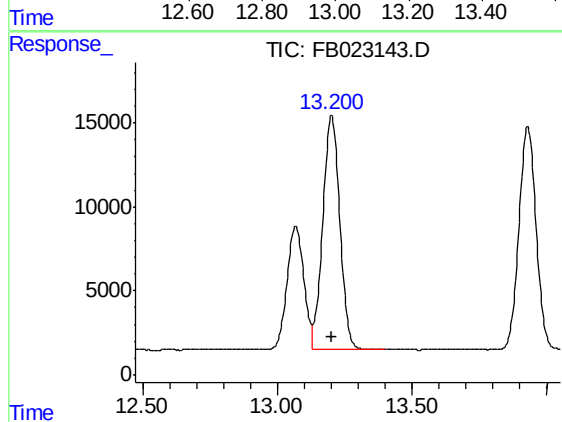

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 617627
Conc: 16.97 ng/ml

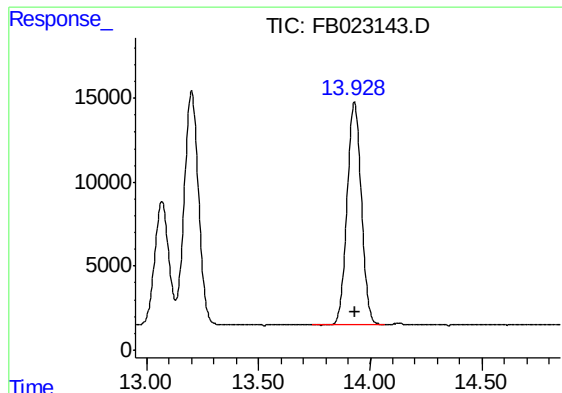

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 590556
Conc: 17.01 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-4-(0-2)MS

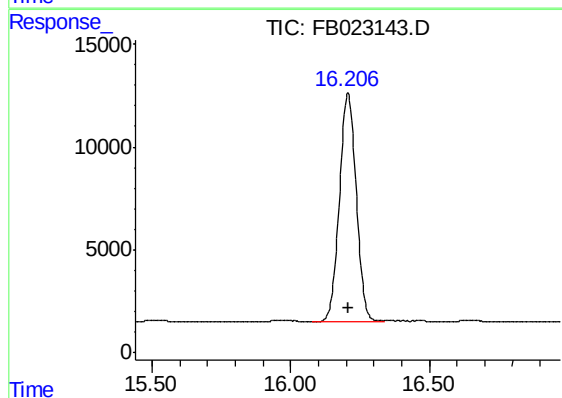

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.003 min
Response: 466579
Conc: 16.64 ng/ml