

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
Data File : FB023147.D
Signal(s) : FID2B.CH
Acq On : 5 Dec 2019 17:34
Operator : DD/AJ
Sample : K6174-02
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SOLID-COMP

Manual Integrations
APPROVED

Ankita
12/6/2019 3:06:13 PM

Integration File: Calibration.e
Quant Time: Dec 06 00:18:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.856	577222	23.499 ng/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120519\
Data File : FB023147.D
Signal(s) : FID2B.CH
Acq On : 5 Dec 2019 17:34
Operator : DD/AJ
Sample : K6174-02
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1


Instrument :
FID_B
ClientSampleId :
SOLID-COMP


Manual Integrations
APPROVED

Ankita
12/6/2019 3:06:13 PM

Integration File: Calibration.e
Quant Time: Dec 06 00:18:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

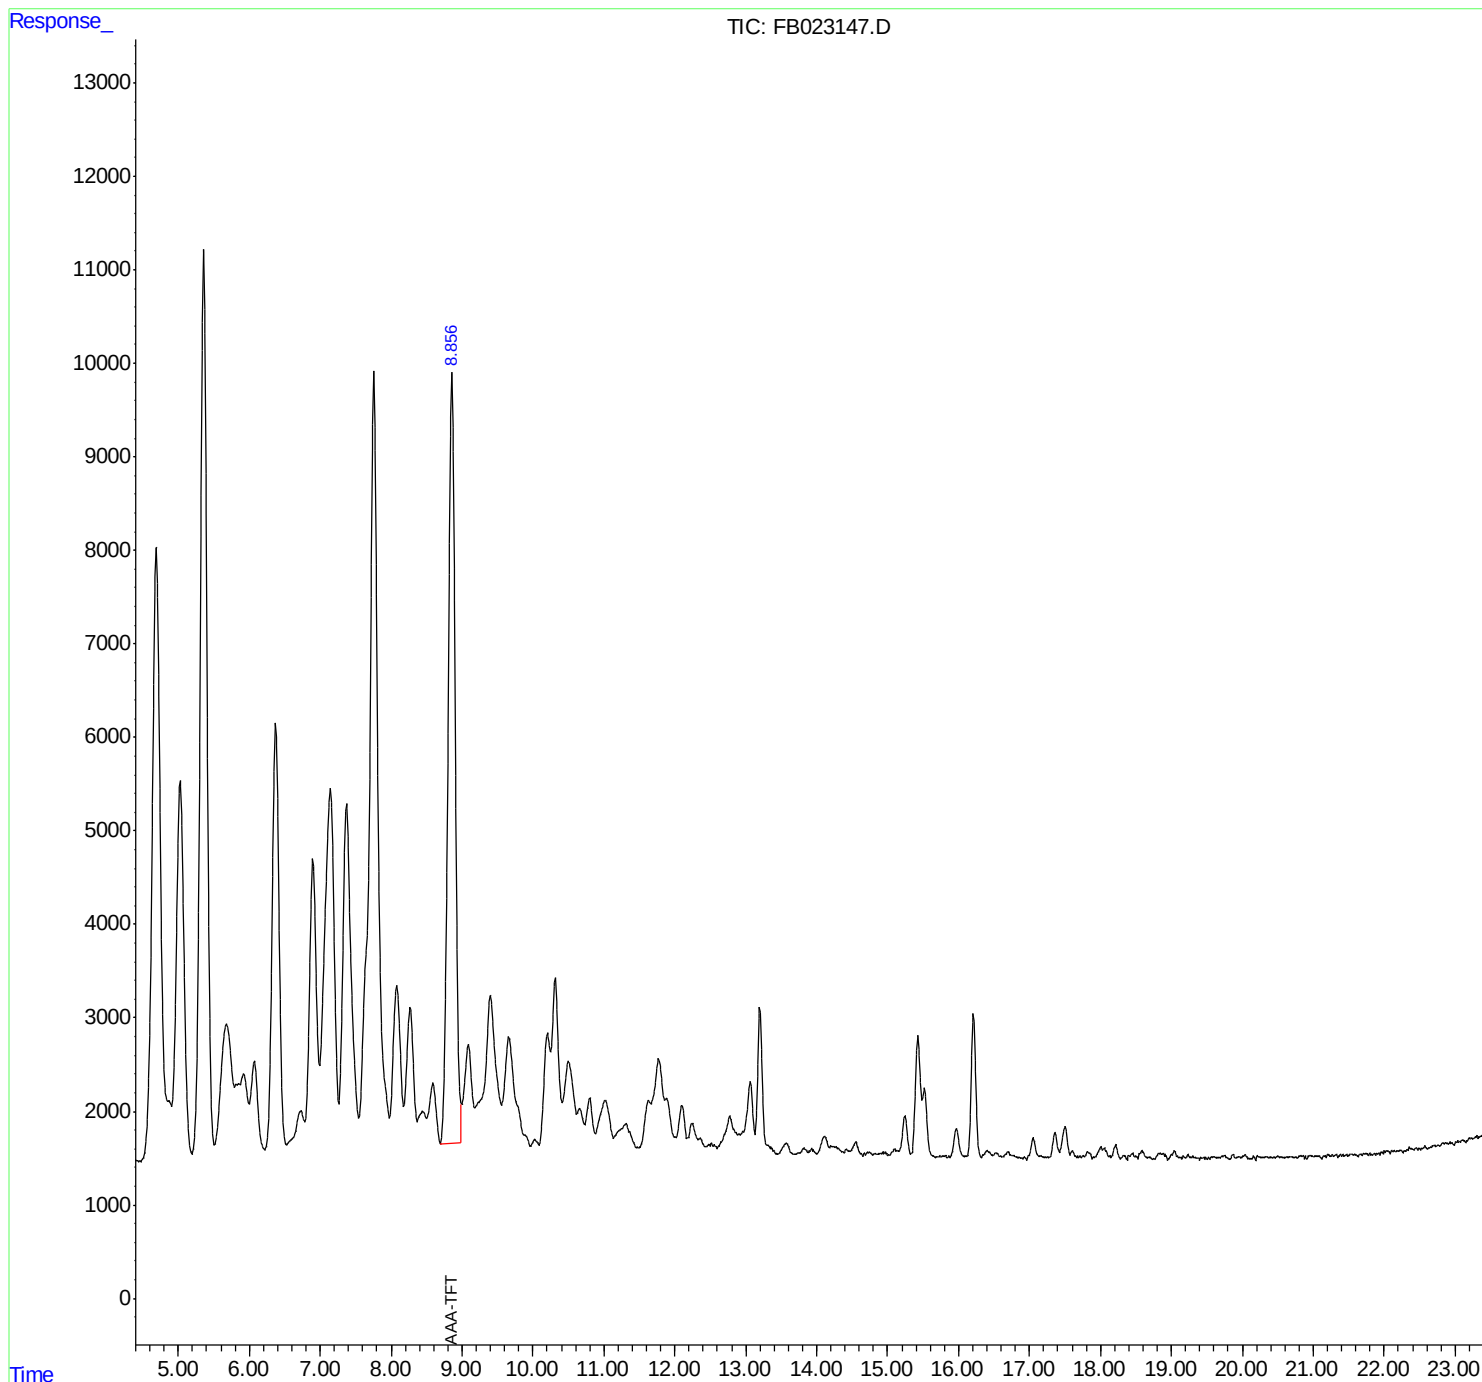

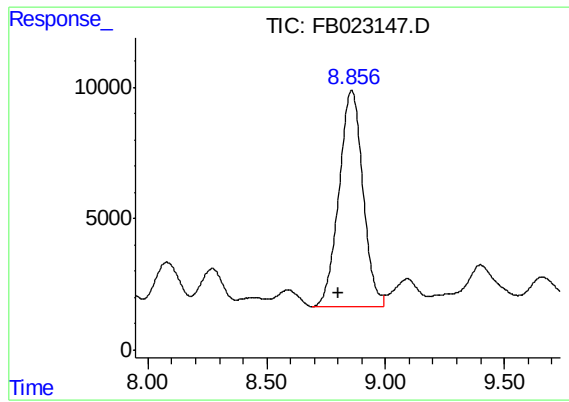

#5 AAA-TFT

R.T.: 8.856 min
Delta R.T.: 0.057 min
Response: 577222
Conc: 23.50 ng/ml m

Instrument :
FID_B
ClientSampleId :
SOLID-COMP

Manual Integrations
APPROVED

Ankita
12/6/2019 3:06:13 PM