

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB120618\
Data File : FB018950.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2018 9:19
Operator : MJ/SJ
Sample : BSF1206S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 06 16:29:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110918.M
Quant Title :
QLast Update : Fri Nov 09 10:53:13 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.106	159319	18.470 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.957	416807	28.498 ng/ml
2) t	2,2,4-Trimethylpentane	7.722	437644	29.836 ng/ml
3) t	n-Heptane	8.060	137065	9.502 ng/ml
4) t	Benzene	8.200	172970	9.547 ng/ml
6) t	Toluene	10.955	450454	29.788 ng/ml
7) t	Ethylbenzene	13.405	151003	9.683 ng/ml
8) t	m-Xylene	13.537	322463	19.410 ng/ml
9) t	O-Xylene	14.269	336192	19.595 ng/ml
10) t	1,2,4-Trimethylbenzene	16.552	393882	19.856 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB120618\
Data File : FB018950.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2018 9:19
Operator : MJ/SJ
Sample : BSF1206S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 06 16:29:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110918.M
Quant Title :
QLast Update : Fri Nov 09 10:53:13 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

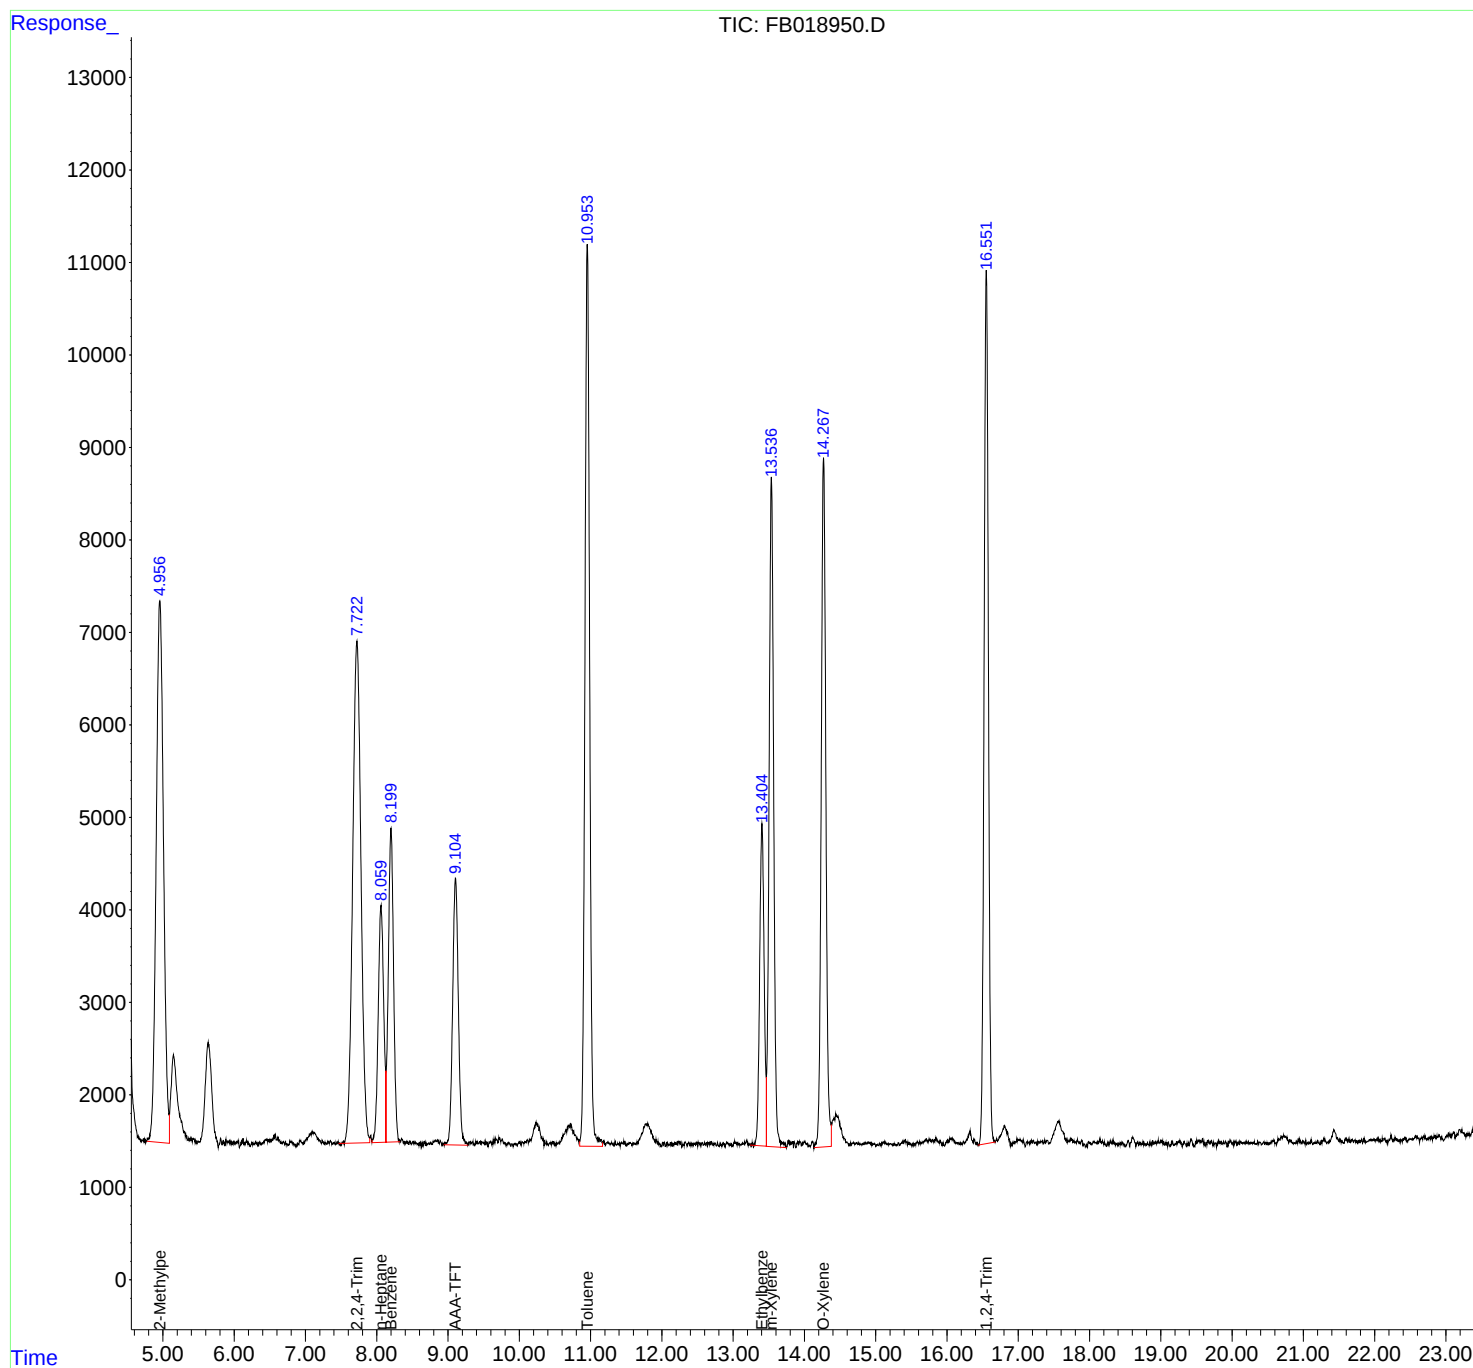

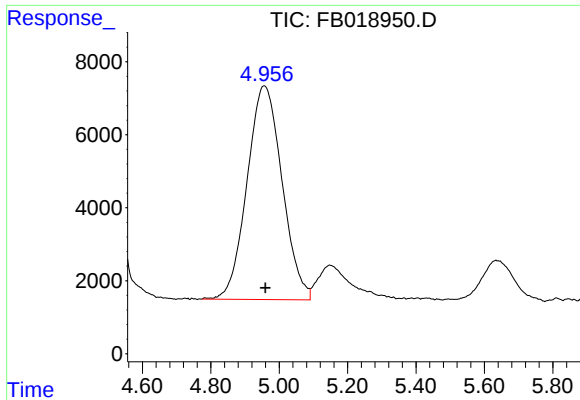


#1 2-Methylpentane

R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 416807
Conc: 28.50 ng/ml

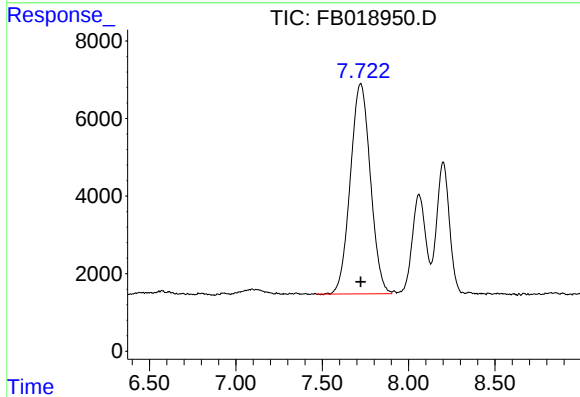


#2 2,2,4-Trimethylpentane

R.T.: 7.722 min
Delta R.T.: 0.000 min
Response: 437644
Conc: 29.84 ng/ml

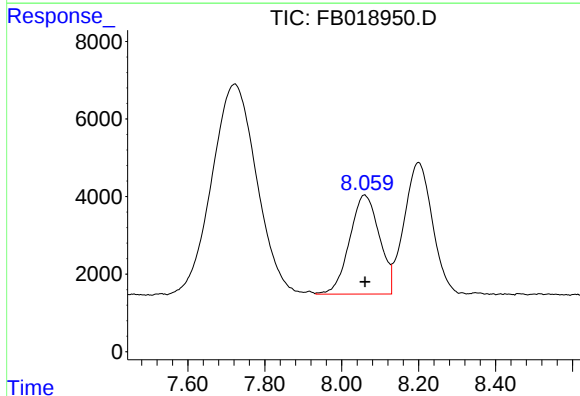


#3 n-Heptane

R.T.: 8.060 min
Delta R.T.: -0.001 min
Response: 137065
Conc: 9.50 ng/ml

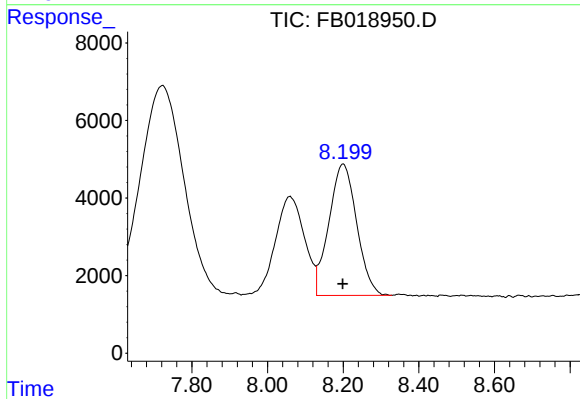


#4 Benzene

R.T.: 8.200 min
Delta R.T.: 0.001 min
Response: 172970
Conc: 9.55 ng/ml

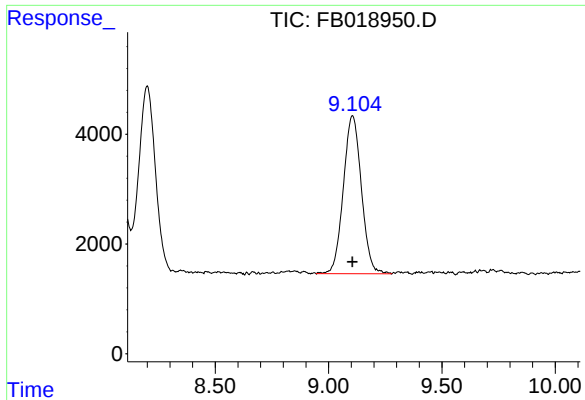


#5 AAA-TFT

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 159319
Conc: 18.47 ng/ml

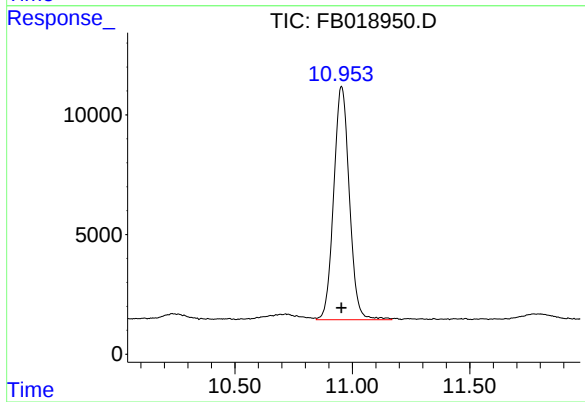


#6 Toluene

R.T.: 10.955 min
Delta R.T.: 0.000 min
Response: 450454
Conc: 29.79 ng/ml

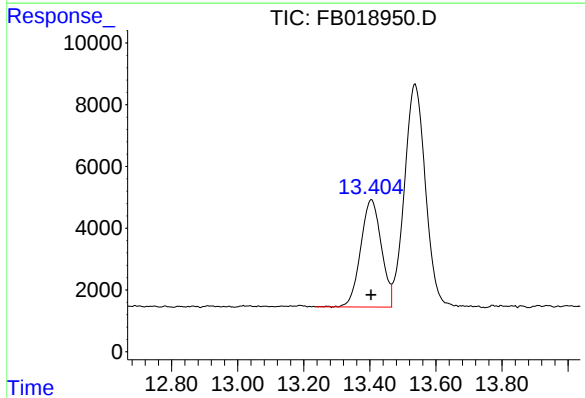


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: 0.002 min
Response: 151003
Conc: 9.68 ng/ml

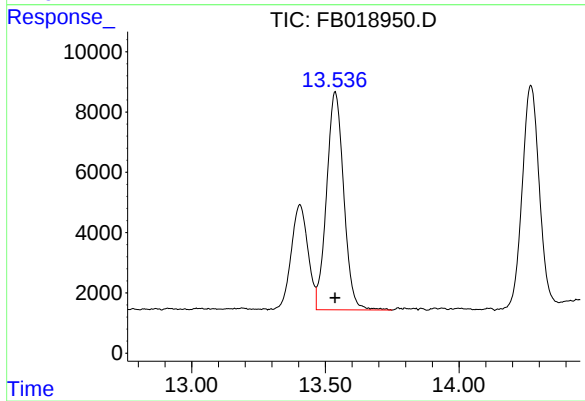


#8 m-Xylene

R.T.: 13.537 min
Delta R.T.: 0.000 min
Response: 322463
Conc: 19.41 ng/ml

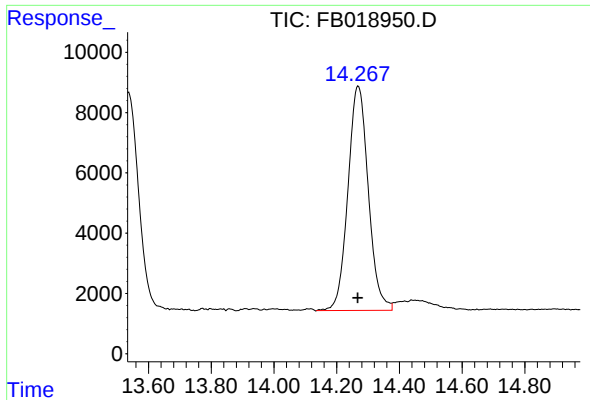

#9 O-Xylene

R.T.: 14.269 min
Delta R.T.: 0.001 min
Response: 336192
Conc: 19.60 ng/ml

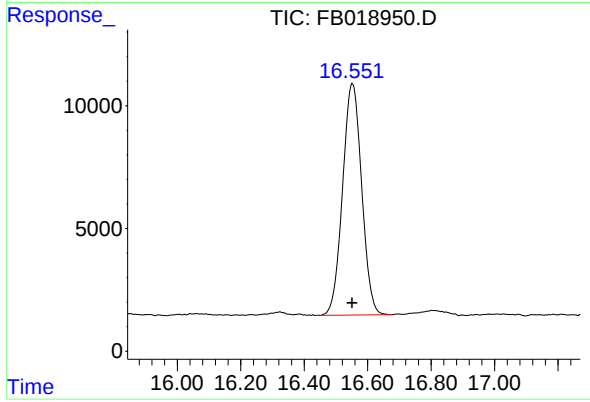

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: 0.002 min
Response: 393882
Conc: 19.86 ng/ml