

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120619\
Data File : FB023150.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2019 11:23
Operator : DD/AJ
Sample : VBF1206S1
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 06 22:30:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.793	503932	20.515 ng/ml
Target Compounds				
6) t	Toluene	10.632	3843	0.095 ng/ml
8) t	m-Xylene	13.196	3871	0.106 ng/ml
9) t	O-Xylene	13.933	3552	0.102 ng/ml
10) t	1,2,4-Trimethylbenzene	16.203	6575	0.234 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120619\
Data File : FB023150.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2019 11:23
Operator : DD/AJ
Sample : VBF1206S1
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 06 22:30:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

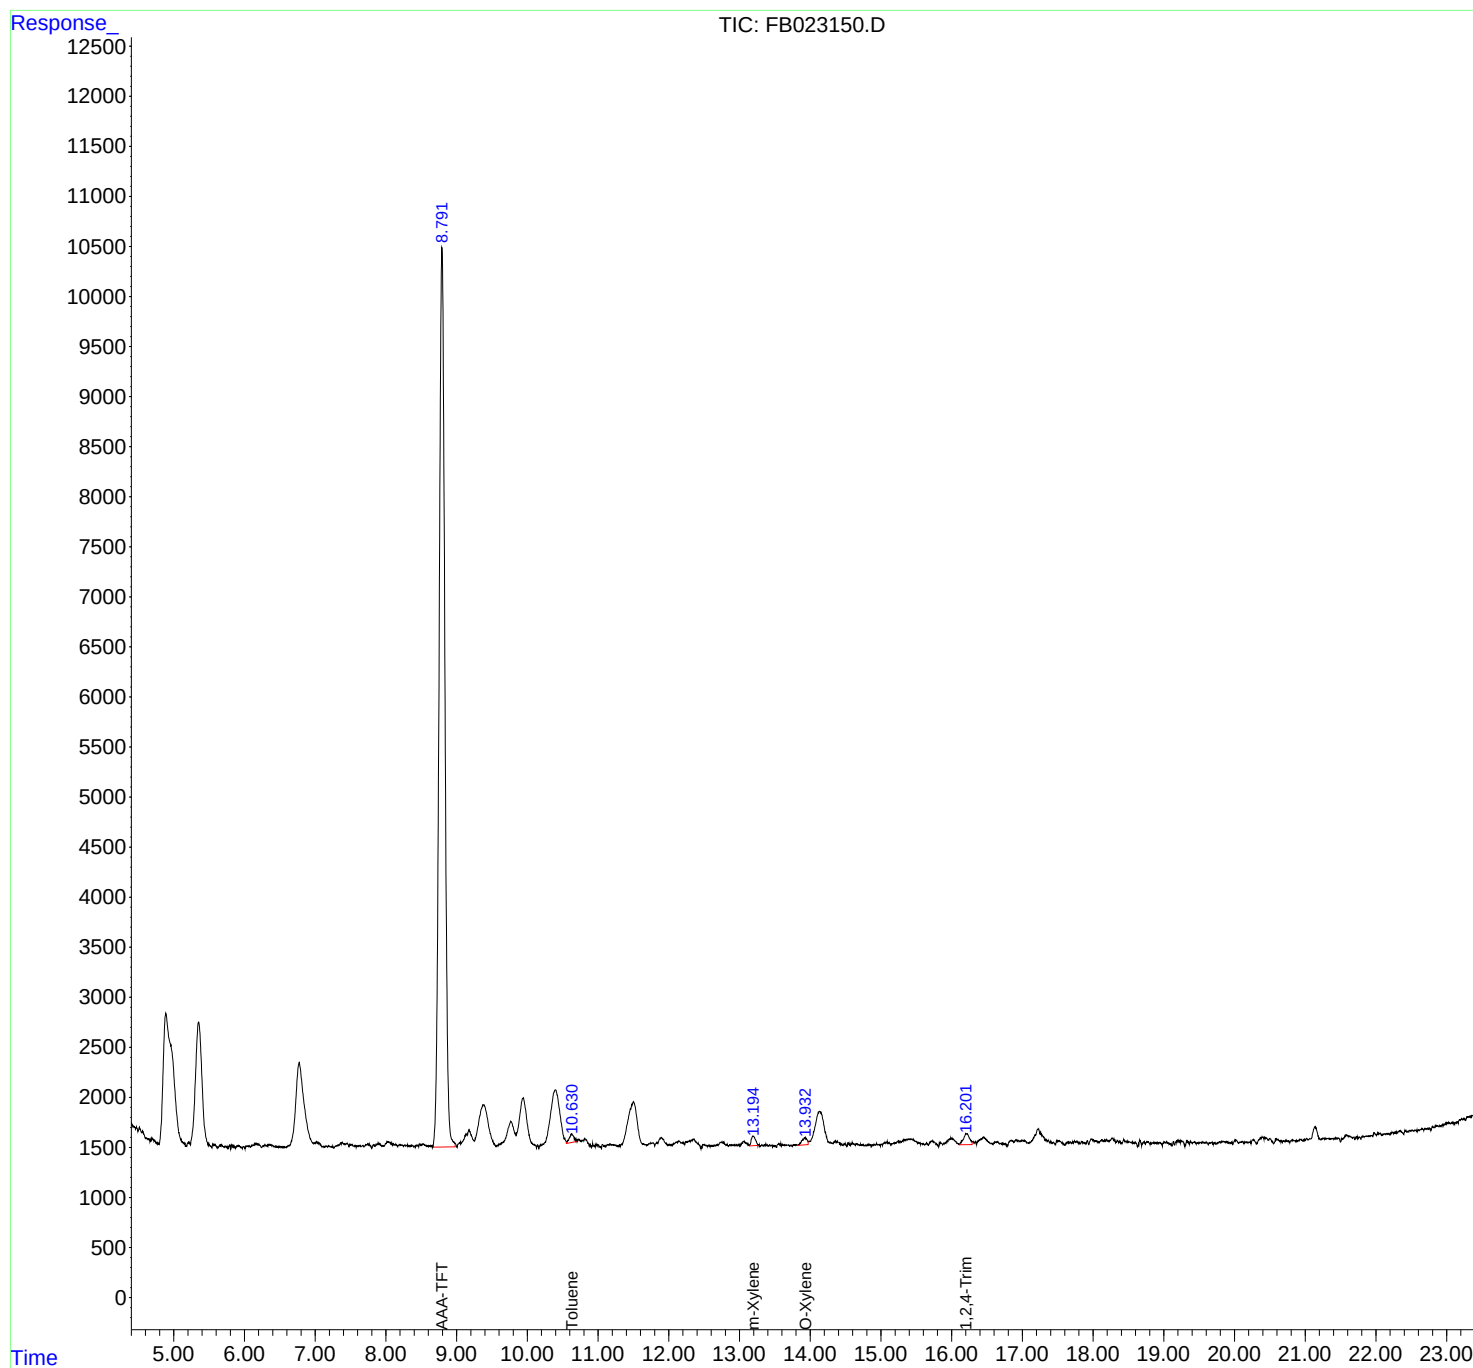

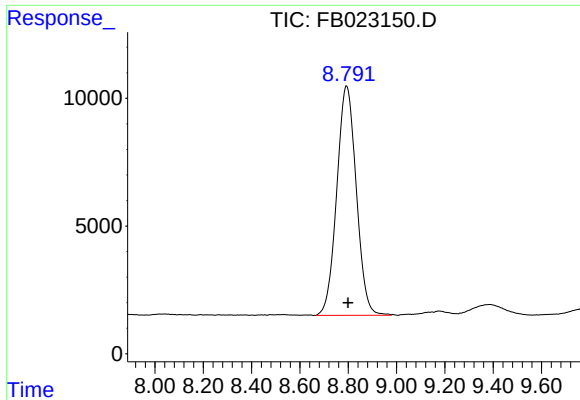


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.006 min
Response: 503932
Conc: 20.52 ng/ml

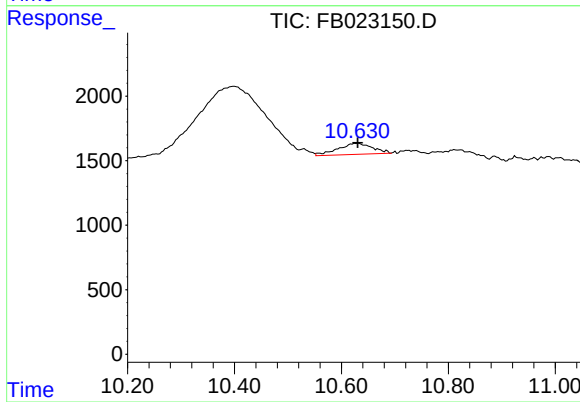


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.001 min
Response: 3843
Conc: 0.10 ng/ml

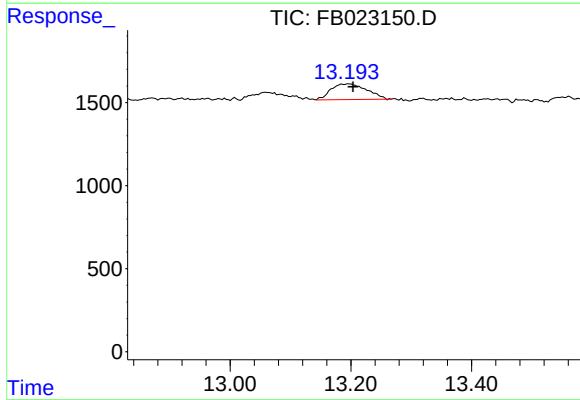


#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: -0.007 min
Response: 3871
Conc: 0.11 ng/ml

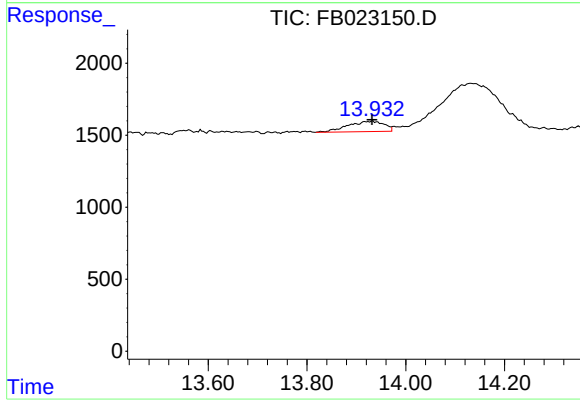

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.002 min
Response: 3552
Conc: 0.10 ng/ml

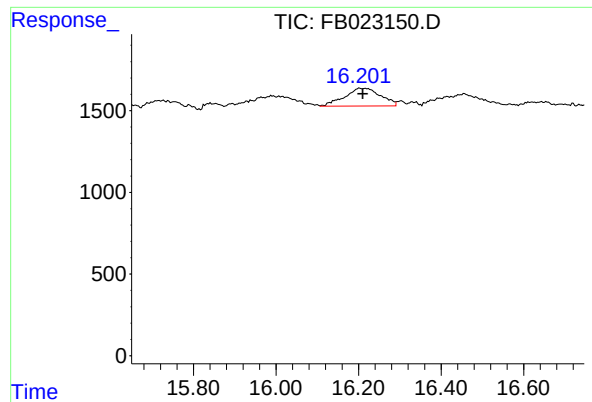

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: -0.007 min
Response: 6575
Conc: 0.23 ng/ml