

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120619\
 Data File : FB023158.D
 Signal(s) : FID2B.CH
 Acq On : 6 Dec 2019 23:09
 Operator : DD/AJ
 Sample : K6111-02
 Misc : 4.99g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 07 02:15:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	521481	21.230 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	919951	28.152 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	1076155	30.861 ng/ml
3) t n-Heptane	7.751	349449	10.163 ng/ml
4) t Benzene	7.886	421580	10.118 ng/ml
6) t Toluene	10.624	1240624	30.797 ng/ml
7) t Ethylbenzene	13.064	396305	10.270 ng/ml
8) t m-Xylene	13.197	754032	20.721 ng/ml
9) t O-Xylene	13.925	721057	20.767 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	605982	21.609 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120619\
Data File : FB023158.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2019 23:09
Operator : DD/AJ
Sample : K6111-02
Misc : 4.99g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 07 02:15:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

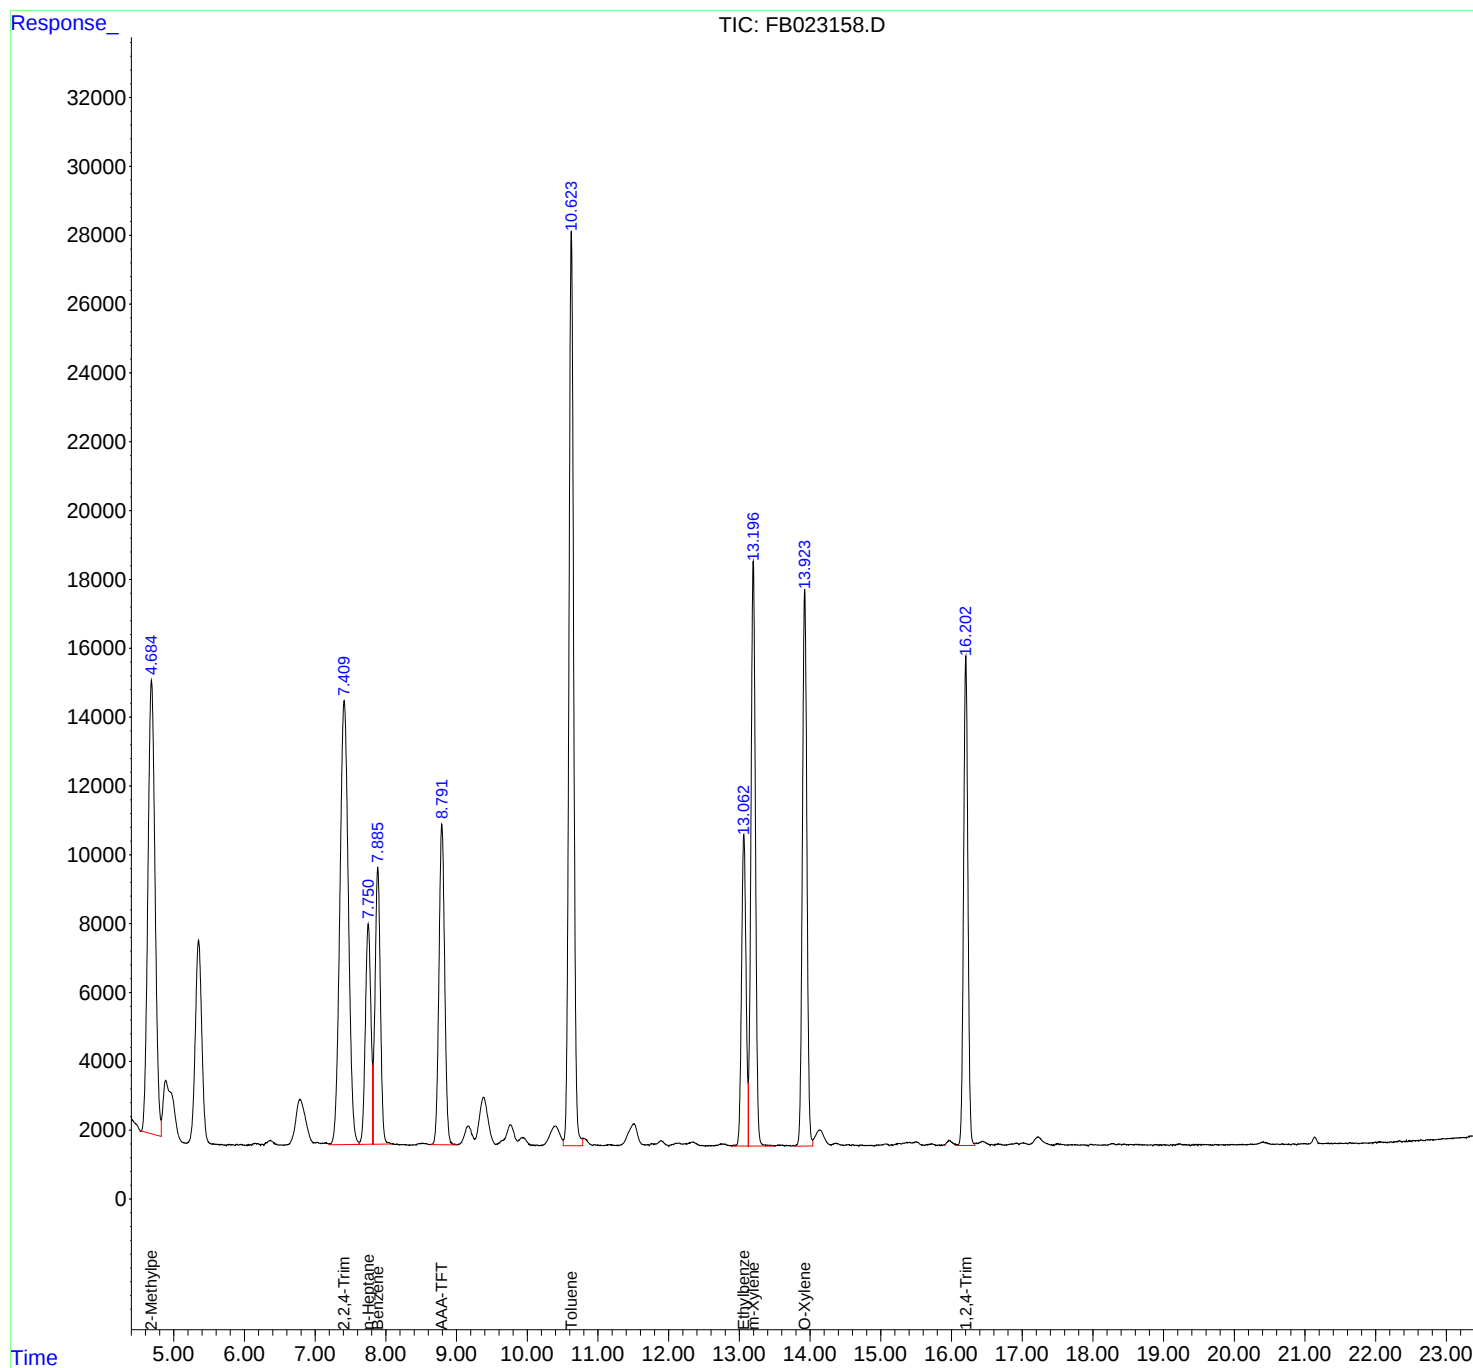

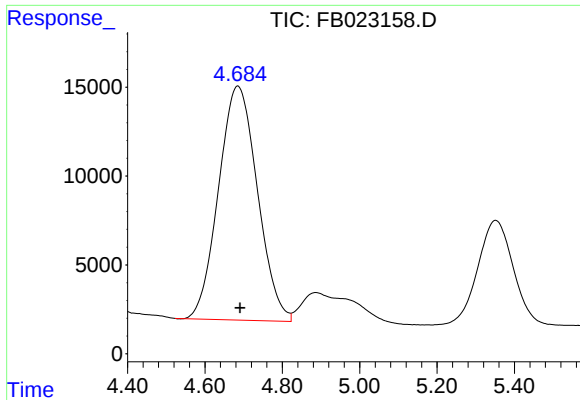


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.006 min
Response: 919951
Conc: 28.15 ng/ml

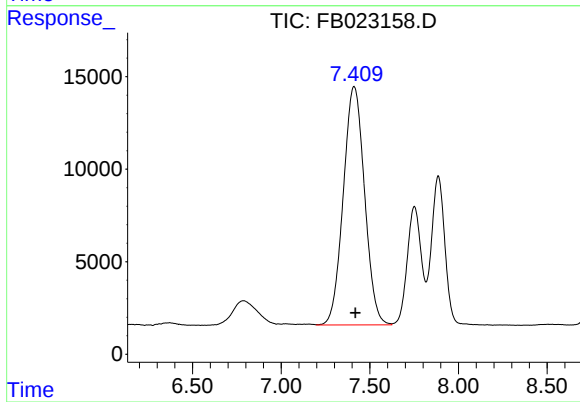


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.007 min
Response: 1076155
Conc: 30.86 ng/ml

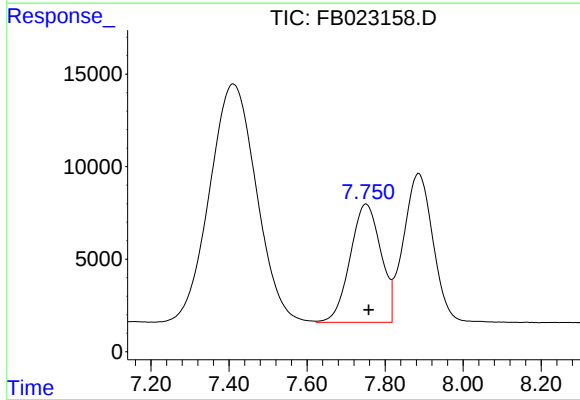


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.006 min
Response: 349449
Conc: 10.16 ng/ml

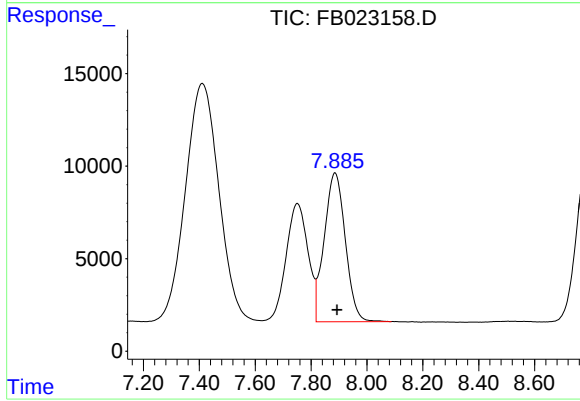


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.006 min
Response: 421580
Conc: 10.12 ng/ml

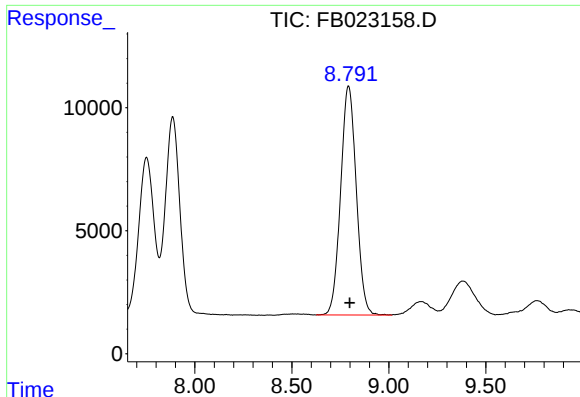


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.007 min
Response: 521481
Conc: 21.23 ng/ml

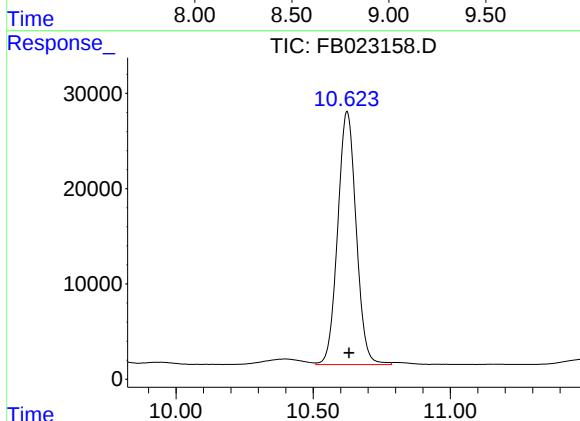


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.006 min
Response: 1240624
Conc: 30.80 ng/ml

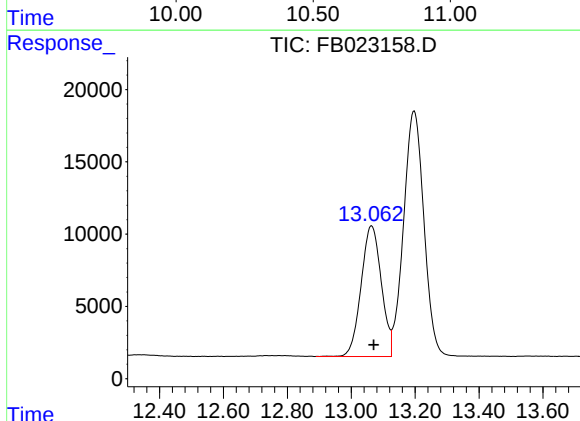


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.007 min
Response: 396305
Conc: 10.27 ng/ml

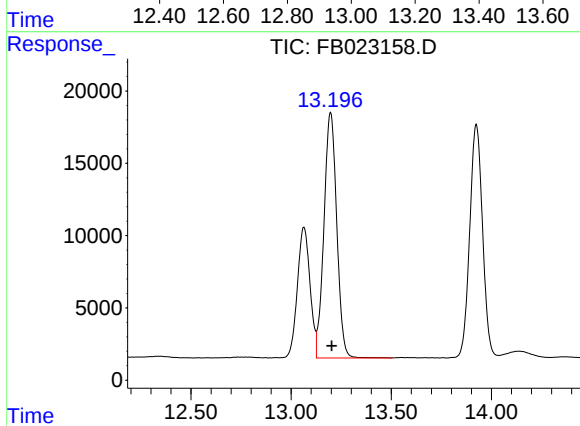


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.006 min
Response: 754032
Conc: 20.72 ng/ml

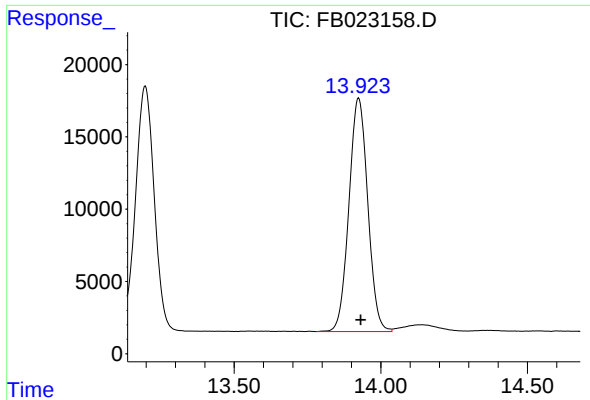

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.007 min
Response: 721057
Conc: 20.77 ng/ml

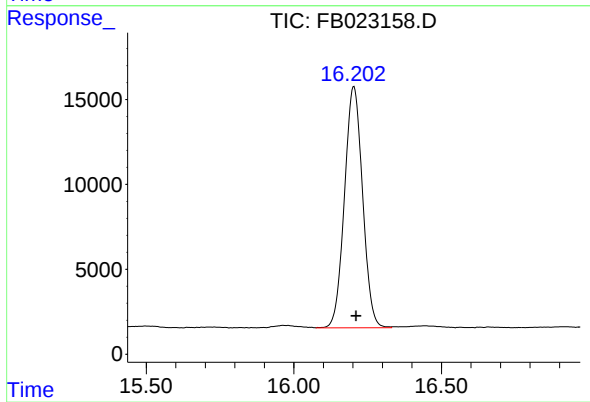

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: -0.007 min
Response: 605982
Conc: 21.61 ng/ml