

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120619\
 Data File : FB023151.D
 Signal(s) : FID2B.CH
 Acq On : 6 Dec 2019 11:53
 Operator : DD/AJ
 Sample : BSF1206S1
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 06 22:30:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.795	479653	19.527 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.687	854702	26.155 ng/ml
2) t	2,2,4-Trimethylpentane	7.413	996539	28.578 ng/ml
3) t	n-Heptane	7.754	322878	9.391 ng/ml
4) t	Benzene	7.888	399390	9.586 ng/ml
6) t	Toluene	10.626	1174184	29.148 ng/ml
7) t	Ethylbenzene	13.067	374313	9.700 ng/ml
8) t	m-Xylene	13.200	709007	19.484 ng/ml
9) t	O-Xylene	13.928	683347	19.681 ng/ml
10) t	1,2,4-Trimethylbenzene	16.206	566448	20.199 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120619\
Data File : FB023151.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2019 11:53
Operator : DD/AJ
Sample : BSF1206S1
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 06 22:30:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

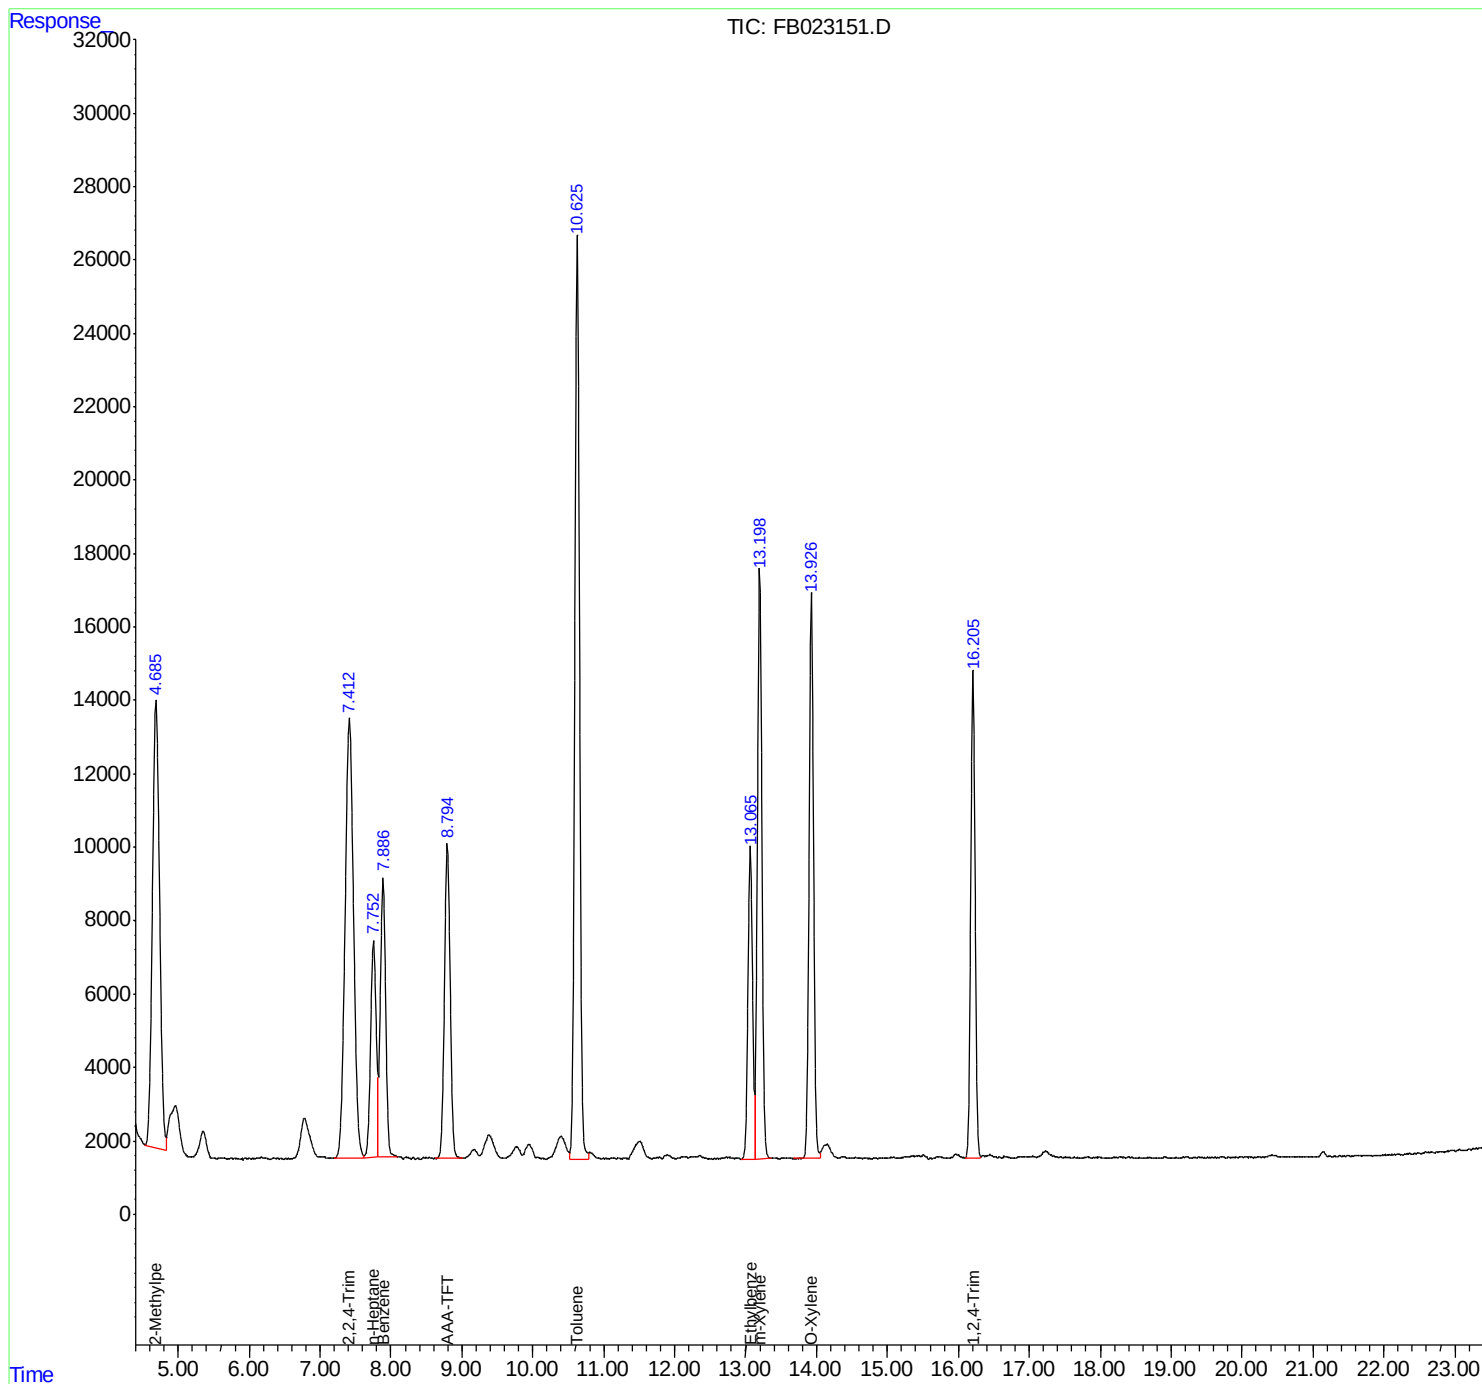

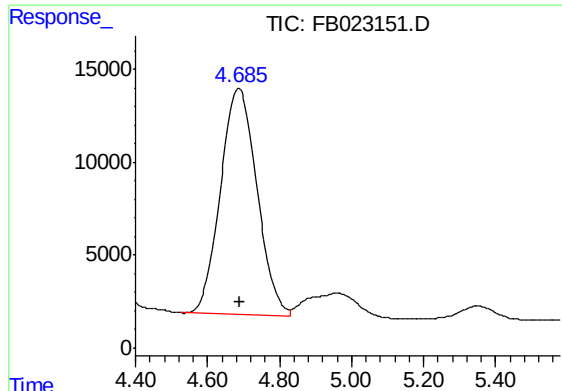


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.004 min
Response: 854702
Conc: 26.16 ng/ml

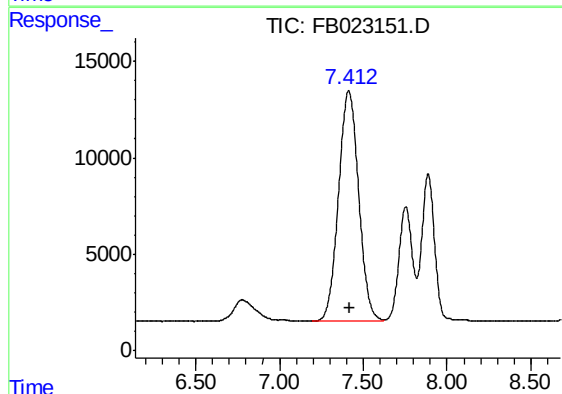


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.005 min
Response: 996539
Conc: 28.58 ng/ml

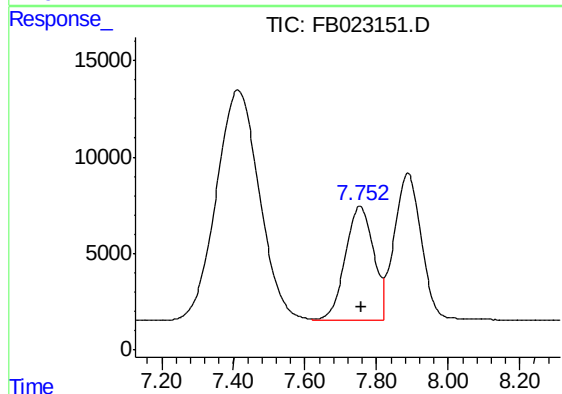


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 322878
Conc: 9.39 ng/ml

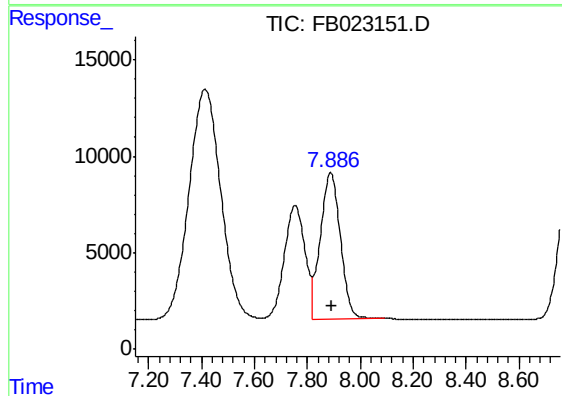


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.005 min
Response: 399390
Conc: 9.59 ng/ml

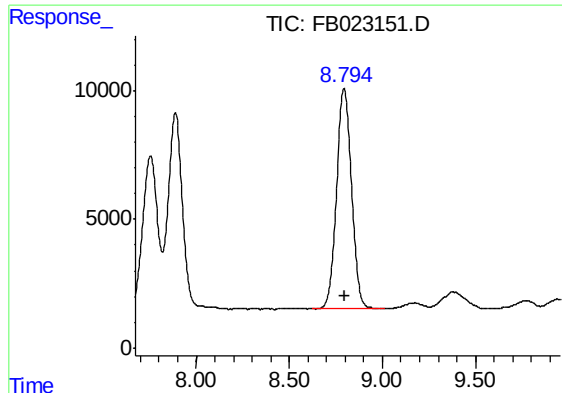


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 479653
Conc: 19.53 ng/ml

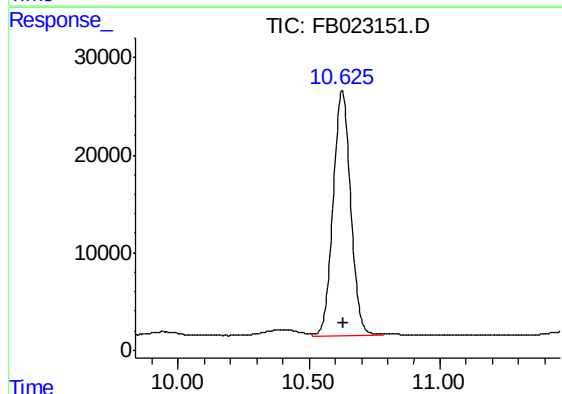


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.004 min
Response: 1174184
Conc: 29.15 ng/ml

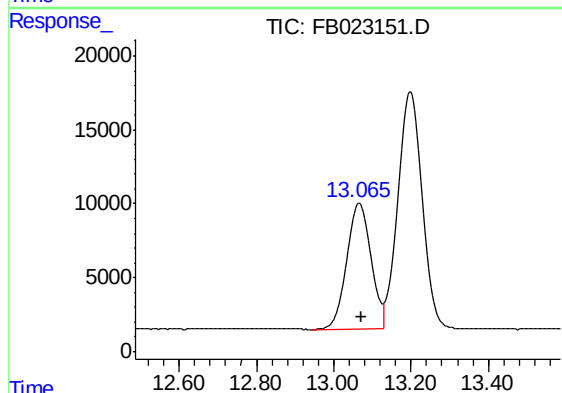


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.004 min
Response: 374313
Conc: 9.70 ng/ml

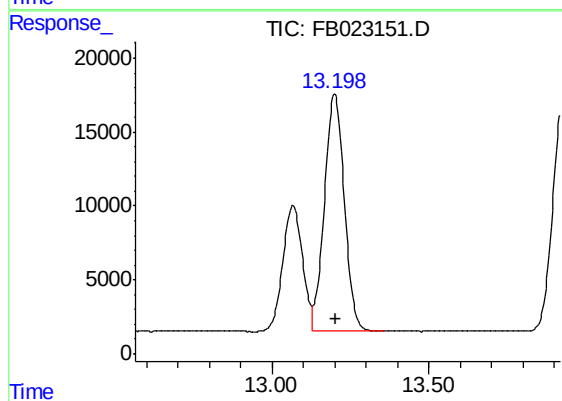


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.004 min
Response: 709007
Conc: 19.48 ng/ml

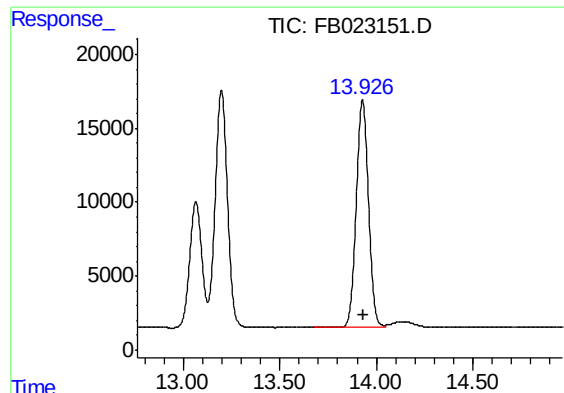

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 683347
Conc: 19.68 ng/ml

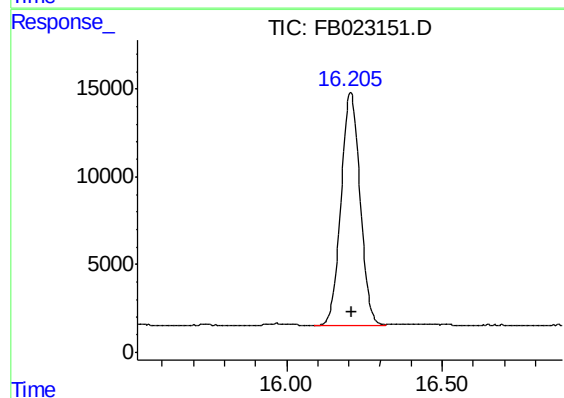

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.004 min
Response: 566448
Conc: 20.20 ng/ml