

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120619\
 Data File : FB023153.D
 Signal(s) : FID2B.CH
 Acq On : 6 Dec 2019 14:53
 Operator : DD/AJ
 Sample : K6113-02MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 06 22:30:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	462859	18.843 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	885104	27.085 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	922847	26.465 ng/ml
3) t n-Heptane	7.755	302031	8.784 ng/ml
4) t Benzene	7.889	412374	9.897 ng/ml
6) t Toluene	10.627	1189200	29.521 ng/ml
7) t Ethylbenzene	13.068	367726	9.530 ng/ml
8) t m-Xylene	13.201	692796	19.038 ng/ml
9) t O-Xylene	13.928	664240	19.131 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	538168	19.191 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120619\
Data File : FB023153.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2019 14:53
Operator : DD/AJ
Sample : K6113-02MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 06 22:30:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

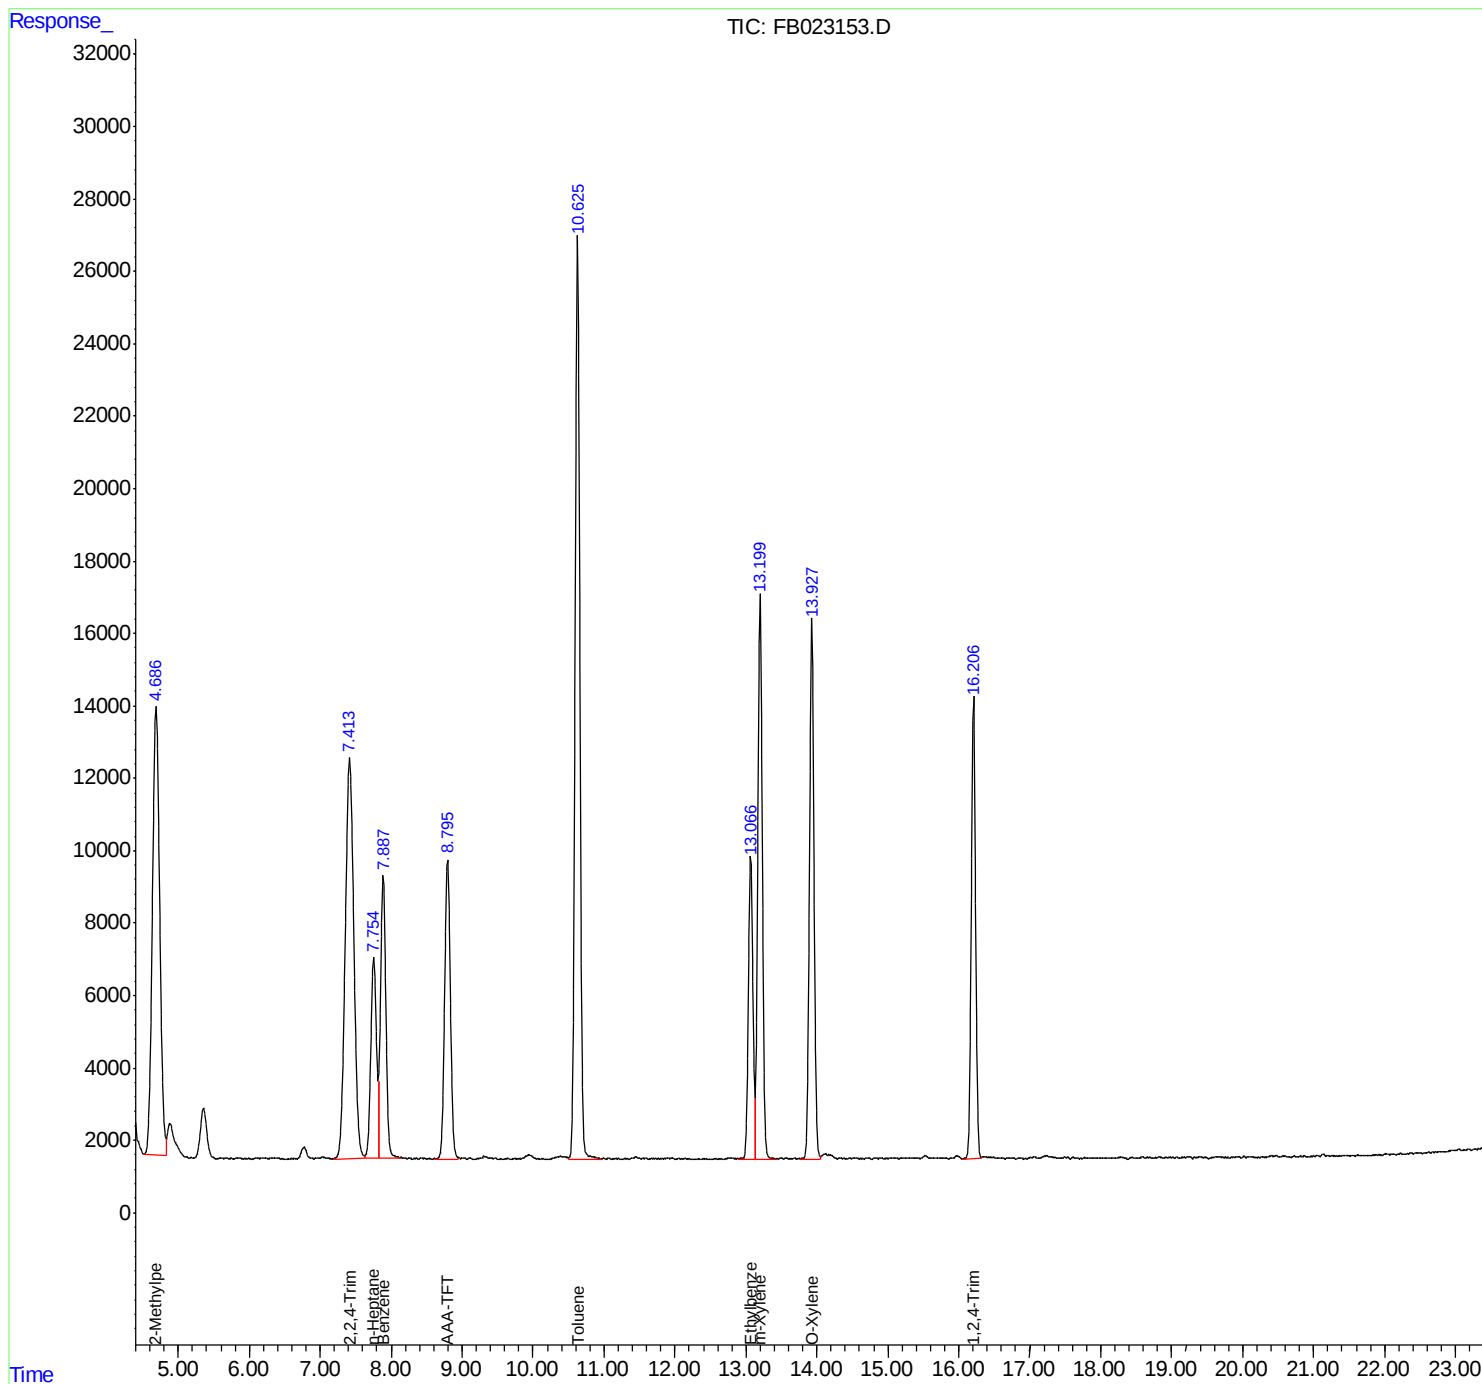

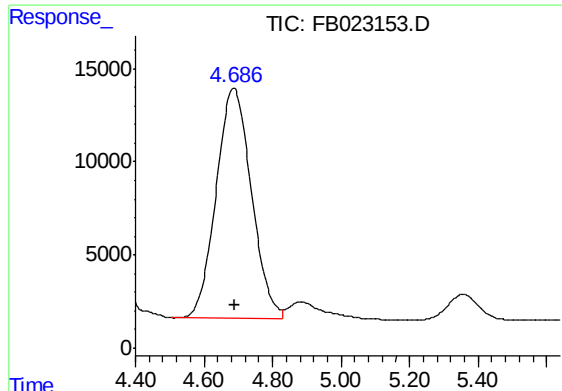


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.004 min
Response: 885104
Conc: 27.09 ng/ml

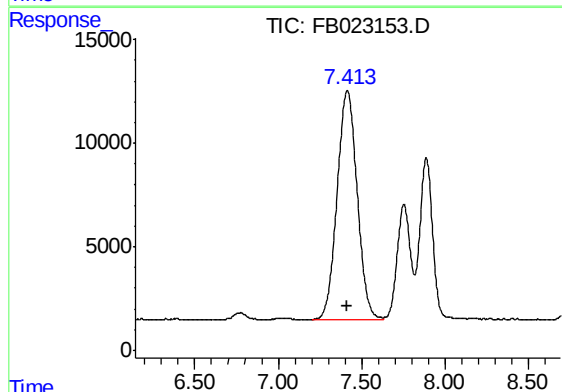


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.004 min
Response: 922847
Conc: 26.46 ng/ml

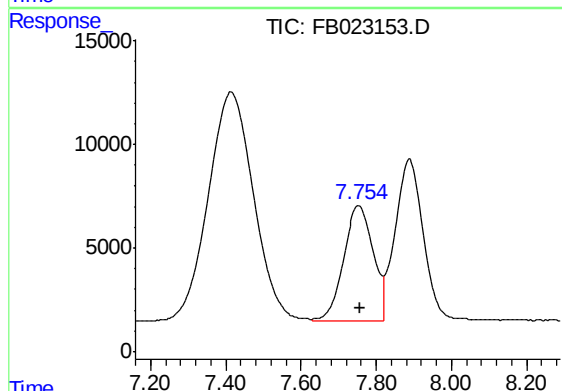


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 302031
Conc: 8.78 ng/ml

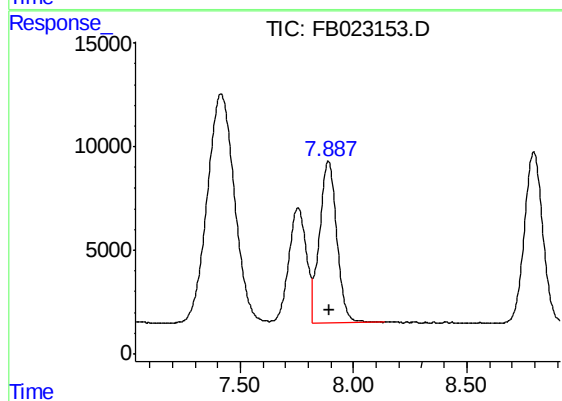


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 412374
Conc: 9.90 ng/ml

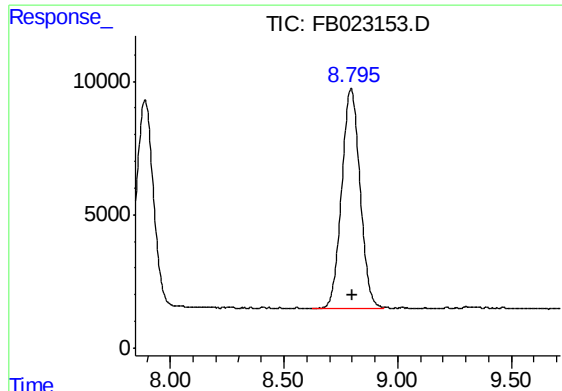


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 462859
Conc: 18.84 ng/ml

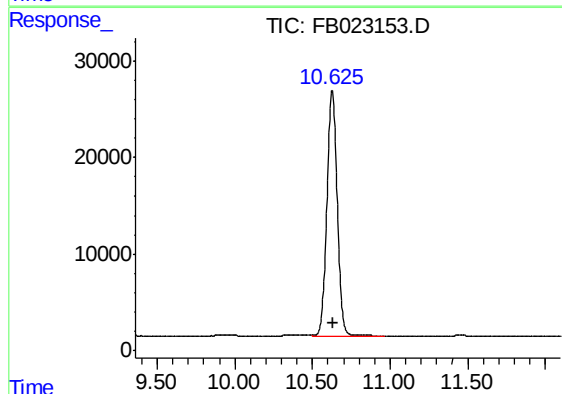


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.004 min
Response: 1189200
Conc: 29.52 ng/ml

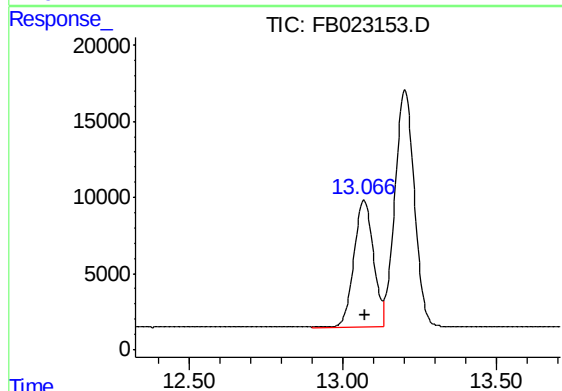


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 367726
Conc: 9.53 ng/ml

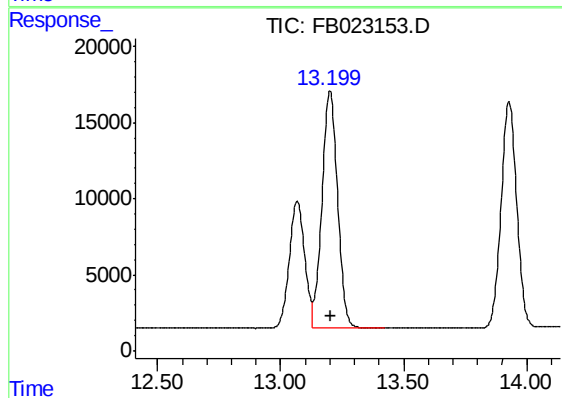


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.003 min
Response: 692796
Conc: 19.04 ng/ml

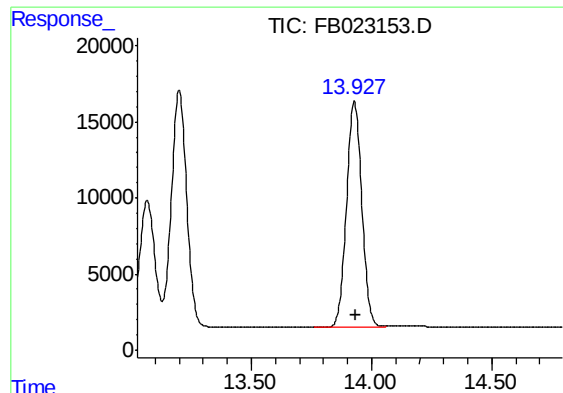

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.003 min
Response: 664240
Conc: 19.13 ng/ml

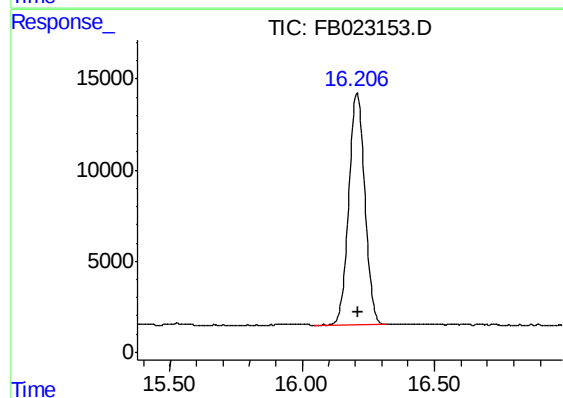

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.003 min
Response: 538168
Conc: 19.19 ng/ml