

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120619\
 Data File : FB023154.D
 Signal(s) : FID2B.CH
 Acq On : 6 Dec 2019 16:15
 Operator : DD/AJ
 Sample : K6113-02MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 06 22:31:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	446873	18.192 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	805800	24.659 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	839428	24.073 ng/ml
3) t n-Heptane	7.754	270622	7.871 ng/ml
4) t Benzene	7.888	371688	8.921 ng/ml
6) t Toluene	10.627	1093610	27.148 ng/ml
7) t Ethylbenzene	13.067	331714	8.596 ng/ml
8) t m-Xylene	13.200	622773	17.114 ng/ml
9) t O-Xylene	13.928	605969	17.453 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	489177	17.444 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120619\
Data File : FB023154.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2019 16:15
Operator : DD/AJ
Sample : K6113-02MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 06 22:31:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

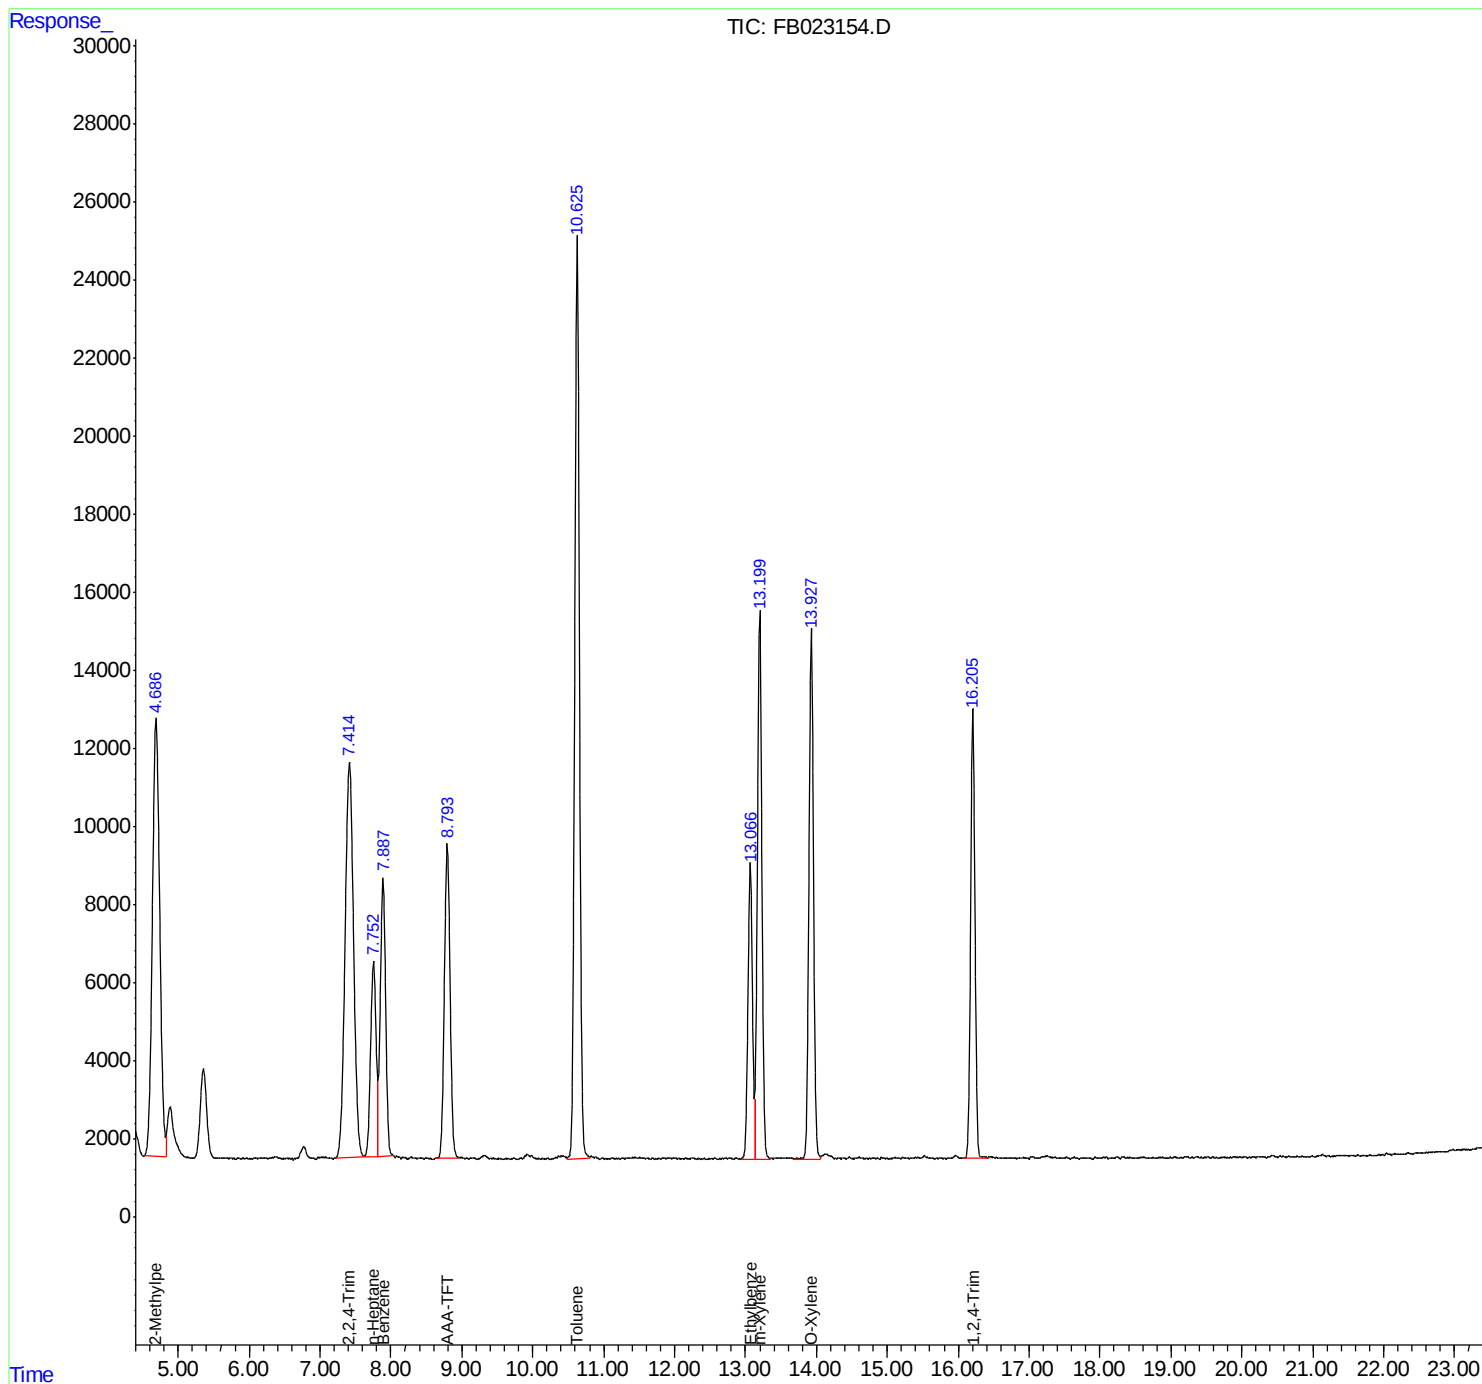

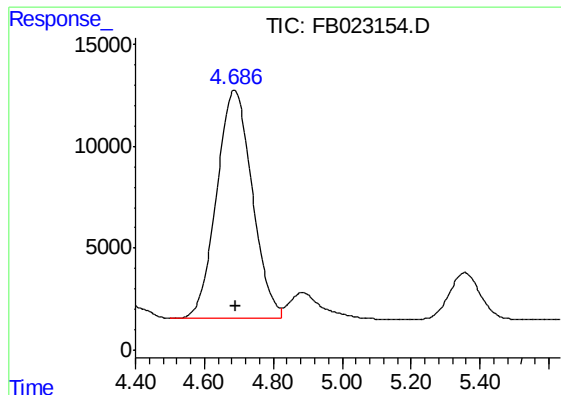


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.004 min
Response: 805800
Conc: 24.66 ng/ml

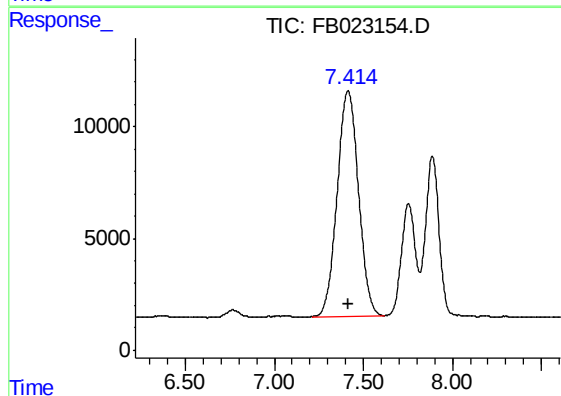


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 839428
Conc: 24.07 ng/ml

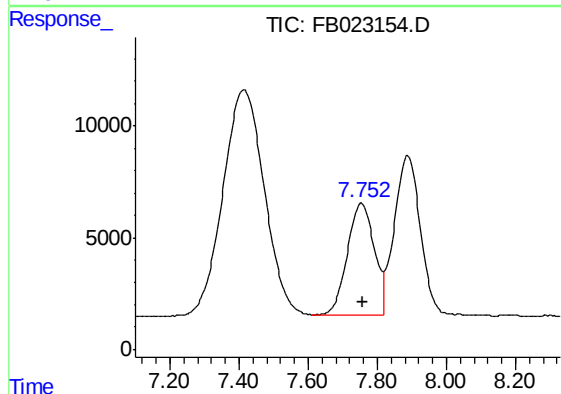


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 270622
Conc: 7.87 ng/ml

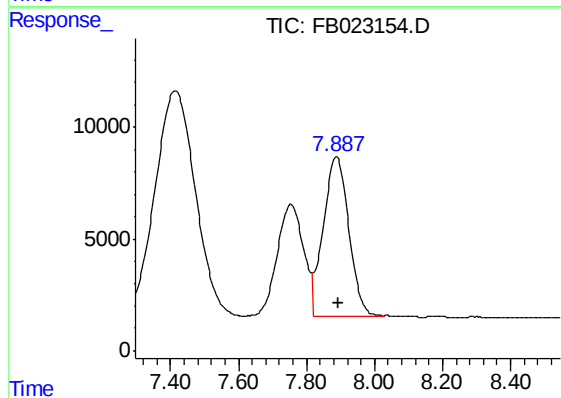


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.004 min
Response: 371688
Conc: 8.92 ng/ml

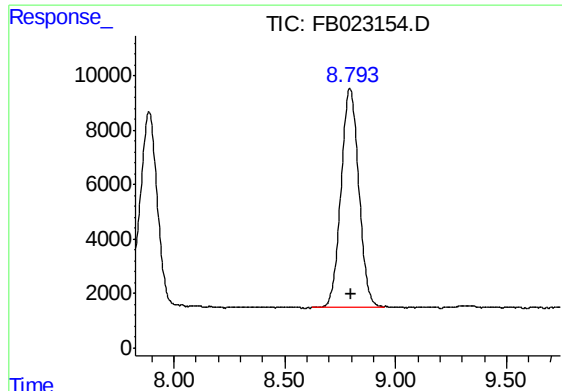


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.005 min
Response: 446873
Conc: 18.19 ng/ml

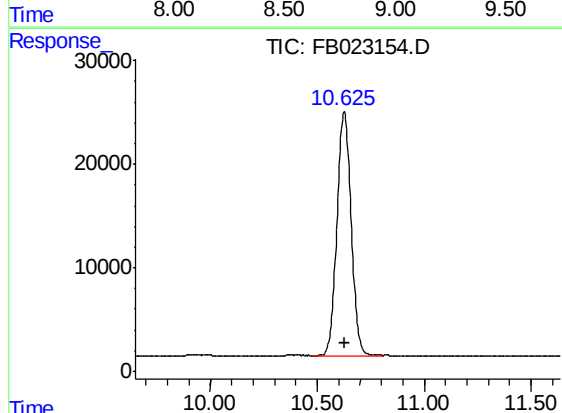


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.004 min
Response: 1093610
Conc: 27.15 ng/ml

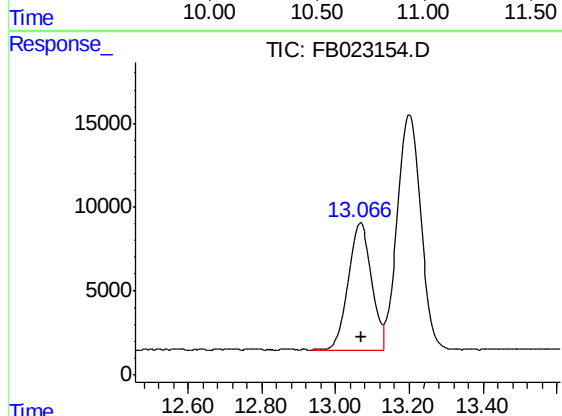


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.003 min
Response: 331714
Conc: 8.60 ng/ml

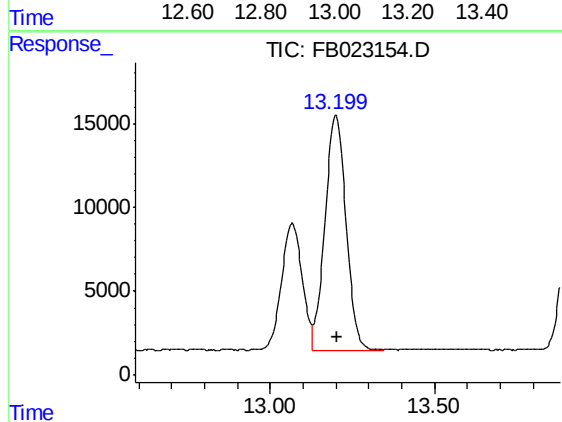


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 622773
Conc: 17.11 ng/ml

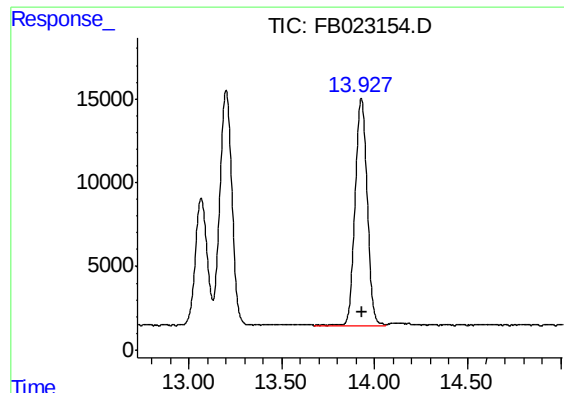

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.003 min
Response: 605969
Conc: 17.45 ng/ml

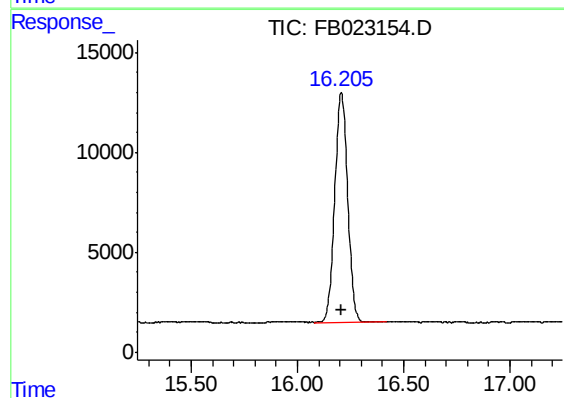

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 489177
Conc: 17.44 ng/ml