

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120623\
 Data File : FB030487.D
 Signal(s) : FID2B.CH
 Acq On : 6 Dec 2023 12:06
 Operator : YP/AJ
 Sample : BSF1206S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1206S1

Integration File: Calibration.e
 Quant Time: Dec 07 00:08:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112823.M
 Quant Title :
 QLast Update : Tue Nov 28 11:30:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	260419	18.261 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	522684	27.814 ng/ml
2) t 2,2,4-Trimethylpentane	7.407	497263	26.563 ng/ml
3) t n-Heptane	7.743	190675	8.817 ng/ml
4) t Benzene	7.880	222350	9.165 ng/ml
6) t Toluene	10.612	654675	26.446 ng/ml
7) t Ethylbenzene	13.048	202136	8.967 ng/ml
8) t m-Xylene	13.181	402148	17.511 ng/ml
9) t O-Xylene	13.908	389220	17.918 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	384598	17.548 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120623\
Data File : FB030487.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2023 12:06
Operator : YP/AJ
Sample : BSF1206S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1206S1

Integration File: Calibration.e
Quant Time: Dec 07 00:08:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112823.M
Quant Title :
QLast Update : Tue Nov 28 11:30:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

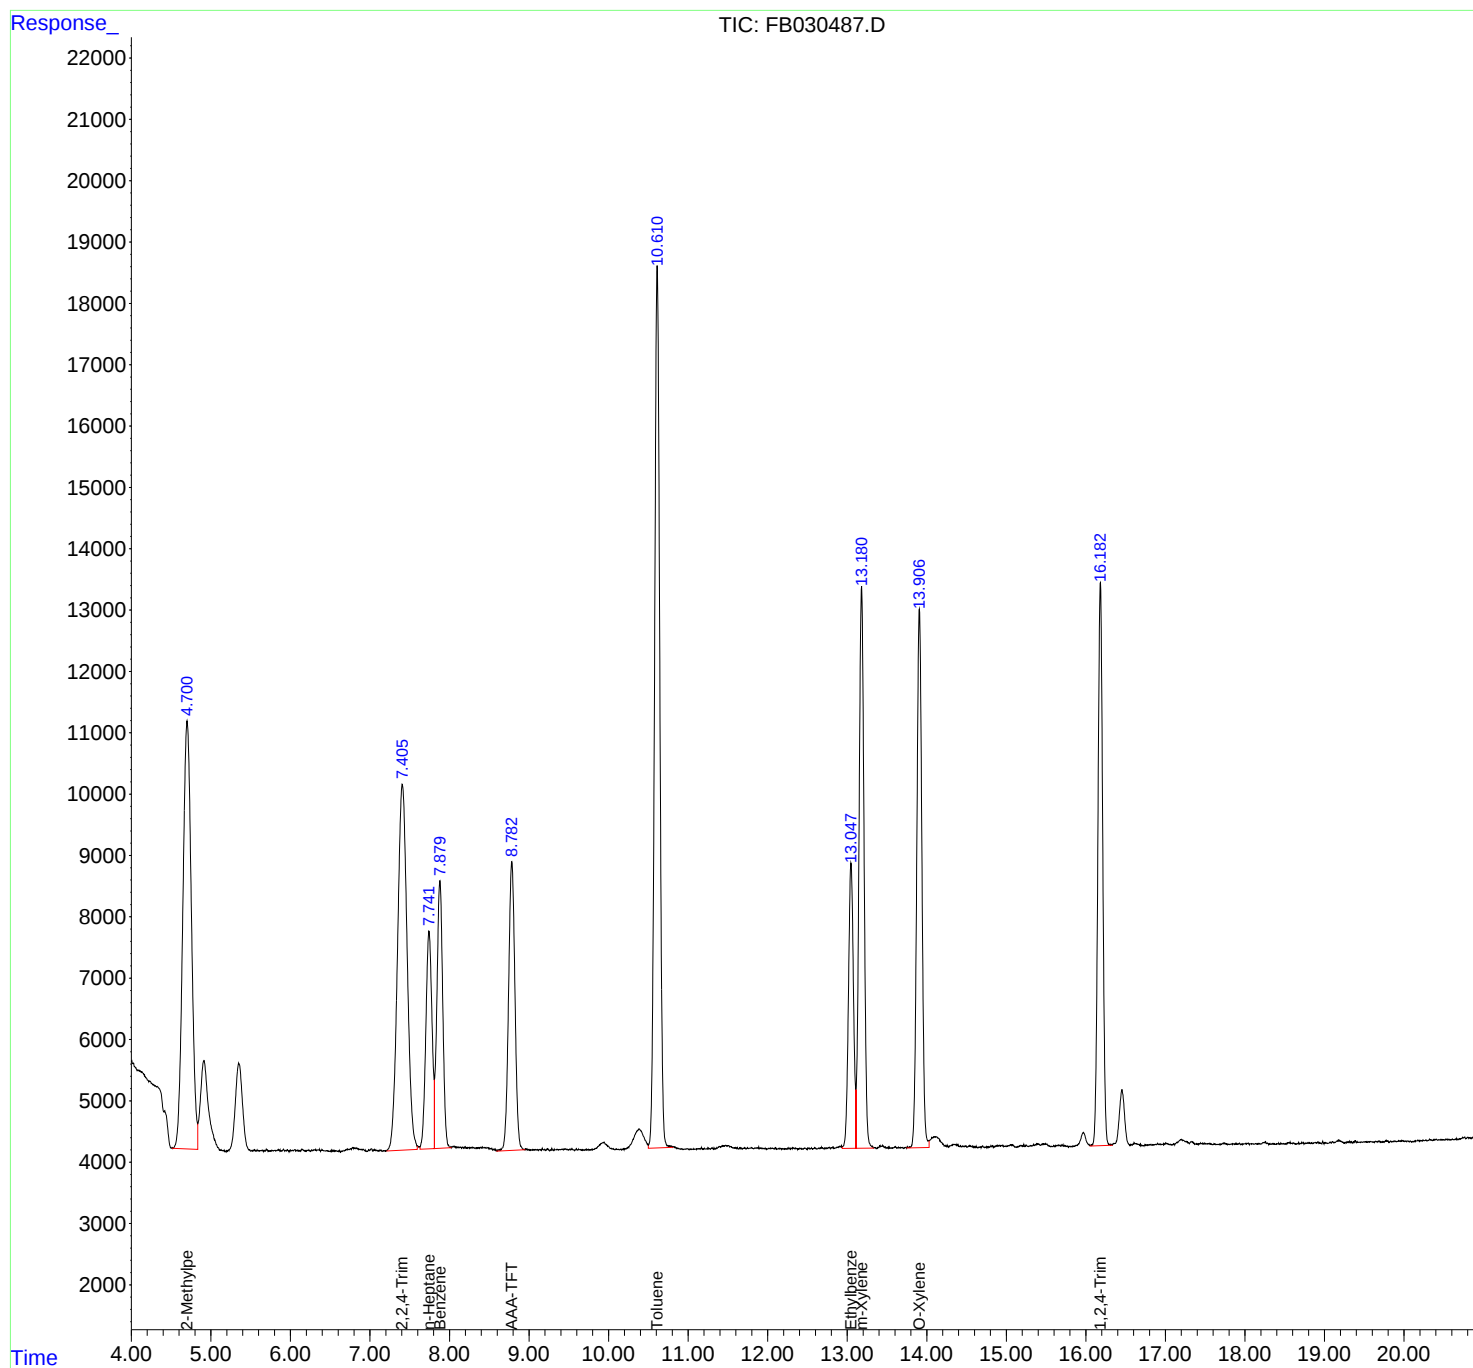


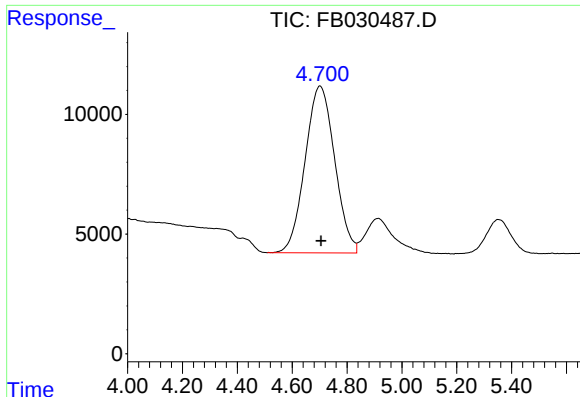

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.003 min
Response: 522684
Conc: 27.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1206S1

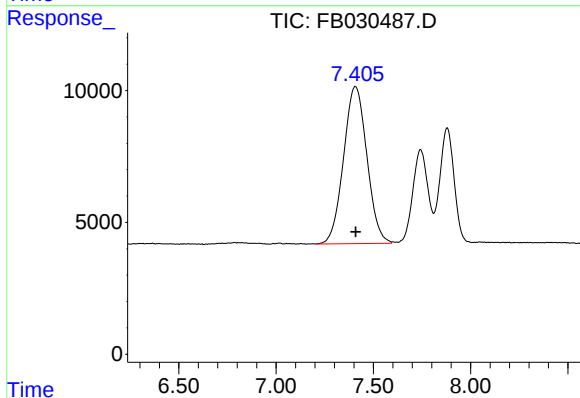


#2 2,2,4-Trimethylpentane

R.T.: 7.407 min
Delta R.T.: -0.002 min
Response: 497263
Conc: 26.56 ng/ml

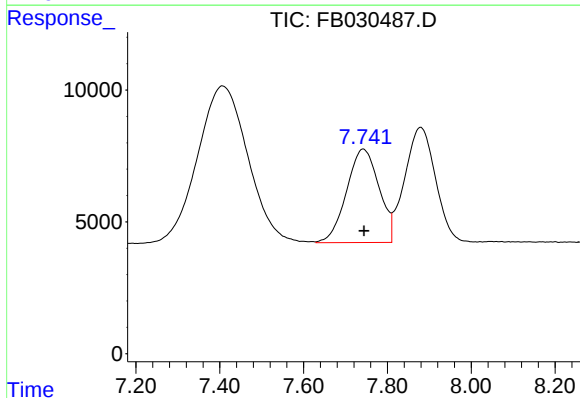


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.001 min
Response: 190675
Conc: 8.82 ng/ml

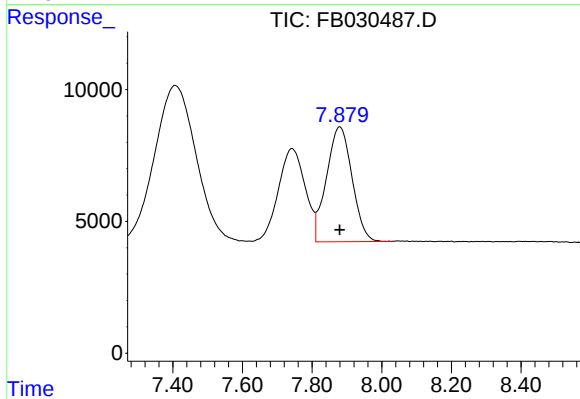

#4 Benzene


R.T.: 7.880 min
Delta R.T.: 0.000 min
Response: 222350
Conc: 9.17 ng/ml

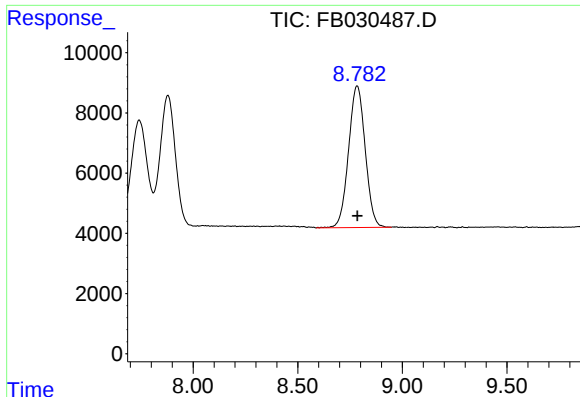

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: 0.000 min
Response: 260419
Conc: 18.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1206S1

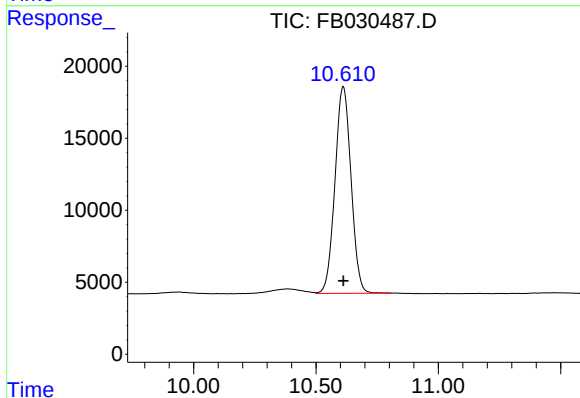


#6 Toluene

R.T.: 10.612 min
Delta R.T.: 0.000 min
Response: 654675
Conc: 26.45 ng/ml

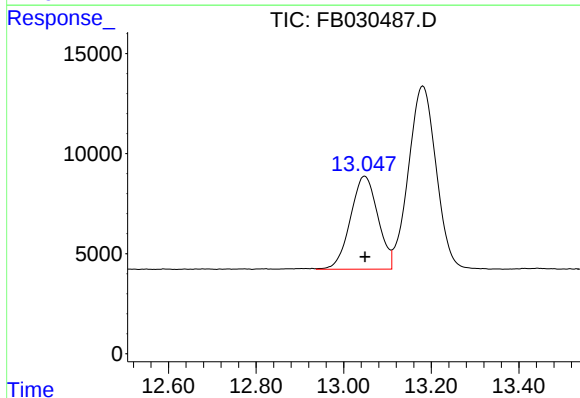


#7 Ethylbenzene

R.T.: 13.048 min
Delta R.T.: 0.000 min
Response: 202136
Conc: 8.97 ng/ml

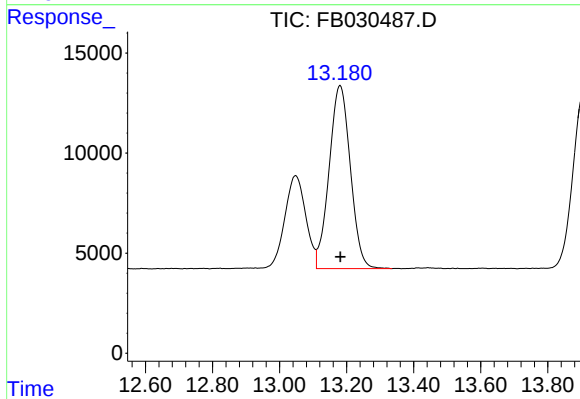

#8 m-Xylene


R.T.: 13.181 min
Delta R.T.: 0.000 min
Response: 402148
Conc: 17.51 ng/ml

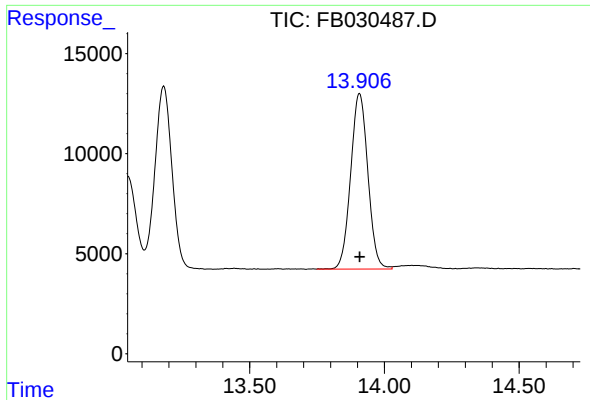

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: 0.000 min
Response: 389220
Conc: 17.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1206S1

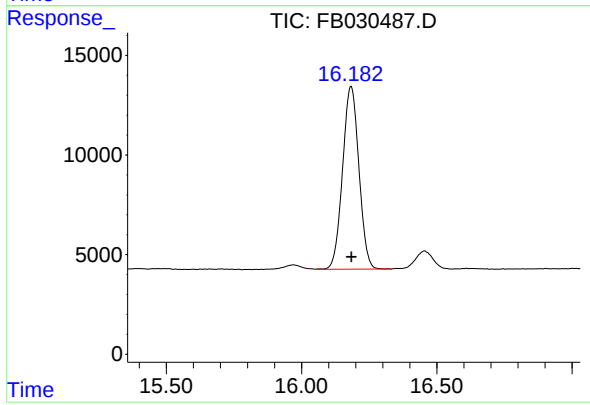

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.001 min
Response: 384598
Conc: 17.55 ng/ml