

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120623\
Data File : FB030499.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2023 20:28
Operator : YP/AJ
Sample : 05628-08 50X
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-03-COMP

Integration File: Calibration.e
Quant Time: Dec 07 00:09:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112823.M
Quant Title :
QLast Update : Tue Nov 28 11:30:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.783	309875	21.729 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120623\
Data File : FB030499.D
Signal(s) : FID2B.CH
Acq On : 6 Dec 2023 20:28
Operator : YP/AJ
Sample : 05628-08 50X
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-03-COMP

Integration File: Calibration.e
Quant Time: Dec 07 00:09:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112823.M
Quant Title :
QLast Update : Tue Nov 28 11:30:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

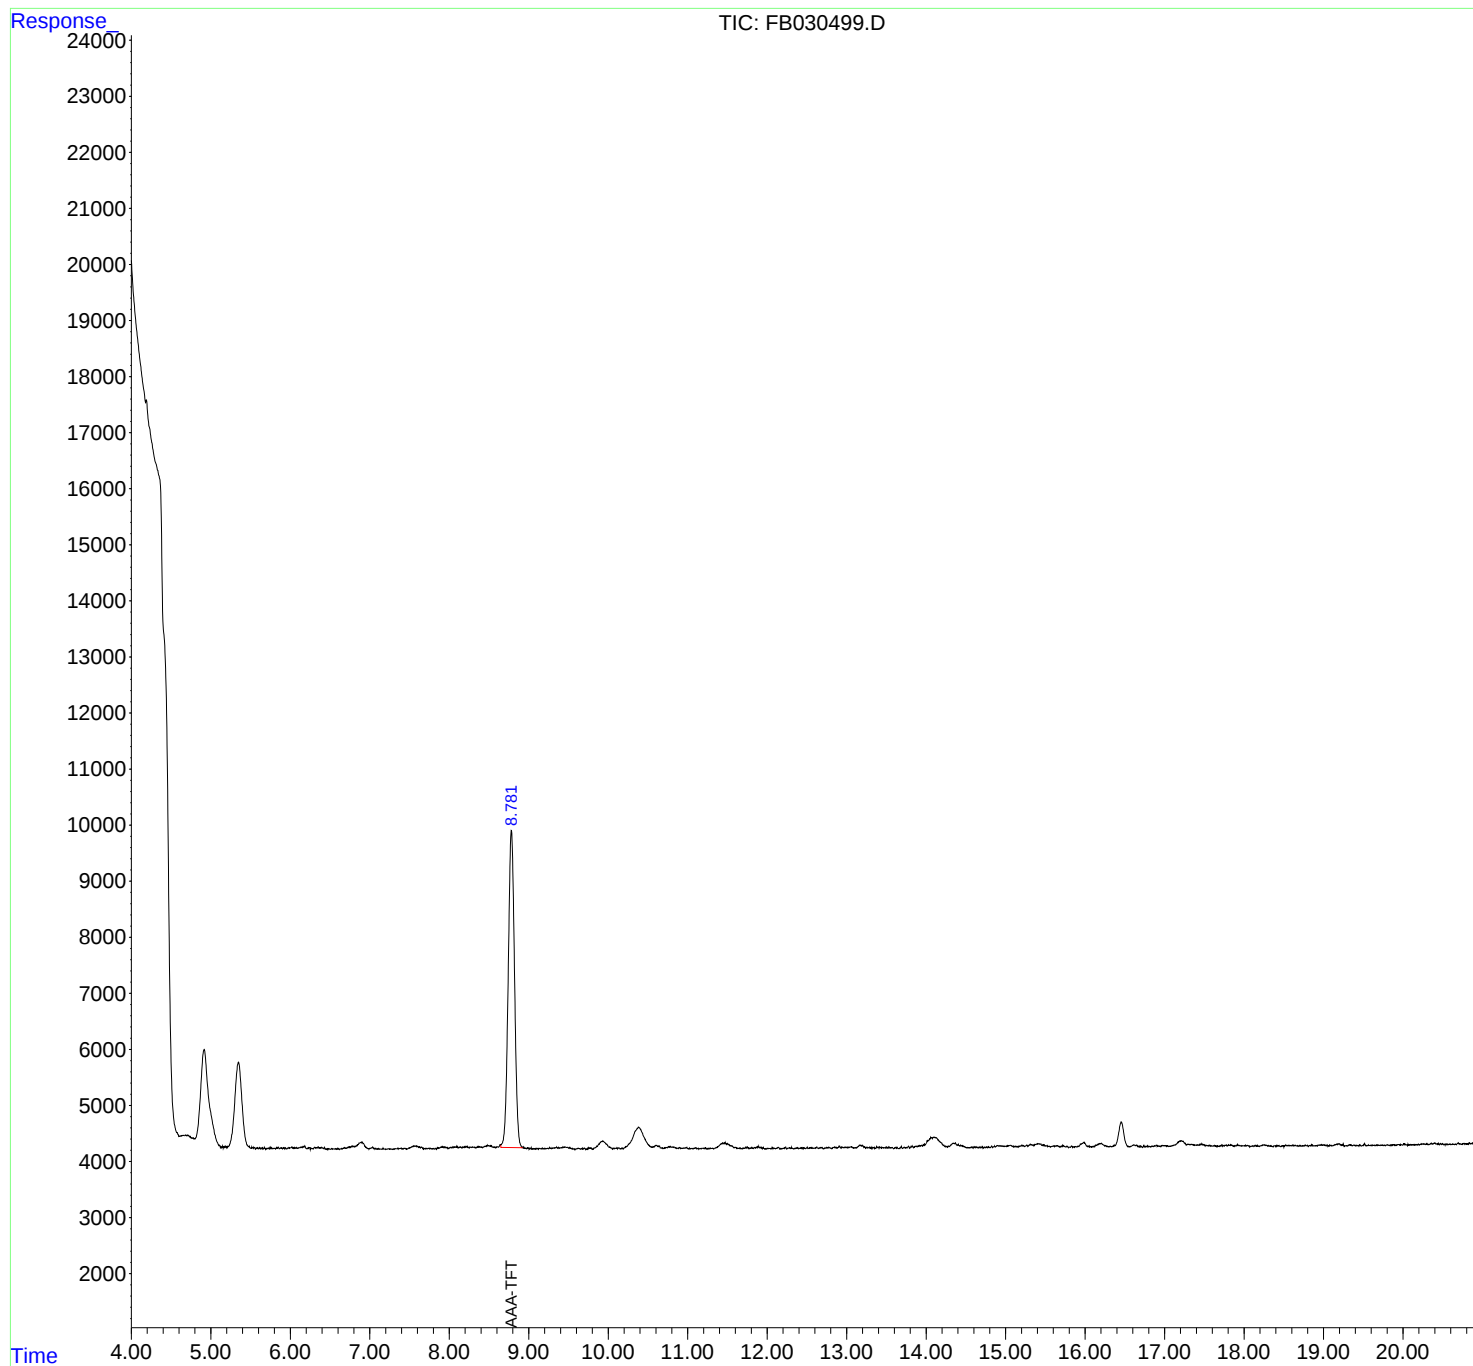

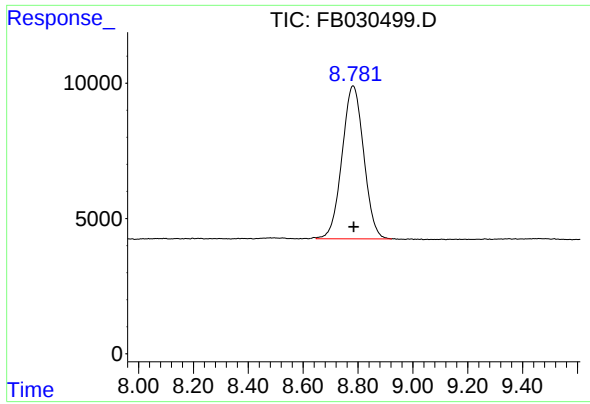

#5 AAA-TFT

R.T.: 8.783 min
Delta R.T.: -0.002 min
Response: 309875
Conc: 21.73 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-03-COMP