

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120821\
 Data File : FB026372.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2021 13:34
 Operator : AJ/MA
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 GRO STD

Integration File: Calibration.e
 Quant Time: Dec 08 13:13:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 13:12:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	205001	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	523196	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	601453	30.000 ng/ml
3) t n-Heptane	7.751	189251	10.000 ng/ml
4) t Benzene	7.887	219088	10.000 ng/ml
6) t Toluene	10.619	623205	30.000 ng/ml
7) t Ethylbenzene	13.055	192952	10.000 ng/ml
8) t m-Xylene	13.189	386058	20.000 ng/ml
9) t O-Xylene	13.916	376699	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	386059	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120821\
Data File : FB026372.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2021 13:34
Operator : AJ/MA
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 GRO STD

Integration File: Calibration.e
Quant Time: Dec 08 13:13:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 13:12:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

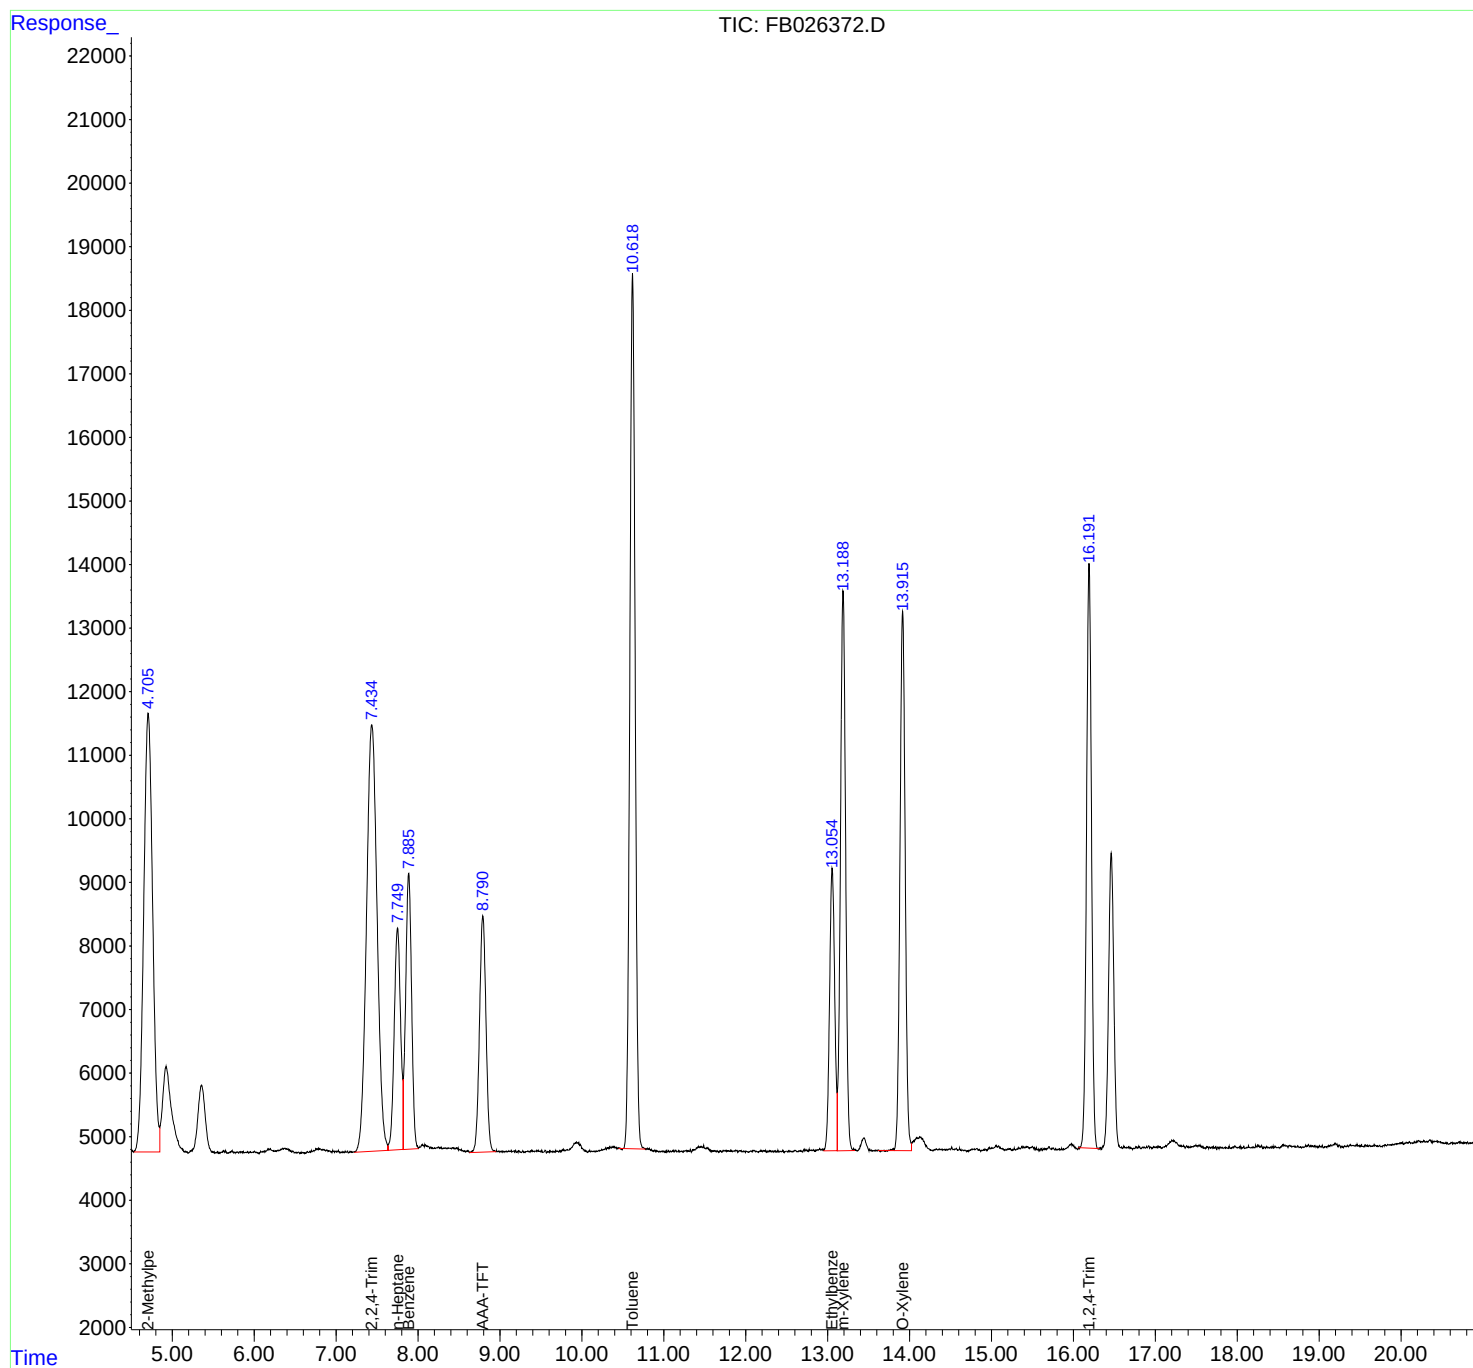


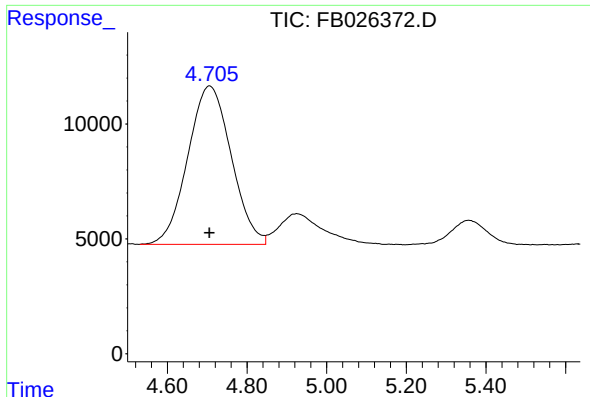

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 523196
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

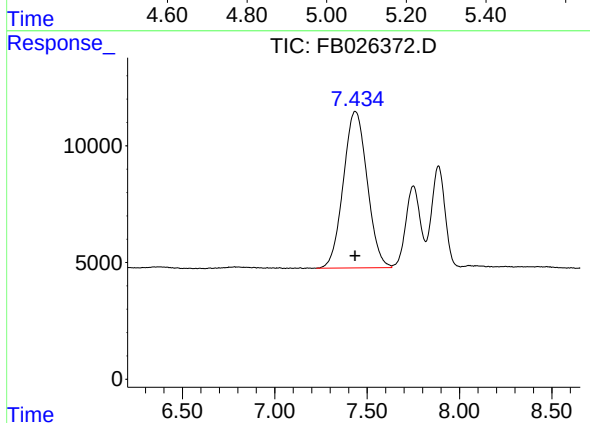


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.000 min
Response: 601453
Conc: 30.00 ng/ml

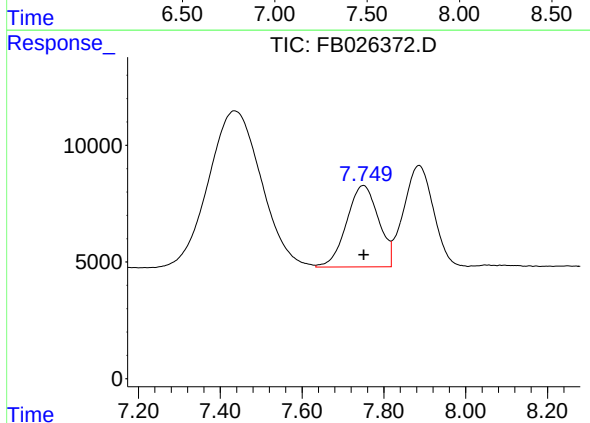


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 189251
Conc: 10.00 ng/ml

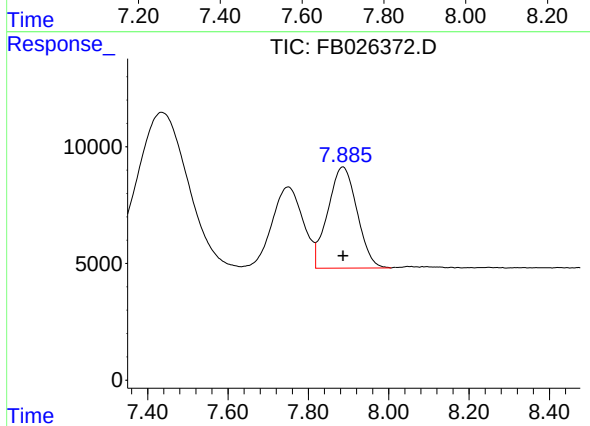

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 219088
Conc: 10.00 ng/ml

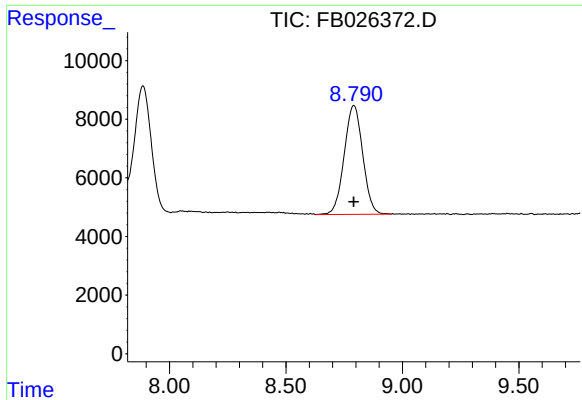

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 205001
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

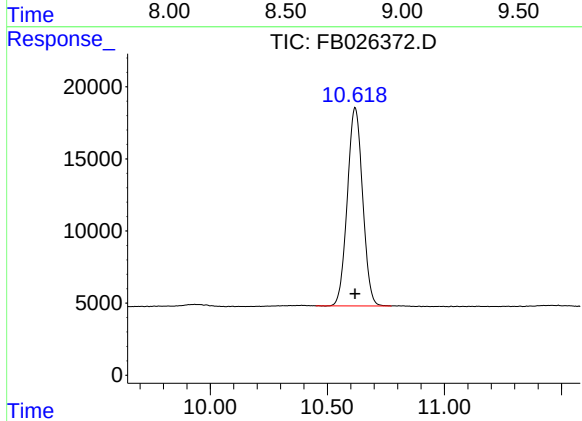


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 623205
Conc: 30.00 ng/ml

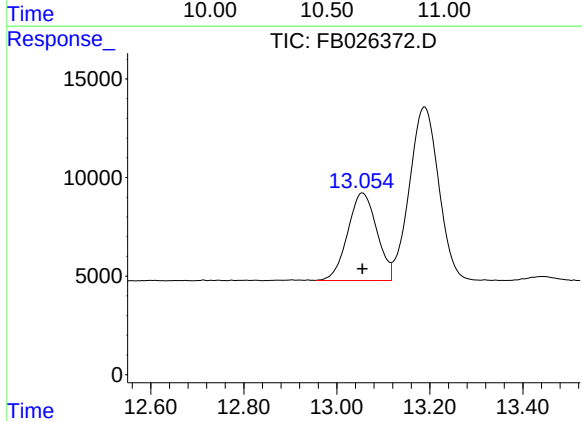


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 192952
Conc: 10.00 ng/ml

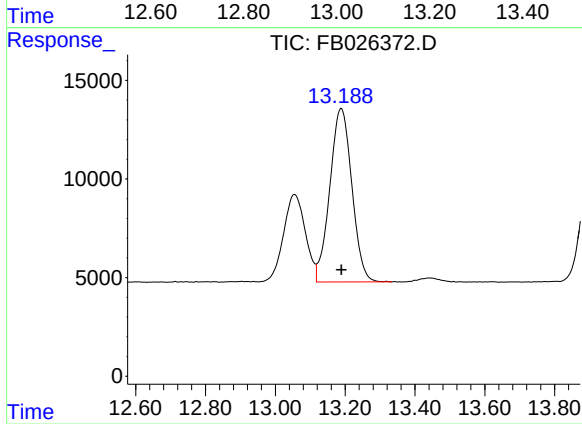

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 386058
Conc: 20.00 ng/ml

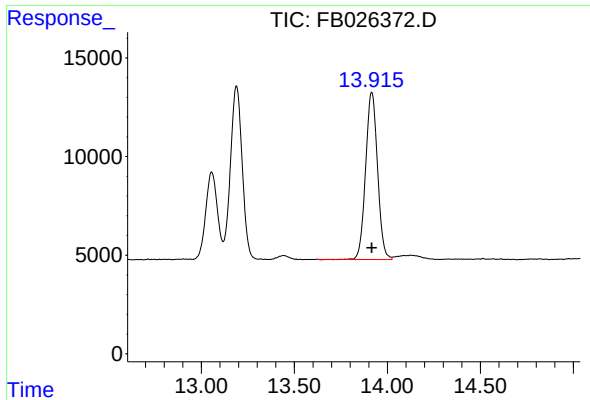

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 376699
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

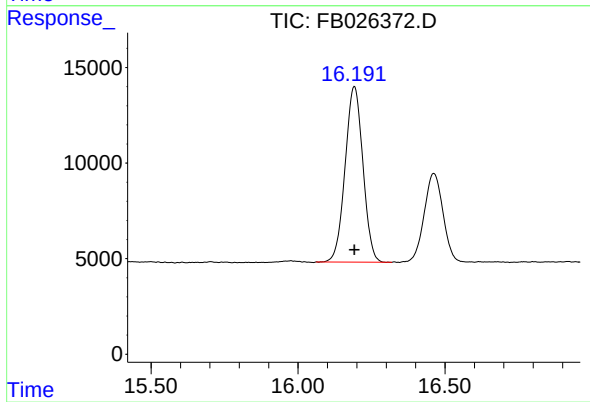

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 386059
Conc: 20.00 ng/ml