

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120919\
Data File : FB023162.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2019 11:27
Operator : DD/AJ
Sample : VBF1209S1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 10 00:49:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.796	455097	18.527 ng/ml
Target Compounds				
6) t	Toluene	10.629	6013	0.149 ng/ml
8) t	m-Xylene	13.200	2899	0.080 ng/ml
9) t	O-Xylene	13.912	1176	0.034 ng/ml
10) t	1,2,4-Trimethylbenzene	16.218	3113	0.111 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120919\
Data File : FB023162.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2019 11:27
Operator : DD/AJ
Sample : VBF1209S1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 10 00:49:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

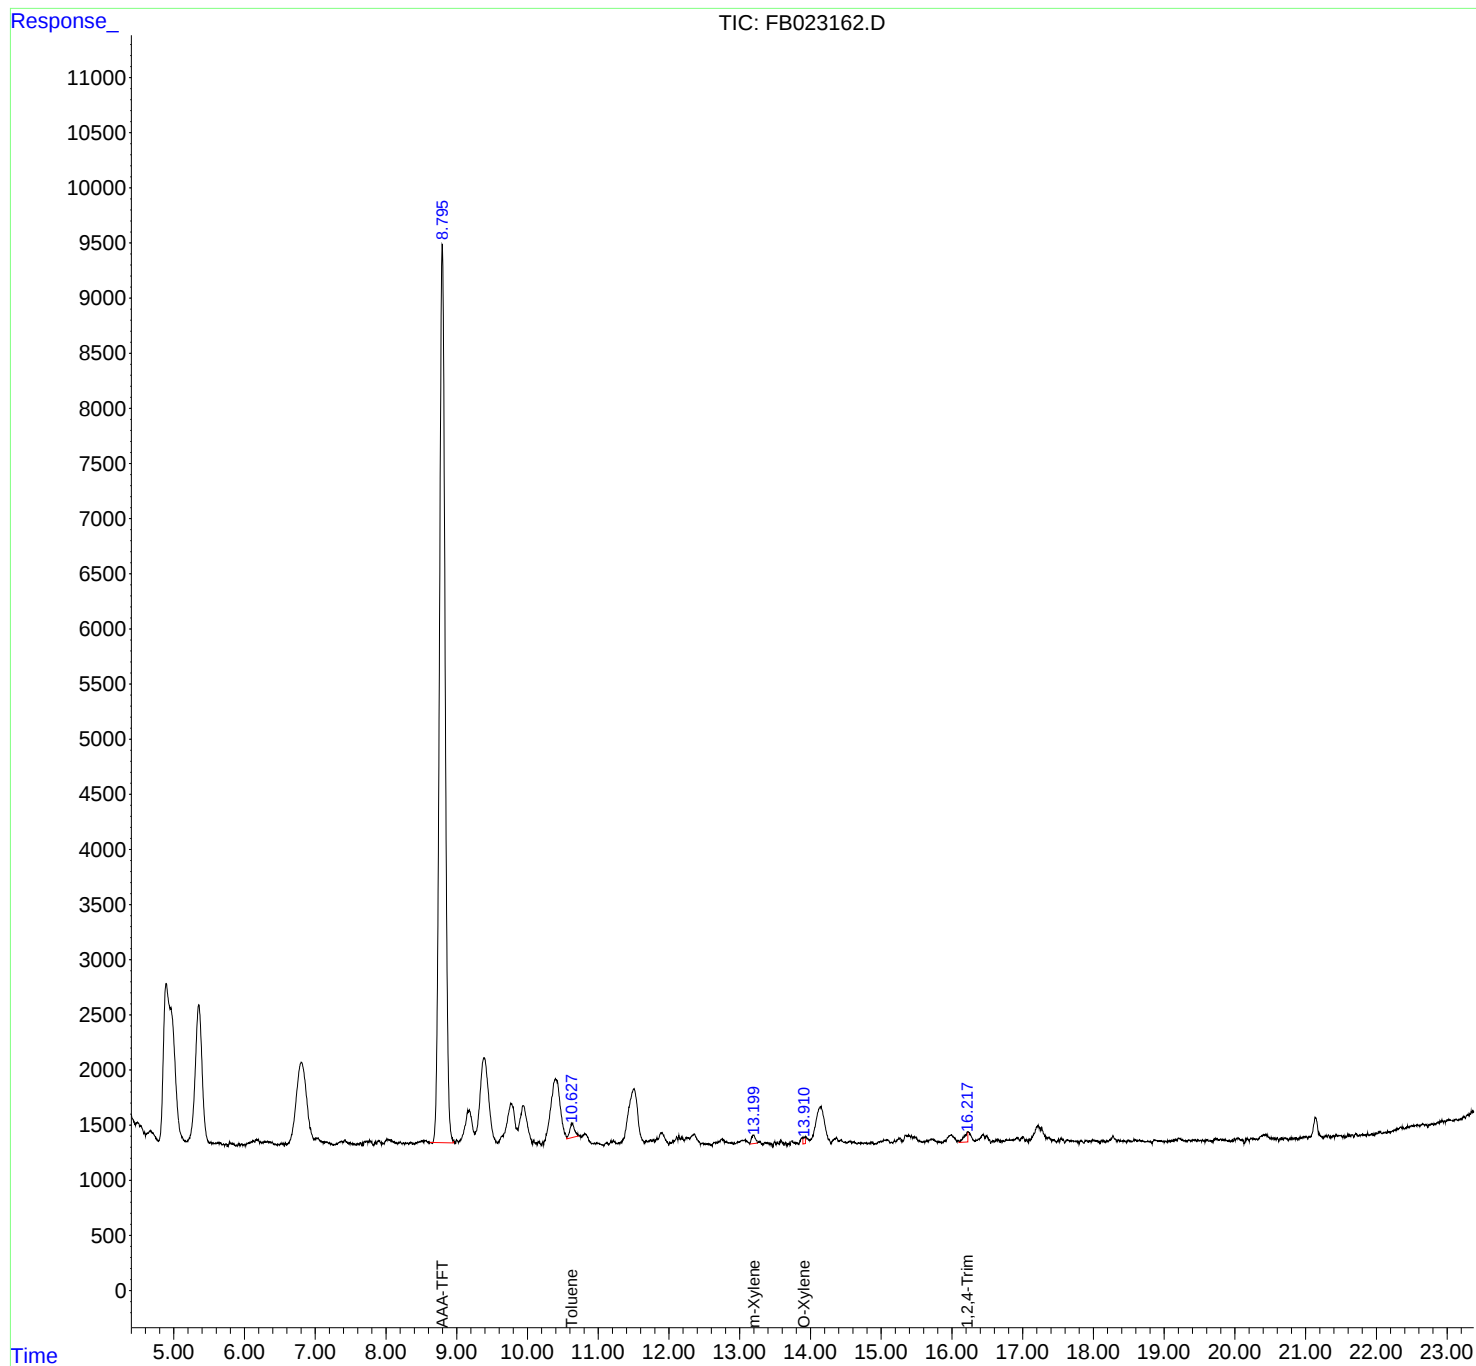


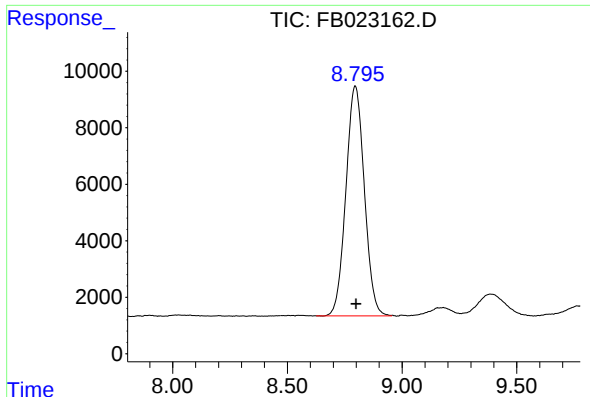

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 455097
Conc: 18.53 ng/ml

Instrument :
FID_B
ClientSampleId :

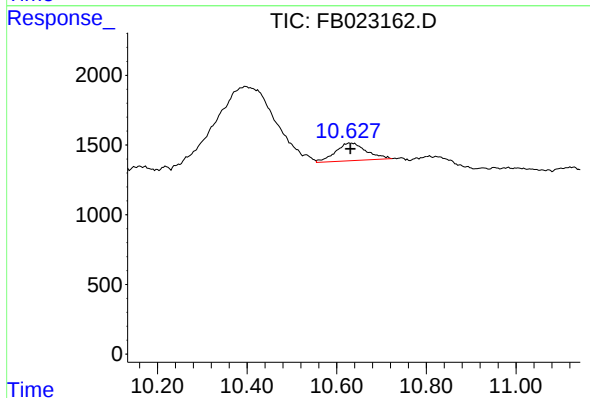


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.002 min
Response: 6013
Conc: 0.15 ng/ml

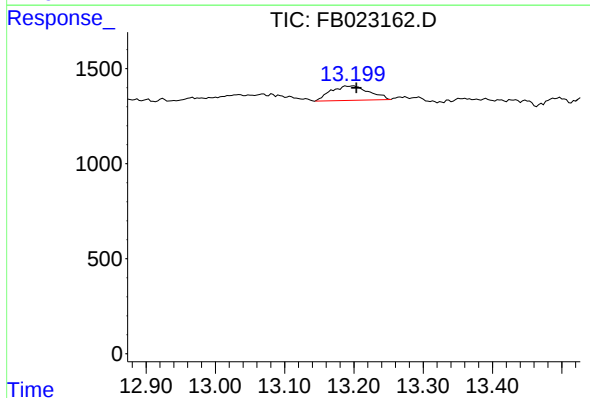


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 2899
Conc: 0.08 ng/ml

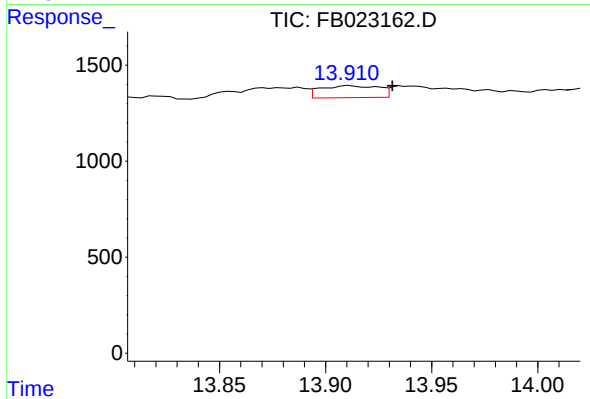

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.020 min
Response: 1176
Conc: 0.03 ng/ml

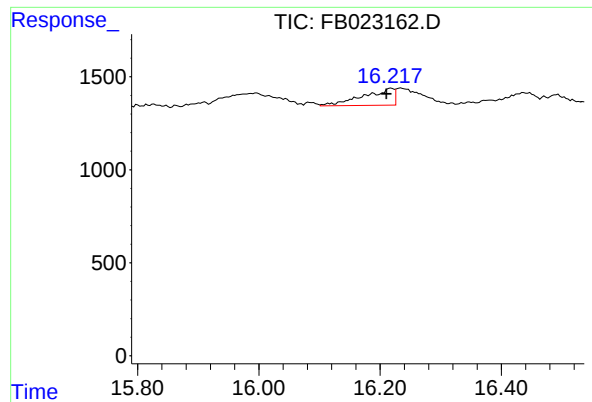

#10 1,2,4-Trimethylbenzene

R.T.: 16.218 min
Delta R.T.: 0.008 min
Response: 3113
Conc: 0.11 ng/ml

Instrument :
FID_B
ClientSampleId :