

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120919\
 Data File : FB023167.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2019 15:16
 Operator : DD/AJ
 Sample : K6111-02MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 10 00:49:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	422302	17.192 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	715749	21.903 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	738735	21.185 ng/ml
3) t n-Heptane	7.755	232503	6.762 ng/ml
4) t Benzene	7.889	341699	8.201 ng/ml
6) t Toluene	10.627	980358	24.336 ng/ml
7) t Ethylbenzene	13.067	313499	8.124 ng/ml
8) t m-Xylene	13.201	545650	14.995 ng/ml
9) t O-Xylene	13.929	551798	15.892 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	424485	15.137 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120919\
Data File : FB023167.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2019 15:16
Operator : DD/AJ
Sample : K6111-02MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 10 00:49:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

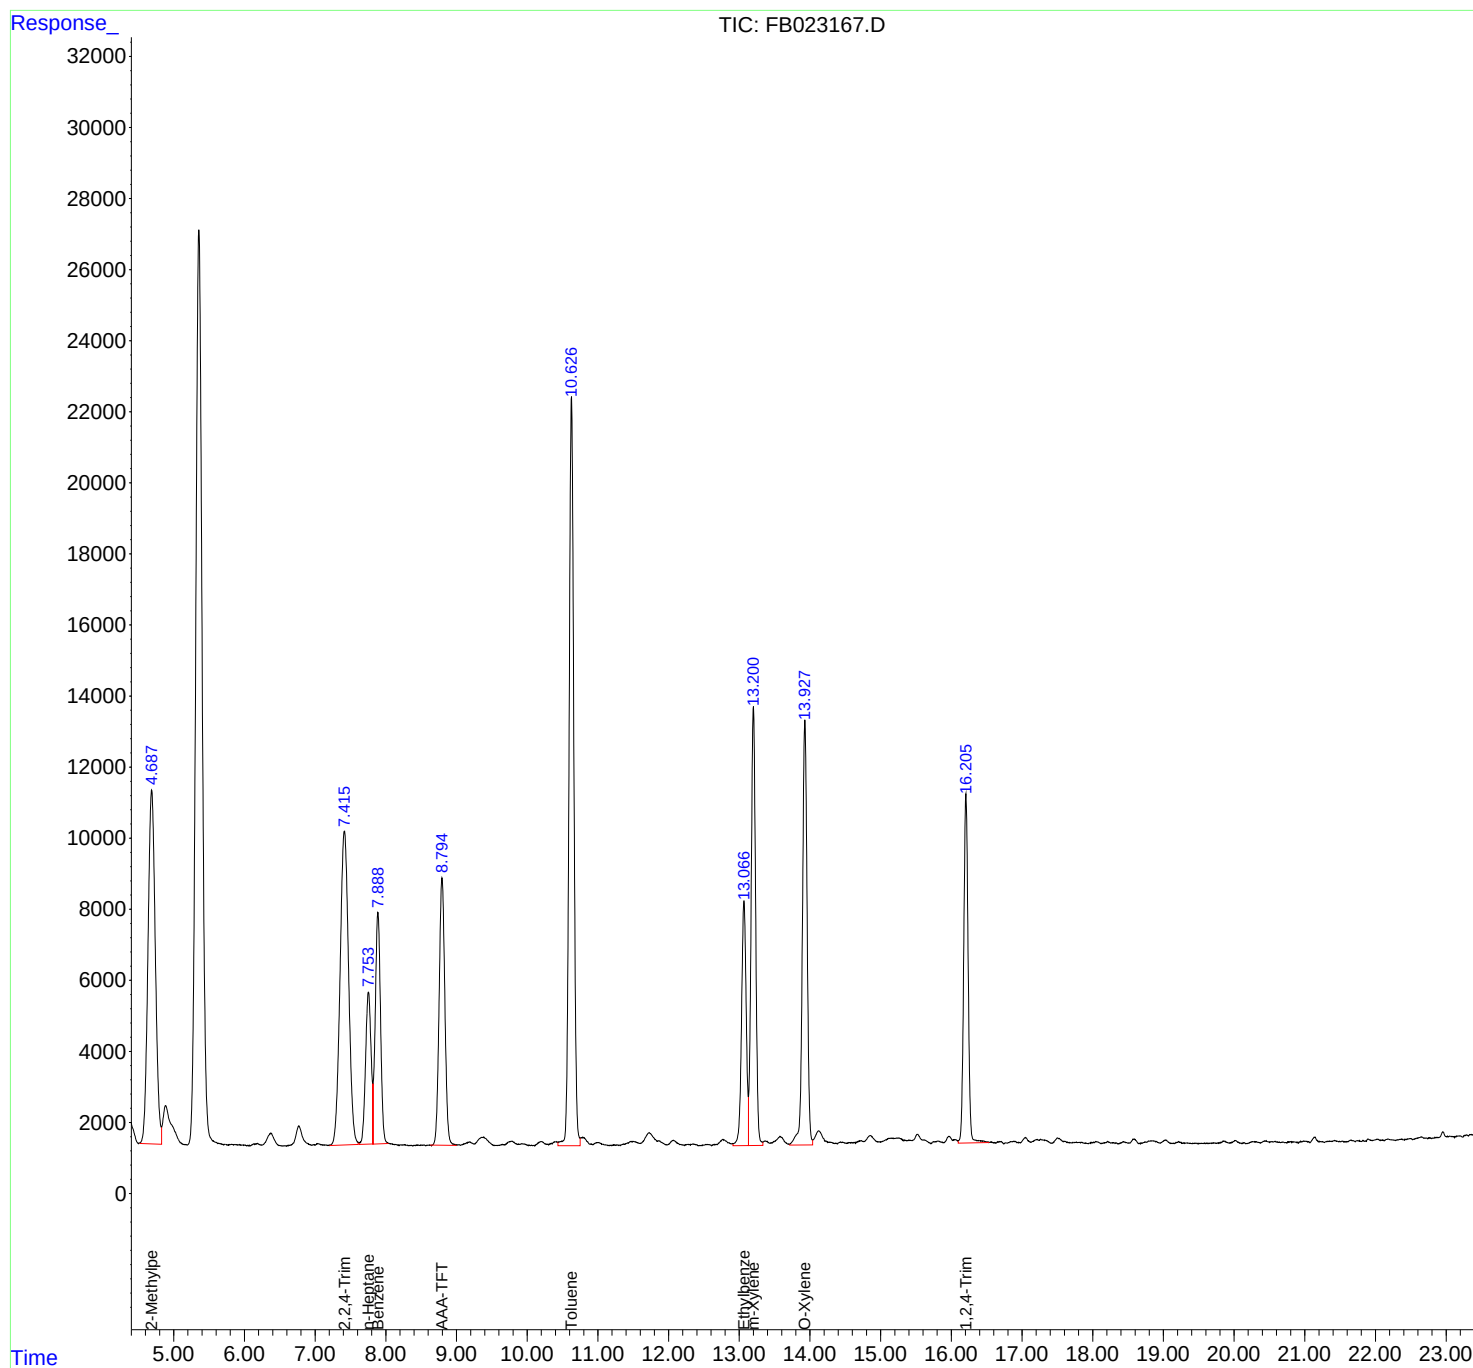


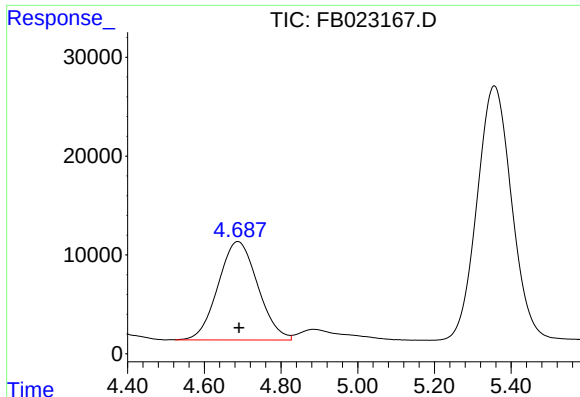

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 715749
Conc: 21.90 ng/ml

Instrument :
FID_B
ClientSampleId :

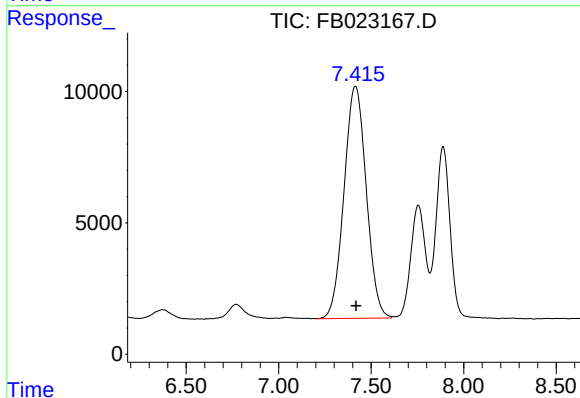


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 738735
Conc: 21.19 ng/ml

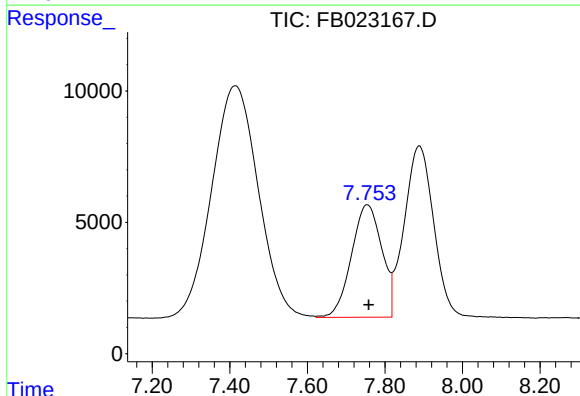


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 232503
Conc: 6.76 ng/ml

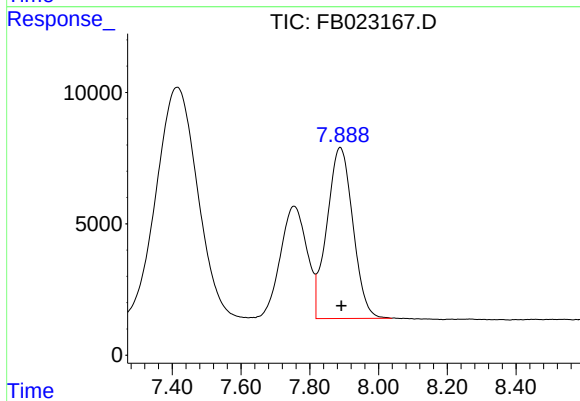

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.003 min
Response: 341699
Conc: 8.20 ng/ml

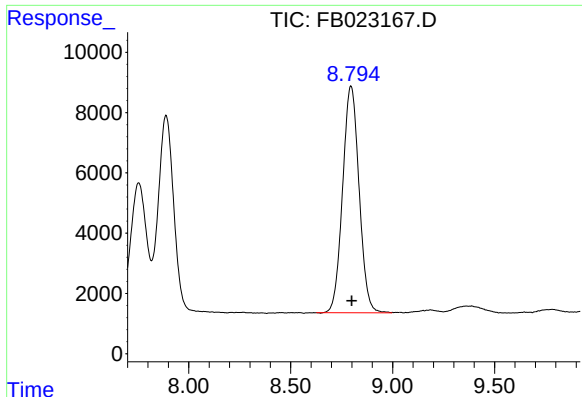

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 422302
Conc: 17.19 ng/ml

Instrument :
FID_B
ClientSampleId :

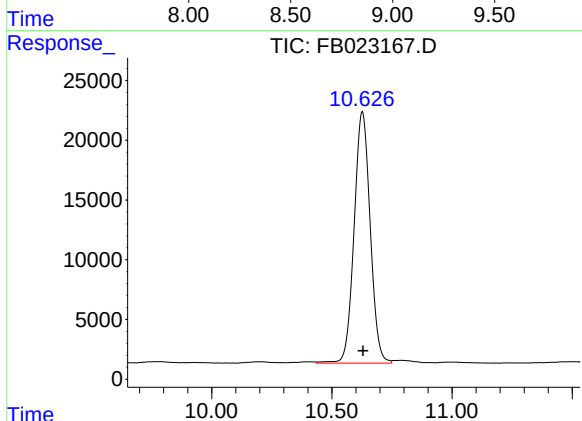


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.003 min
Response: 980358
Conc: 24.34 ng/ml

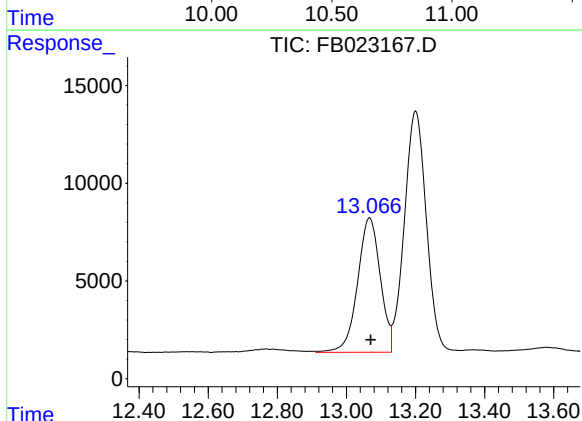


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.003 min
Response: 313499
Conc: 8.12 ng/ml

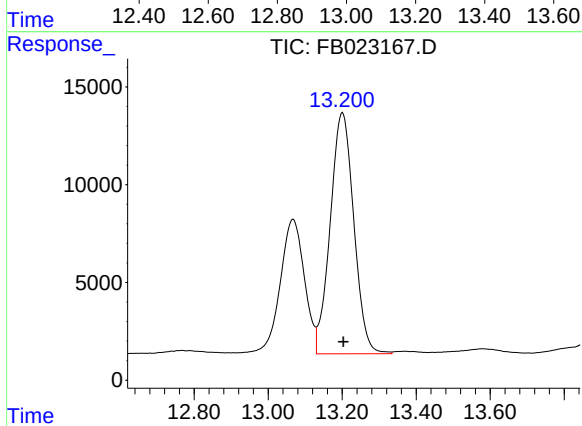

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.003 min
Response: 545650
Conc: 14.99 ng/ml

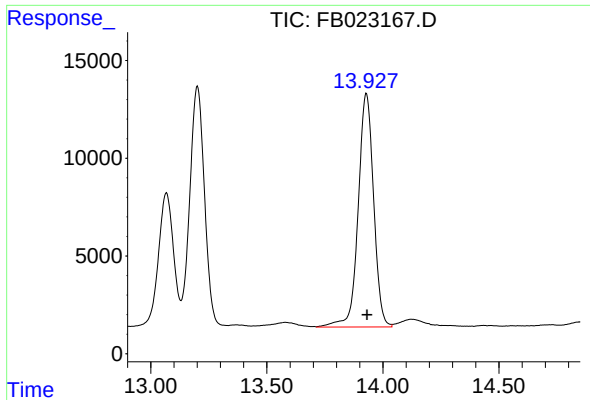

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.003 min
Response: 551798
Conc: 15.89 ng/ml

Instrument :
FID_B
ClientSampleId :

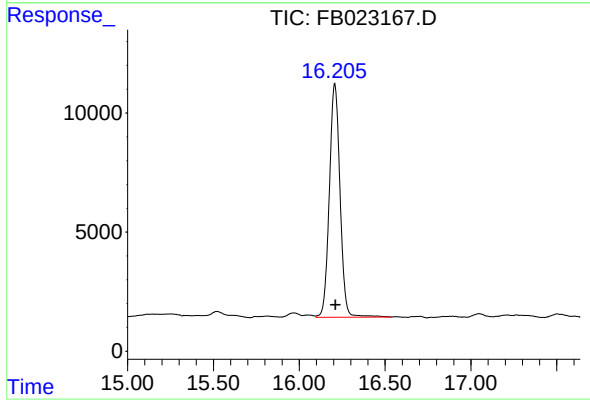

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.003 min
Response: 424485
Conc: 15.14 ng/ml