

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120919\
 Data File : FB023168.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2019 16:40
 Operator : DD/AJ
 Sample : K6111-02MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 10 00:49:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	482947	19.661 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	832685	25.481 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	957008	27.445 ng/ml
3) t n-Heptane	7.754	311373	9.056 ng/ml
4) t Benzene	7.889	384519	9.229 ng/ml
6) t Toluene	10.628	1132473	28.112 ng/ml
7) t Ethylbenzene	13.068	350738	9.089 ng/ml
8) t m-Xylene	13.201	662632	18.209 ng/ml
9) t O-Xylene	13.929	635233	18.295 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	529318	18.875 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120919\
Data File : FB023168.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2019 16:40
Operator : DD/AJ
Sample : K6111-02MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 10 00:49:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

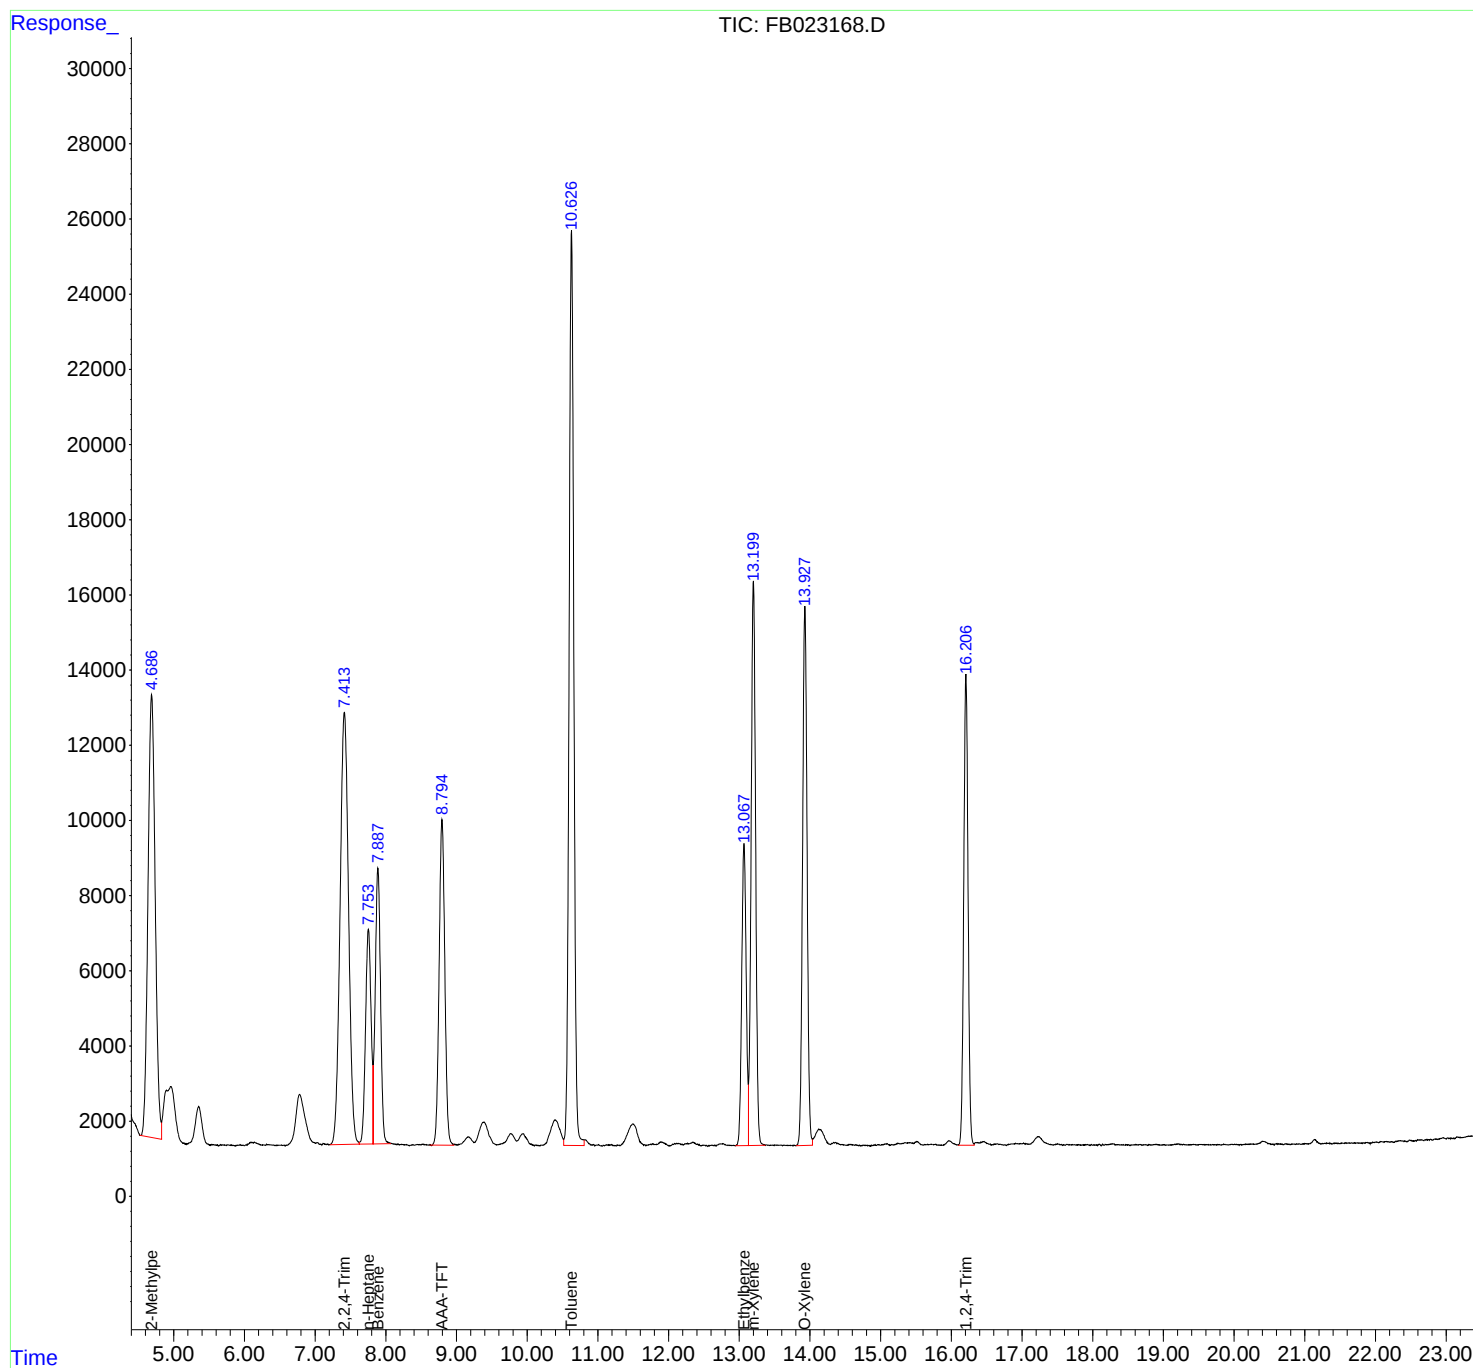


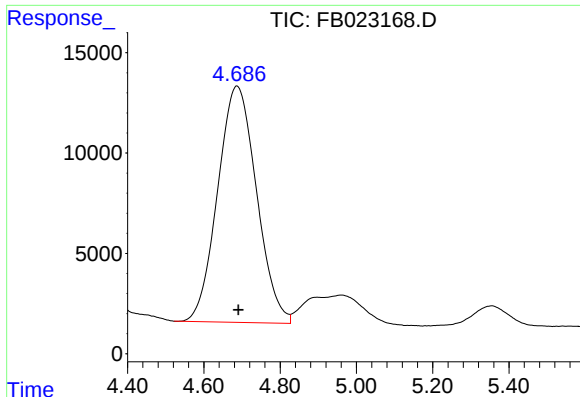

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.004 min
Response: 832685
Conc: 25.48 ng/ml

Instrument :
FID_B
ClientSampleId :

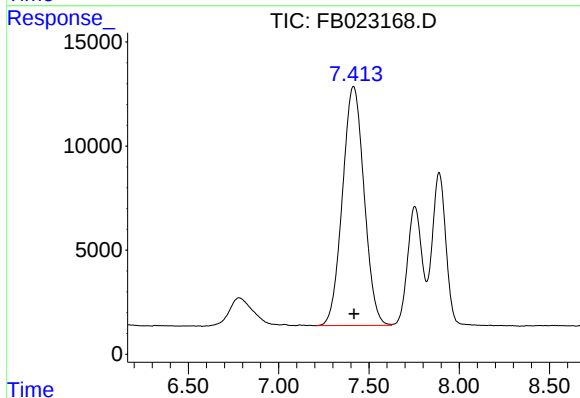


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 957008
Conc: 27.44 ng/ml

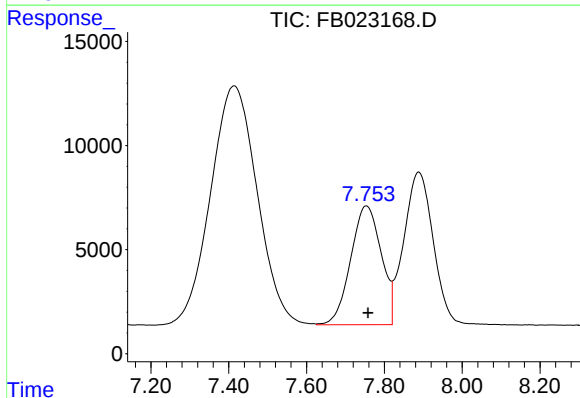


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 311373
Conc: 9.06 ng/ml

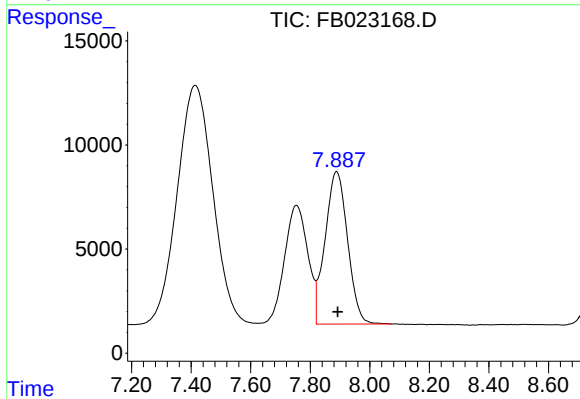

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 384519
Conc: 9.23 ng/ml

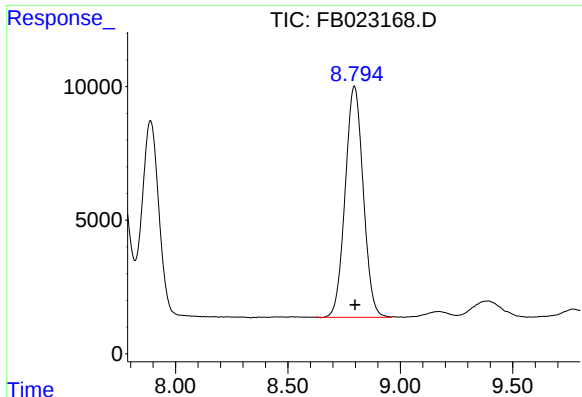

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 482947
Conc: 19.66 ng/ml

Instrument :
FID_B
ClientSampleId :

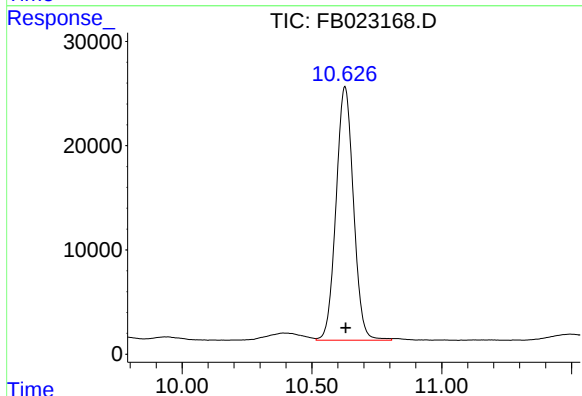


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 1132473
Conc: 28.11 ng/ml

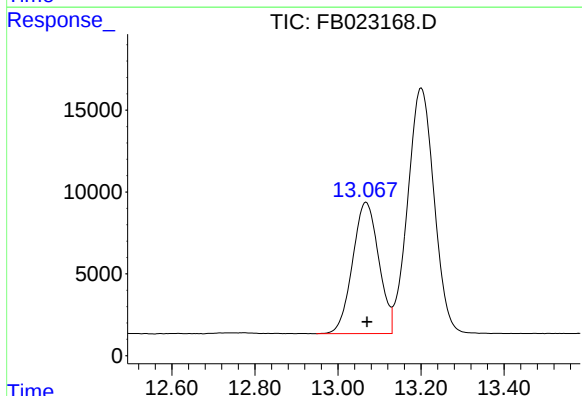


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 350738
Conc: 9.09 ng/ml

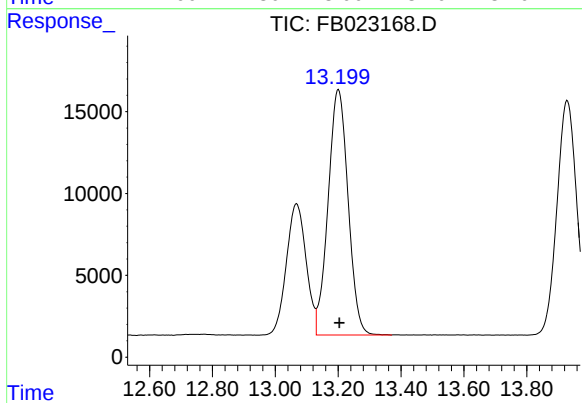

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.003 min
Response: 662632
Conc: 18.21 ng/ml

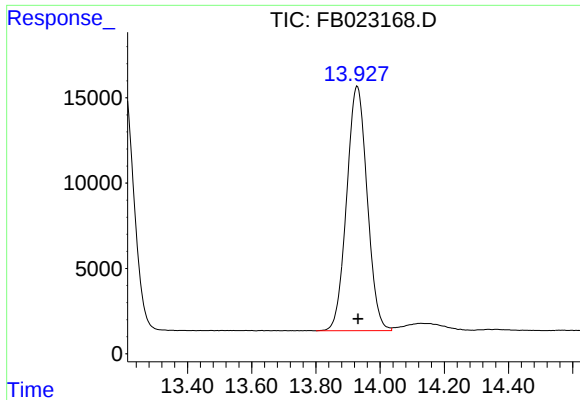

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.003 min
Response: 635233
Conc: 18.30 ng/ml

Instrument :
FID_B
ClientSampleId :

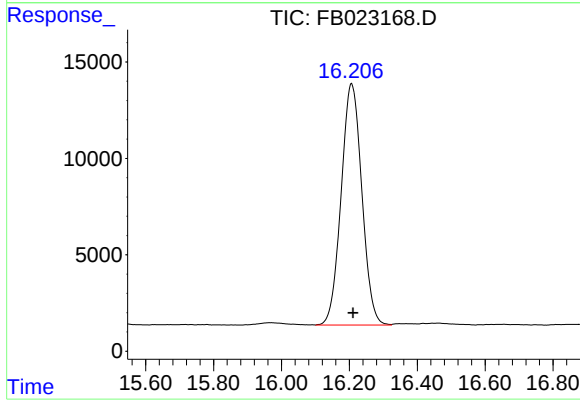

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.003 min
Response: 529318
Conc: 18.87 ng/ml