

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120920\
 Data File : FB025312.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2020 15:47
 Operator : DD/AJ
 Sample : L4880-04MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 KENS-B4-112320-0-2MS

Integration File: Calibration.e
 Quant Time: Dec 10 00:11:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	396014	18.837 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	775664	25.801 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	753597	25.045 ng/ml
3) t n-Heptane	7.759	242749	8.198 ng/ml
4) t Benzene	7.894	348600	9.425 ng/ml
6) t Toluene	10.632	966059	27.491 ng/ml
7) t Ethylbenzene	13.072	287076	8.789 ng/ml
8) t m-Xylene	13.205	574291	17.743 ng/ml
9) t O-Xylene	13.933	559299	17.692 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	451187	16.615 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120920\
Data File : FB025312.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2020 15:47
Operator : DD/AJ
Sample : L4880-04MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-B4-112320-0-2MS

Integration File: Calibration.e
Quant Time: Dec 10 00:11:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

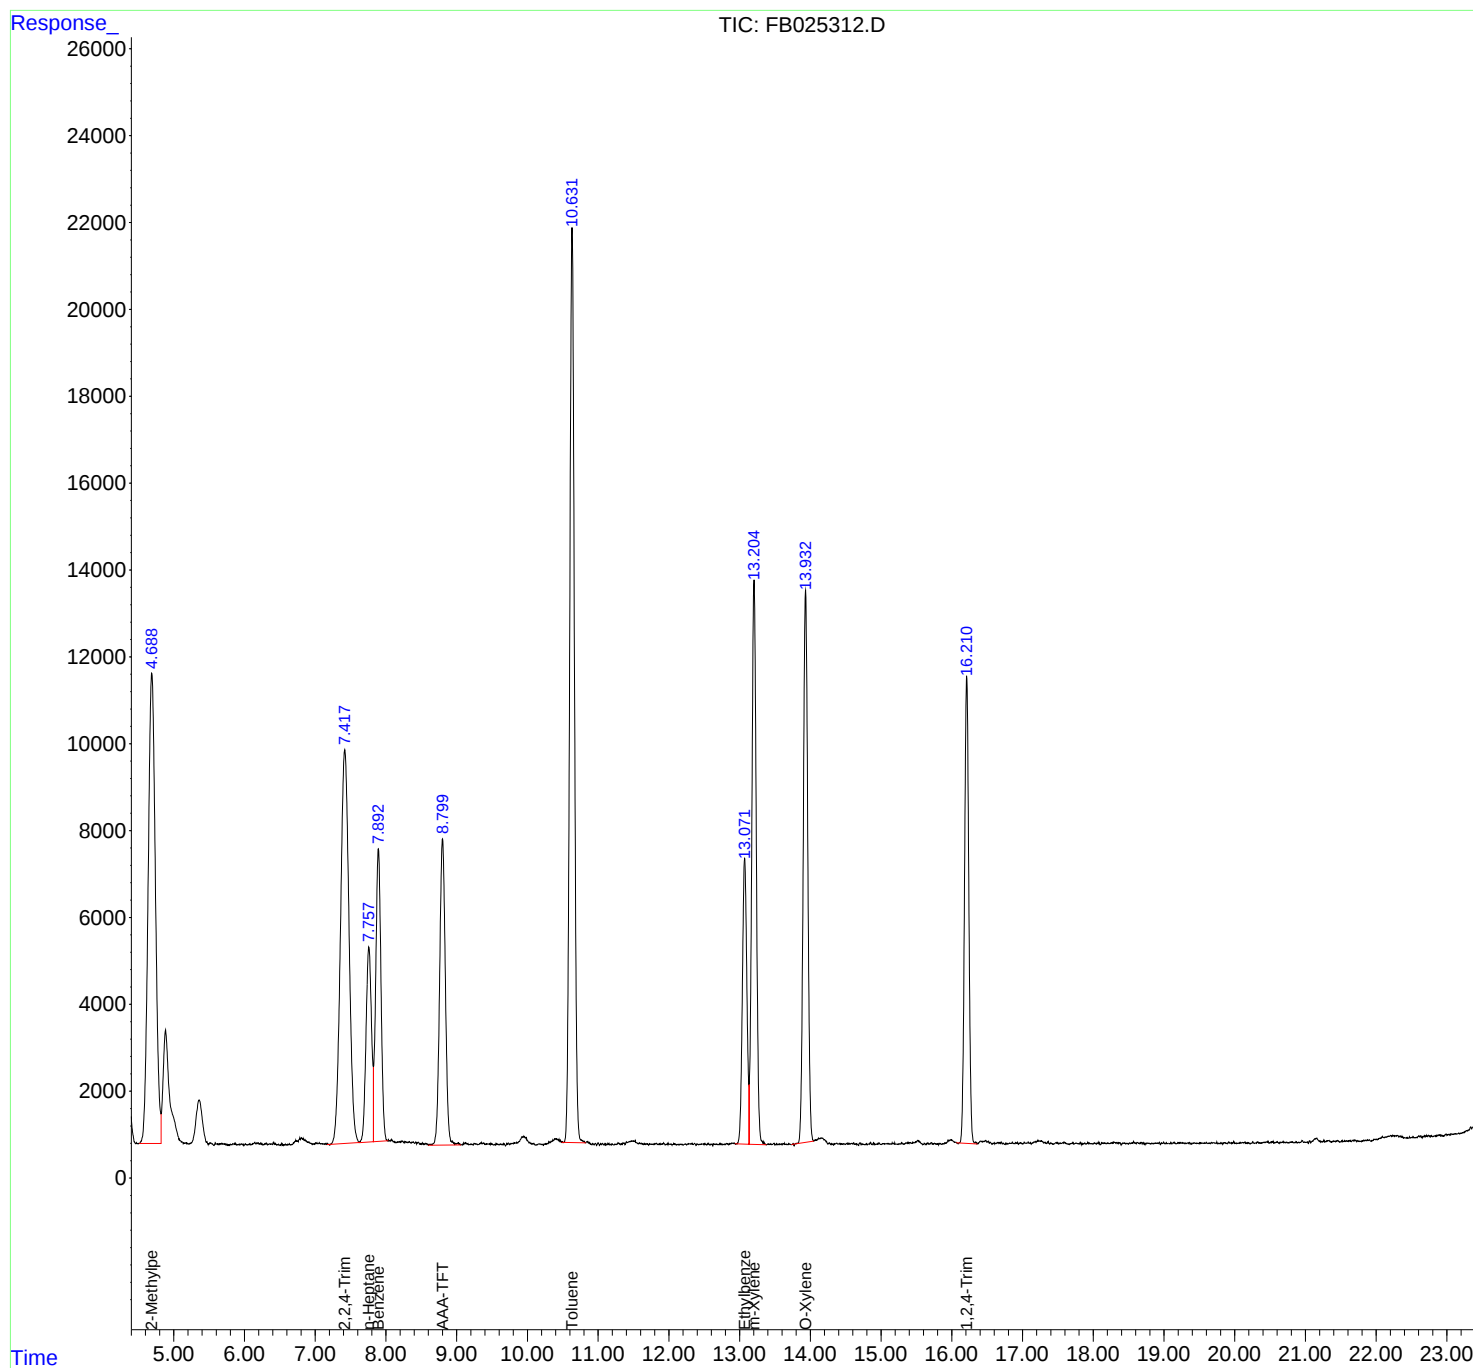


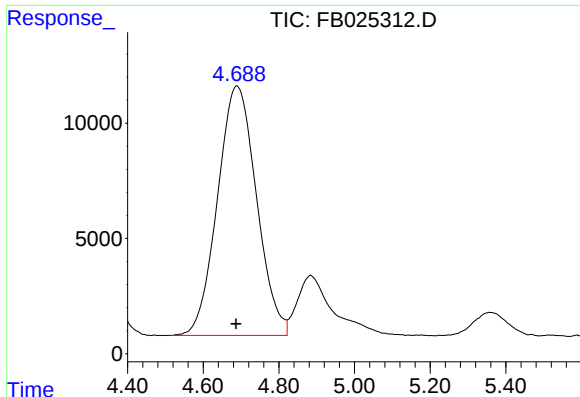

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.003 min
Response: 775664
Conc: 25.80 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B4-112320-0-2MS

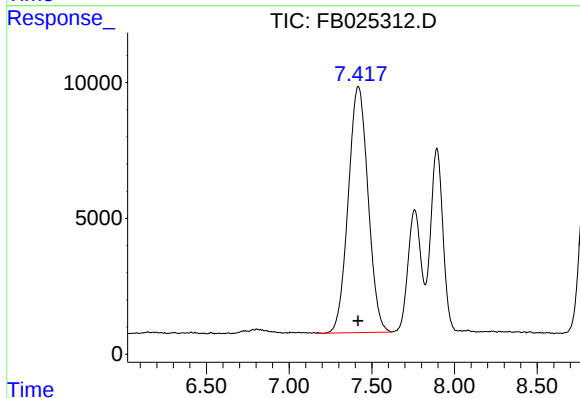


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.001 min
Response: 753597
Conc: 25.05 ng/ml

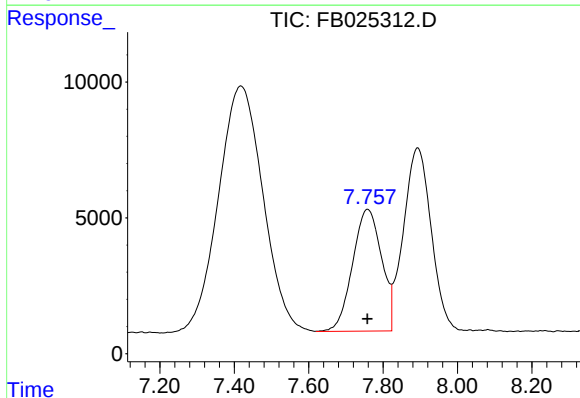


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.001 min
Response: 242749
Conc: 8.20 ng/ml

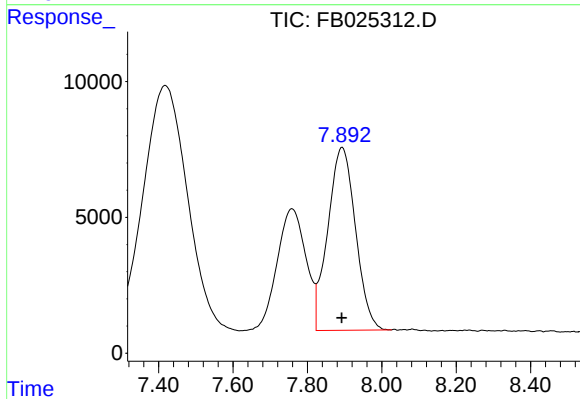

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.001 min
Response: 348600
Conc: 9.42 ng/ml

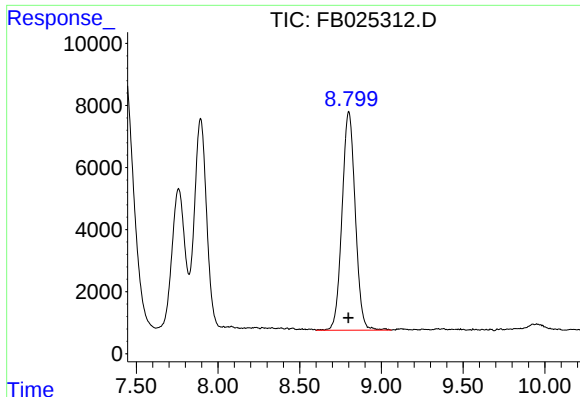

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.002 min
Response: 396014
Conc: 18.84 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B4-112320-0-2MS

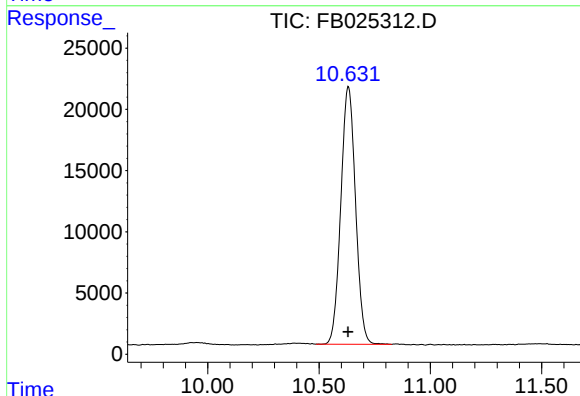


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.002 min
Response: 966059
Conc: 27.49 ng/ml

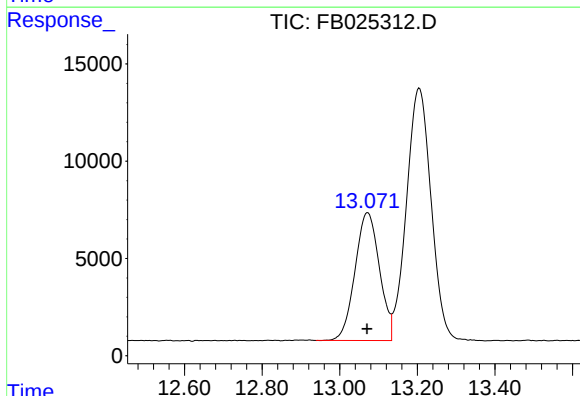


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.002 min
Response: 287076
Conc: 8.79 ng/ml

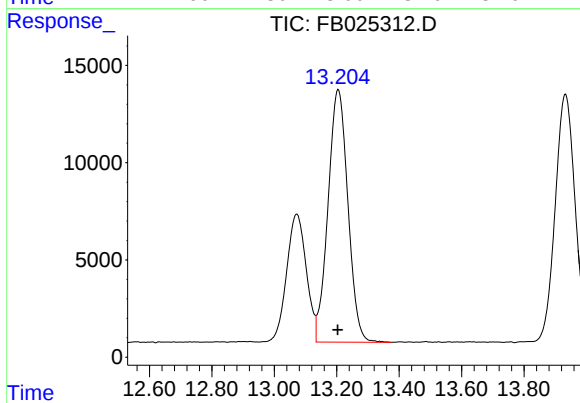

#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.002 min
Response: 574291
Conc: 17.74 ng/ml

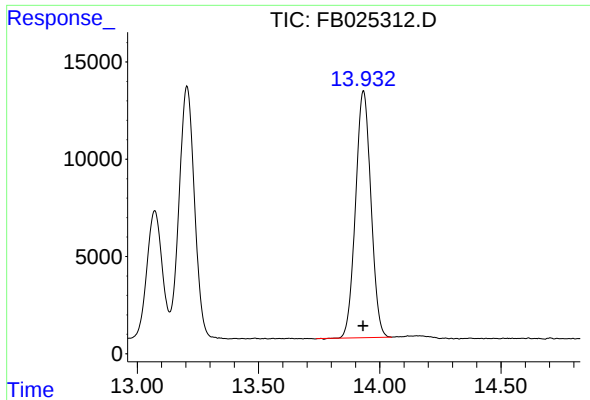

#9 O-Xylene


R.T.: 13.933 min

Delta R.T.: 0.002 min

Response: 559299

Conc: 17.69 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B4-112320-0-2MS

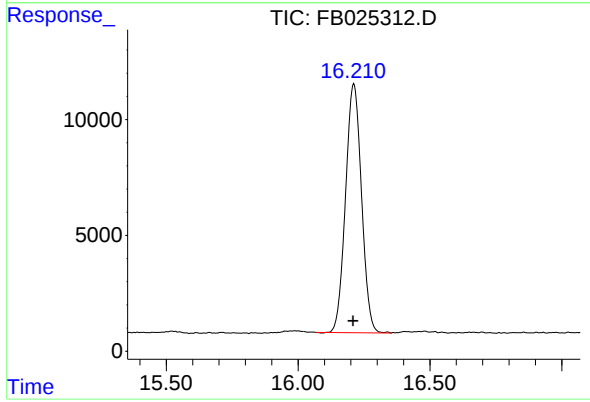

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min

Delta R.T.: 0.002 min

Response: 451187

Conc: 16.62 ng/ml